

Data Path : P:\HPCHEM1\ECD_0\Data\P0050118\
Data File : P0044298.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 May 2018 23:51
Operator : SM/UA
Sample : J2668-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A403577

Manual Integrations
APPROVED

UGO
5/2/2018 12:12:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 03:36:11 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.038	3.297	888424	958701	1.241	0.991
2) SA Decachlor...	9.379	8.057	987675	764176	1.603	0.921m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0050118\
Data File : P0044298.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 May 2018 23:51
Operator : SM/UA
Sample : J2668-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A403577


Manual Integrations
APPROVED

UGO
5/2/2018 12:12:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 03:36:11 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0042518.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 26 04:36:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

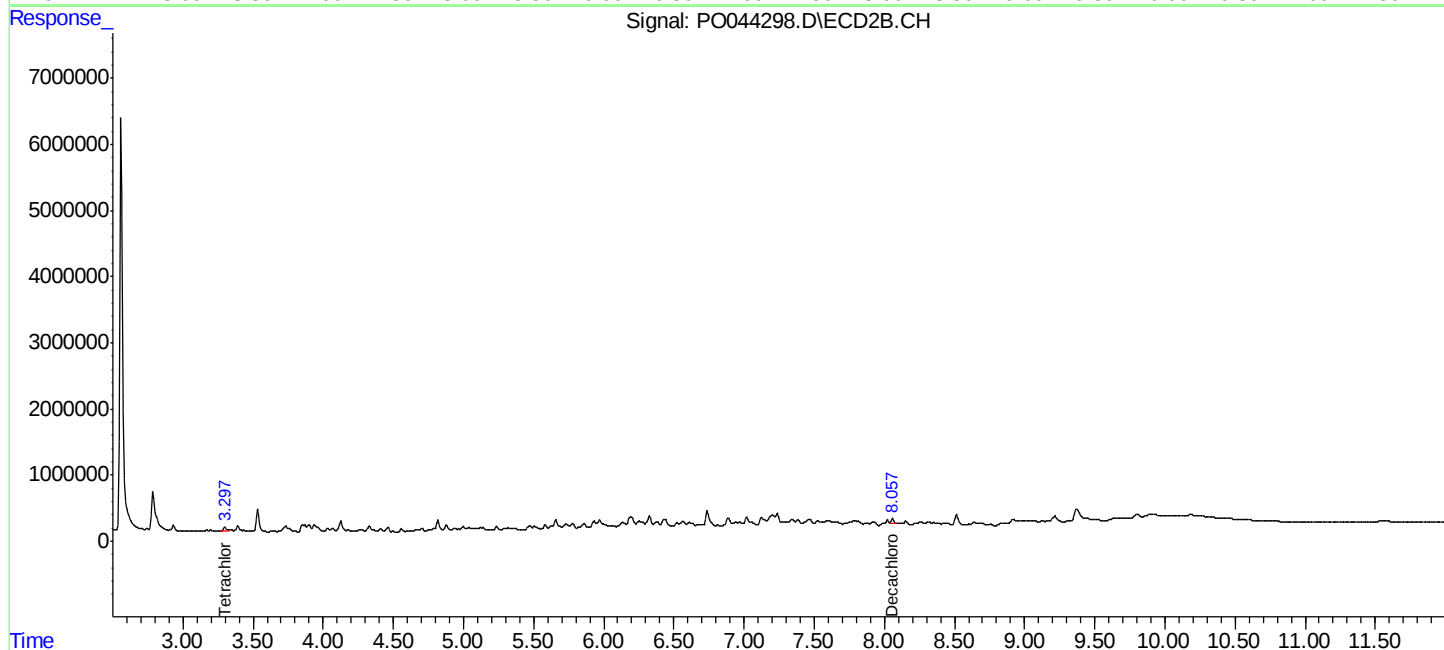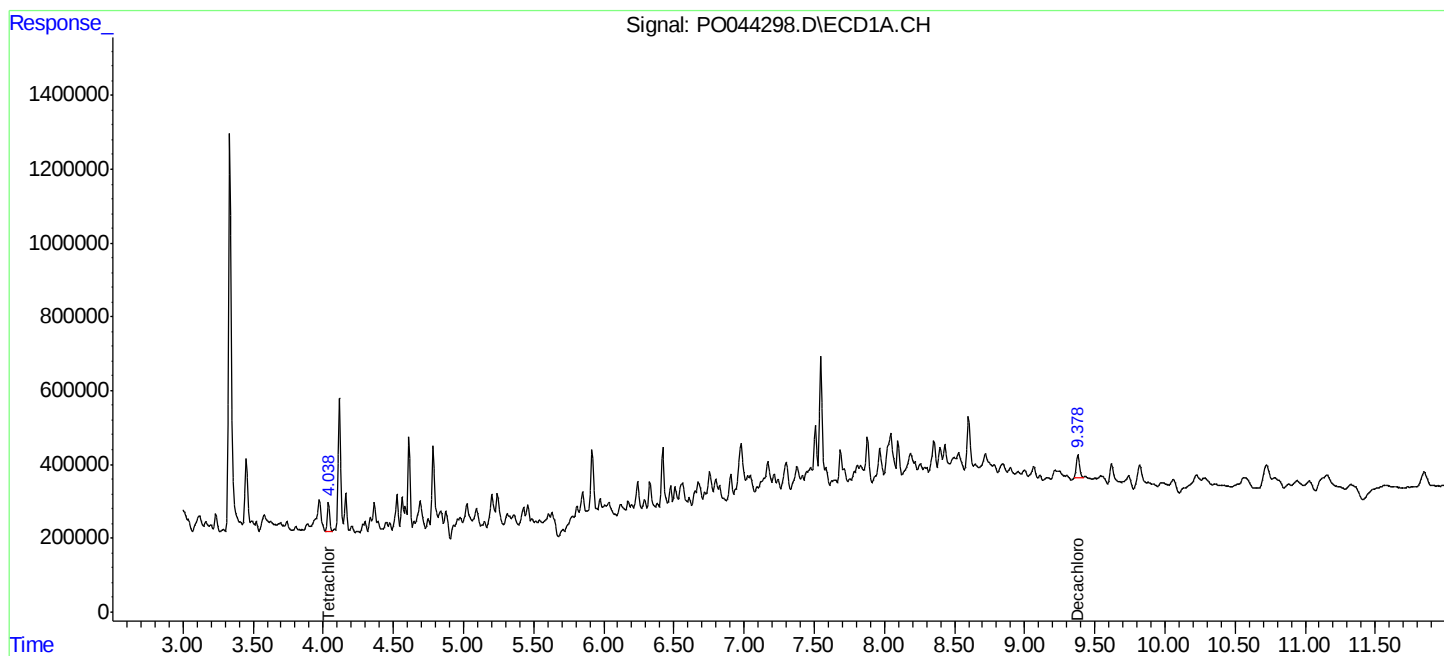

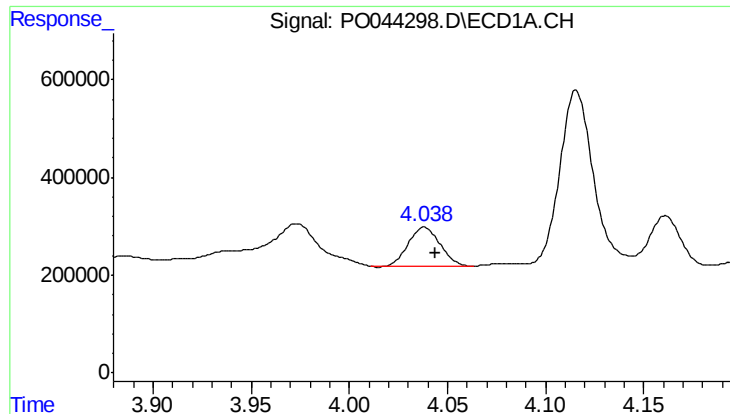


#1 Tetrachloro-m-xylene

R.T.: 4.038 min
Delta R.T.: -0.006 min
Response: 888424
Conc: 1.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
A403577


Manual Integrations
APPROVED

UGO
5/2/2018 12:12:10 PM

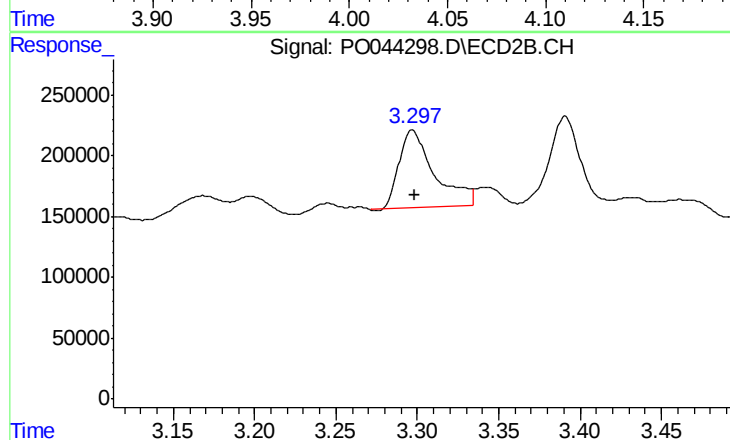


#1 Tetrachloro-m-xylene

R.T.: 3.297 min
Delta R.T.: -0.001 min
Response: 958701
Conc: 0.99 ng/ml

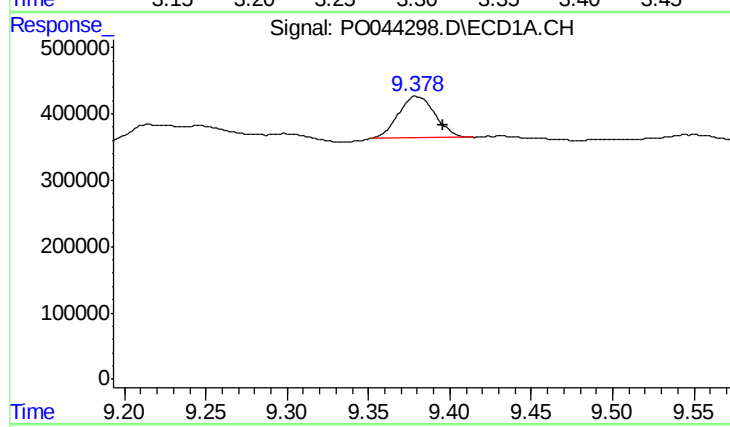

#2 Decachlorobiphenyl

R.T.: 9.379 min
Delta R.T.: -0.017 min
Response: 987675
Conc: 1.60 ng/ml

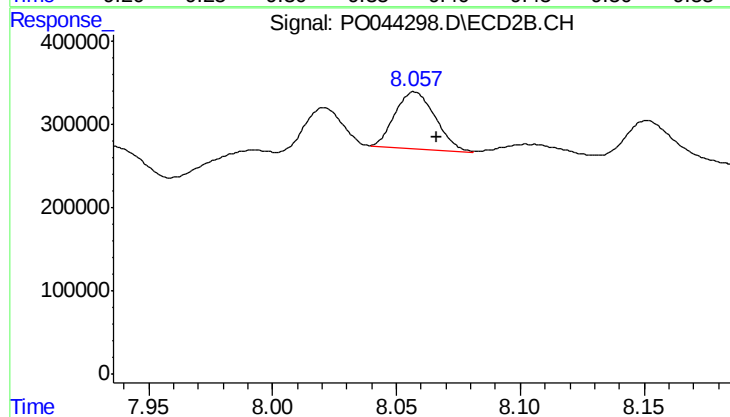

#2 Decachlorobiphenyl

R.T.: 8.057 min
Delta R.T.: -0.010 min
Response: 764176
Conc: 0.92 ng/ml m