

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050119\
 Data File : P0055749.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 May 2019 19:41
 Operator : SM/SJ
 Sample : K2624-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-BLOCK-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 04:17:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 30 05:21:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.281	3.595	714612	754921	25.407	25.878
2) SA Decachlor...	9.880	8.546	711323	484085	16.655	15.238

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050119\
Data File : PO055749.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 May 2019 19:41
Operator : SM/SJ
Sample : K2624-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-BLOCK-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 04:17:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042919.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 30 05:21:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

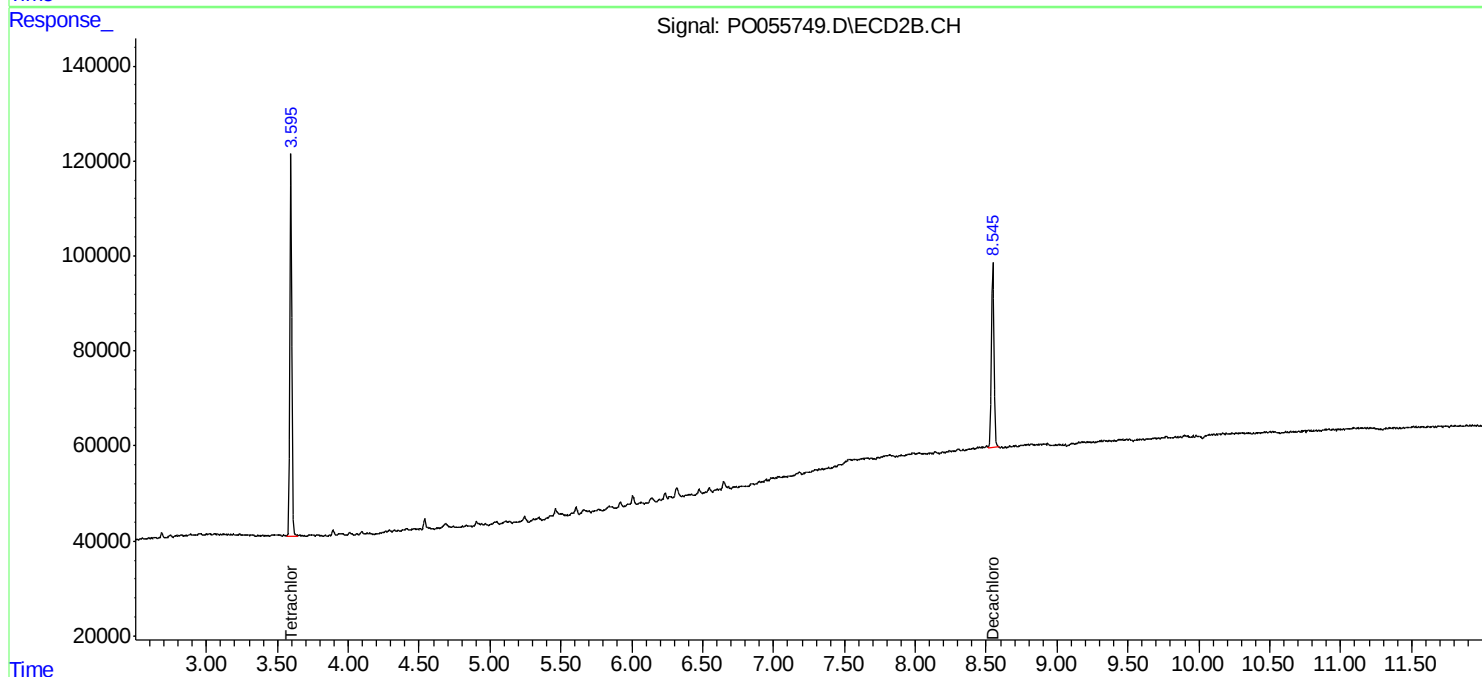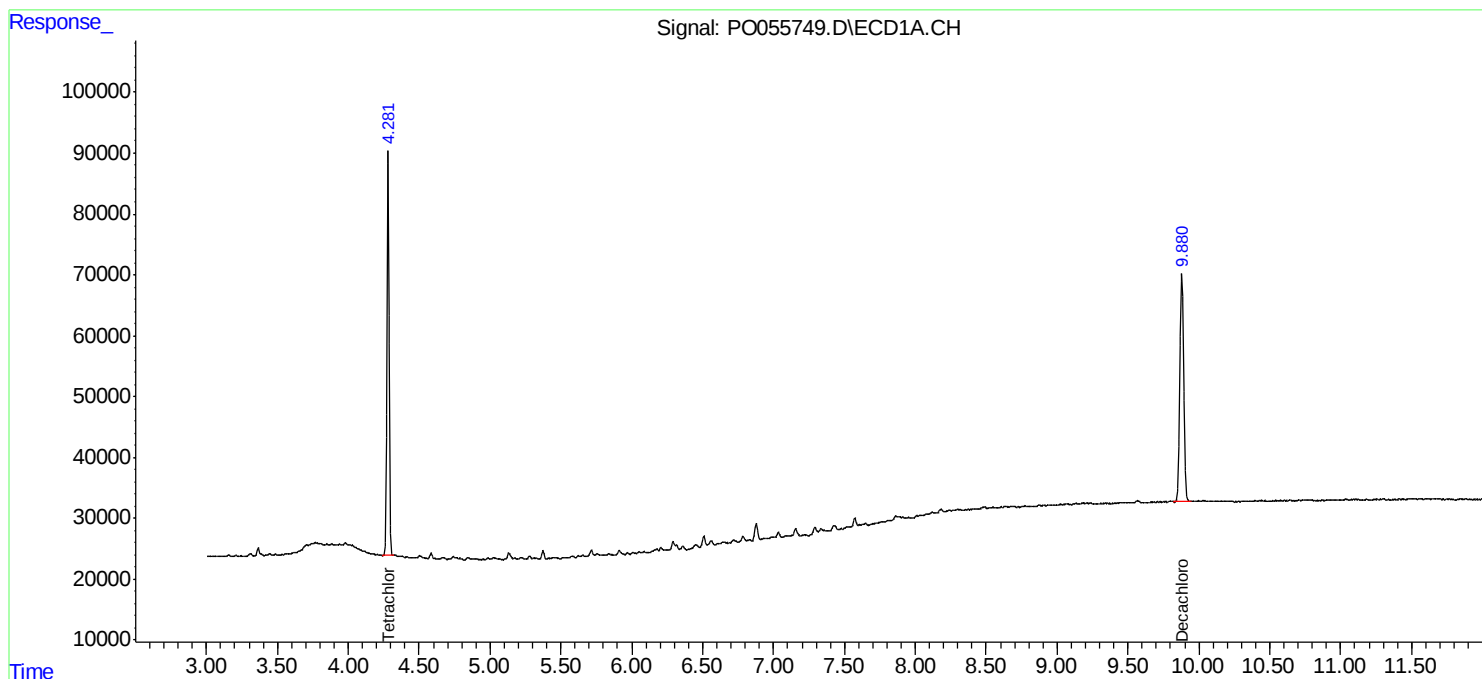


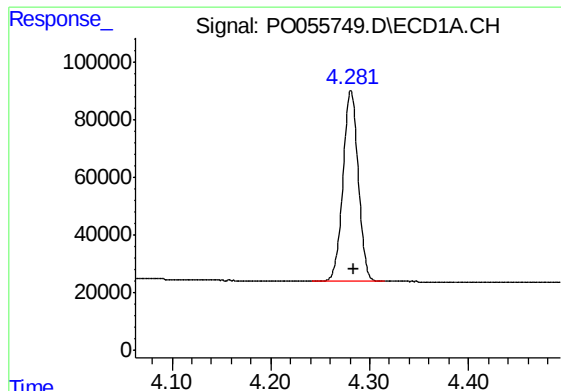

#1 Tetrachloro-m-xylene


R.T.: 4.281 min
Delta R.T.: -0.003 min
Response: 714612
Conc: 25.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-BLOCK-B

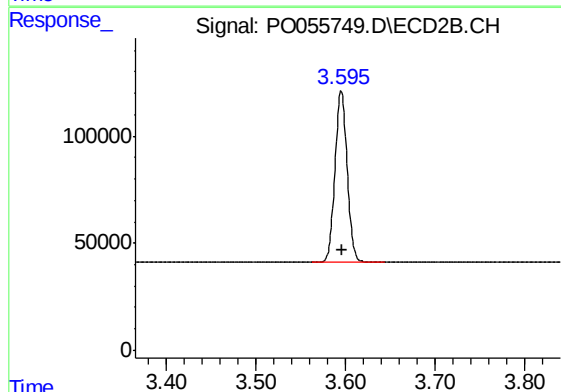


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 754921
Conc: 25.88 ng/ml

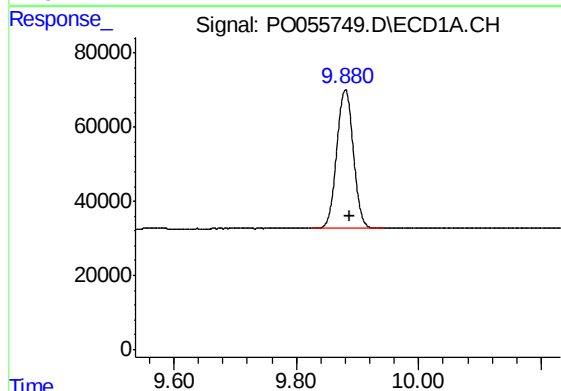

#2 Decachlorobiphenyl

R.T.: 9.880 min
Delta R.T.: -0.006 min
Response: 711323
Conc: 16.65 ng/ml

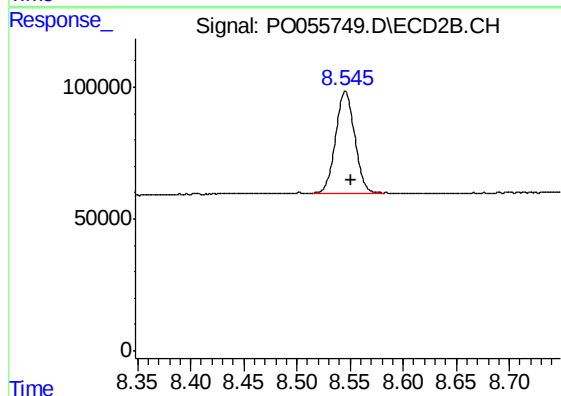

#2 Decachlorobiphenyl

R.T.: 8.546 min
Delta R.T.: -0.005 min
Response: 484085
Conc: 15.24 ng/ml