

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050219\
 Data File : P0055776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 May 2019 11:55
 Operator : SM/SJ
 Sample : K2597-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OB-722

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 03:45:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 30 05:21:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.592	524243	764290	18.639	26.200 #
2) SA Decachlor...	9.879	8.544	539828	373565	12.639	11.759

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050219\
Data File : PO055776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 May 2019 11:55
Operator : SM/SJ
Sample : K2597-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OB-722

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 03:45:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042919.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 30 05:21:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

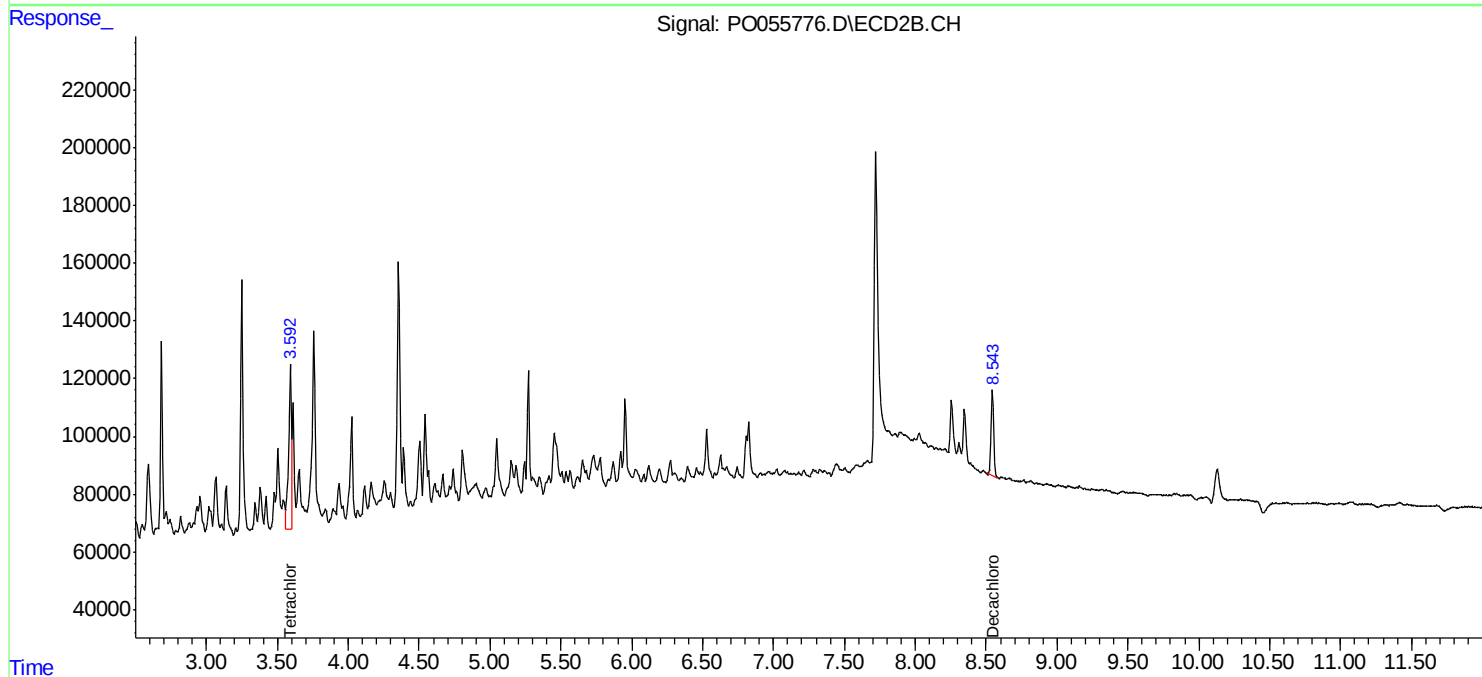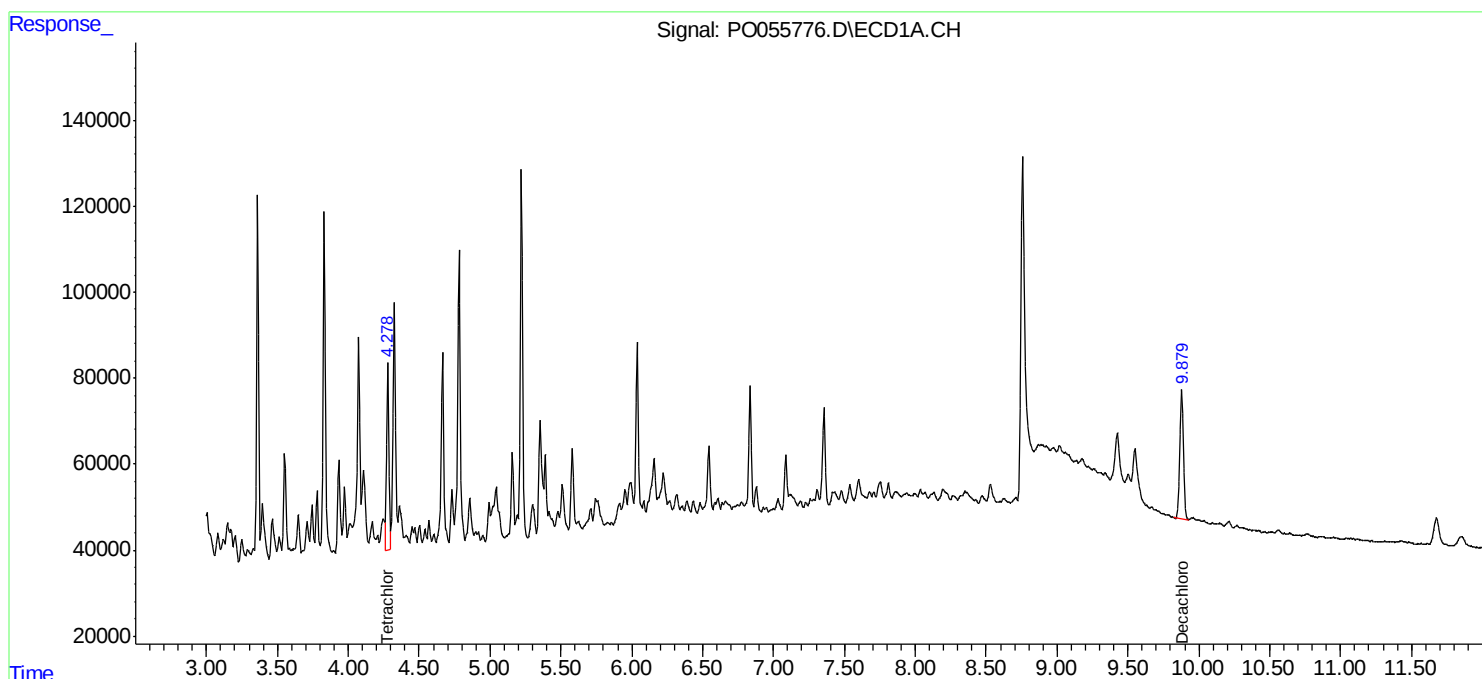


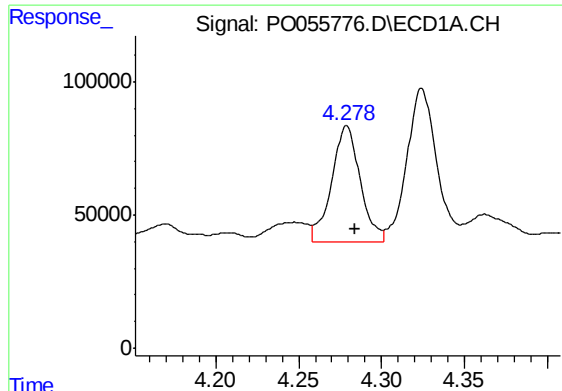

#1 Tetrachloro-m-xylene


R.T.: 4.279 min
Delta R.T.: -0.005 min
Response: 524243
Conc: 18.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
OB-722

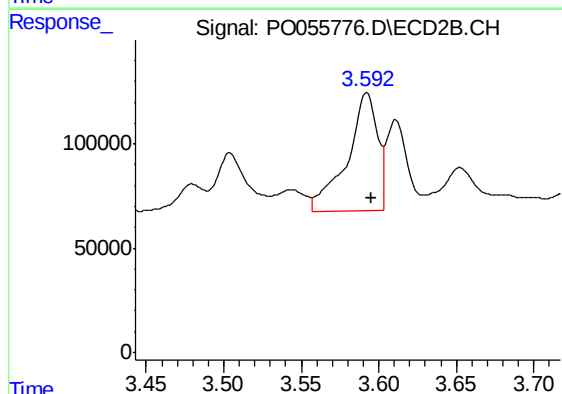


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: -0.004 min
Response: 764290
Conc: 26.20 ng/ml

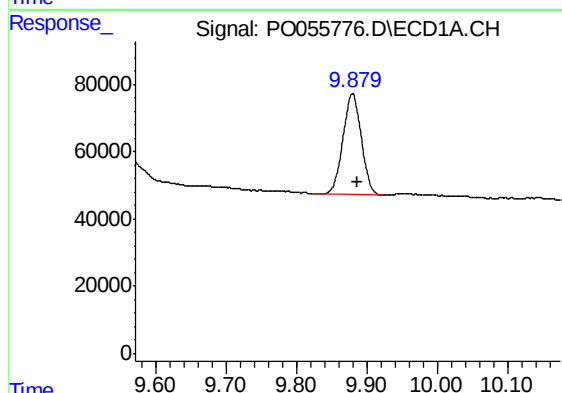

#2 Decachlorobiphenyl

R.T.: 9.879 min
Delta R.T.: -0.007 min
Response: 539828
Conc: 12.64 ng/ml

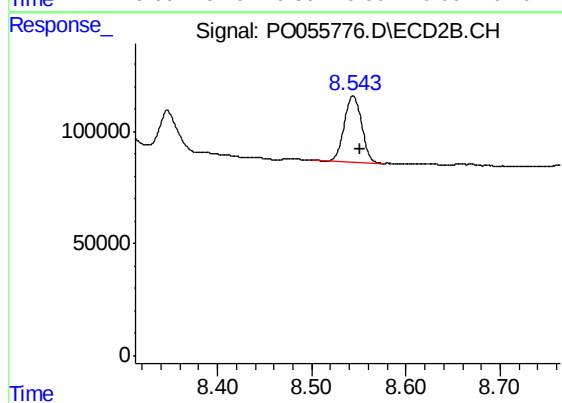

#2 Decachlorobiphenyl

R.T.: 8.544 min
Delta R.T.: -0.007 min
Response: 373565
Conc: 11.76 ng/ml