

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050219\
 Data File : P0055788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 May 2019 15:26
 Operator : SM/SJ
 Sample : K2626-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RI2-4(0-6)

Manual Integrations
 APPROVED

Ankita
 5/3/2019 3:25:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 03:50:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 30 05:21:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.280	3.594	712662	812143	25.338	27.840
2)	SA Decachlor...	9.880	8.546	428450	357937	10.032m	11.267m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050219\
Data File : PO055788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 May 2019 15:26
Operator : SM/SJ
Sample : K2626-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RI2-4(0-6)


Manual Integrations
APPROVED

Ankita
5/3/2019 3:25:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 03:50:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042919.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 30 05:21:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

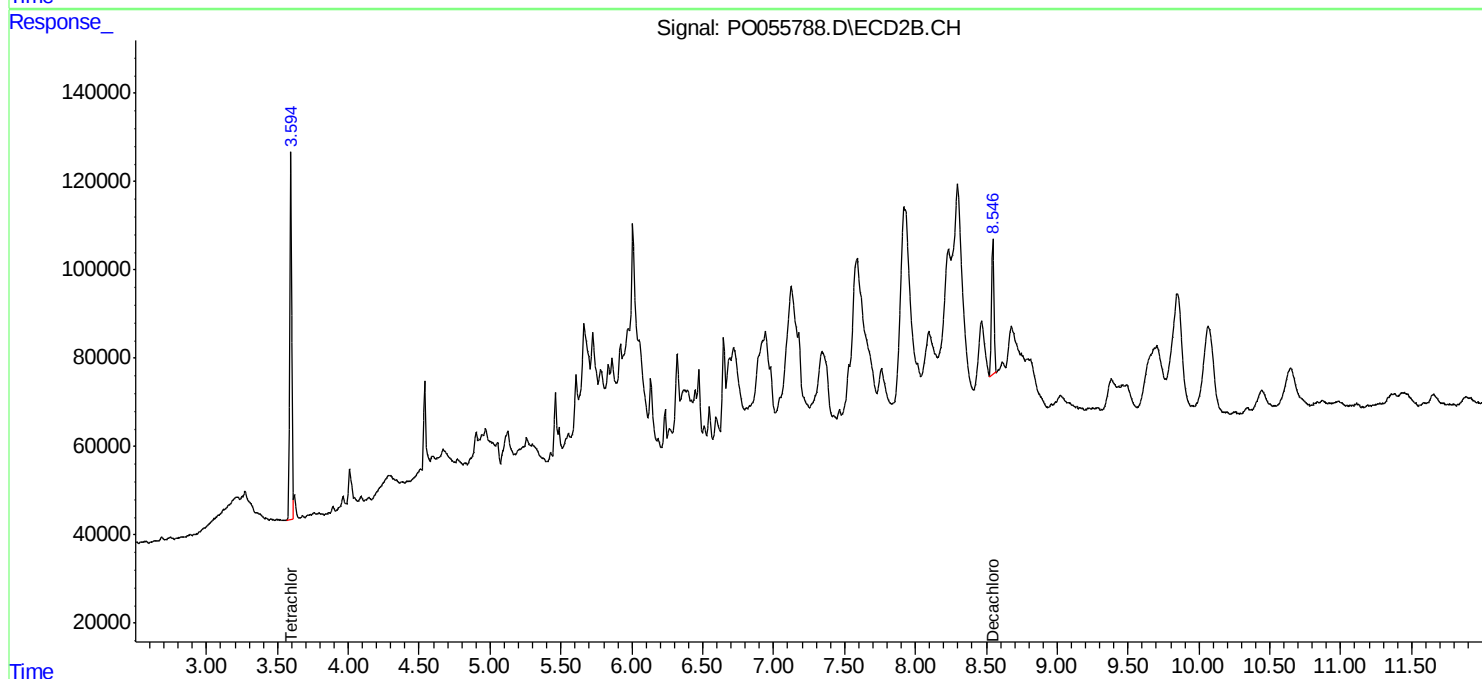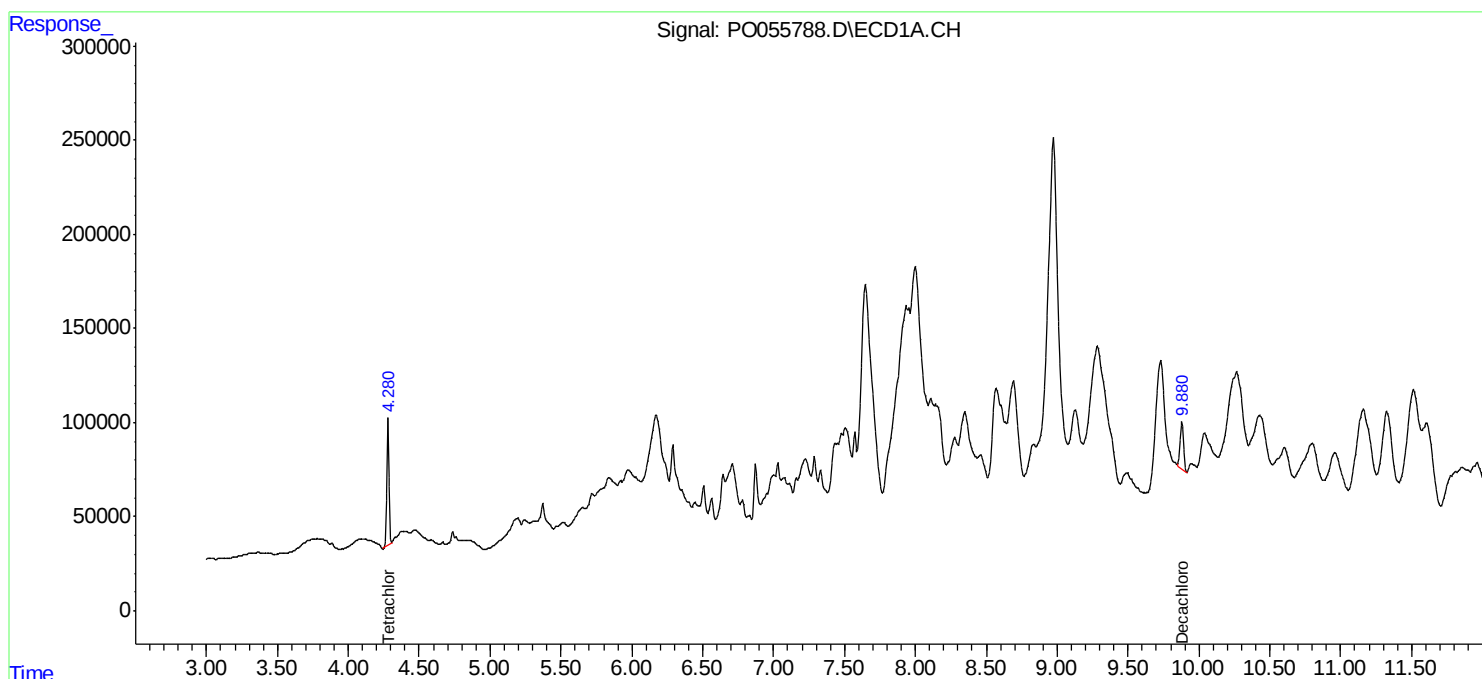

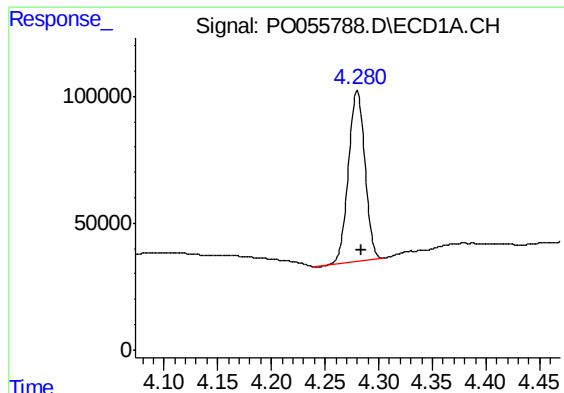


#1 Tetrachloro-m-xylene

R.T.: 4.280 min
Delta R.T.: -0.004 min
Response: 712662
Conc: 25.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
RI2-4(0-6)


Manual Integrations
APPROVED

Ankita
5/3/2019 3:25:54 PM

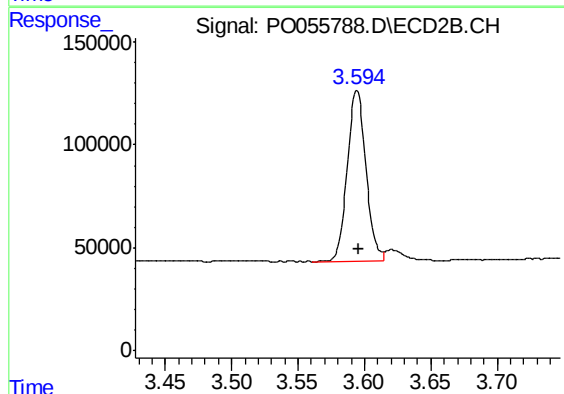


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: -0.001 min
Response: 812143
Conc: 27.84 ng/ml

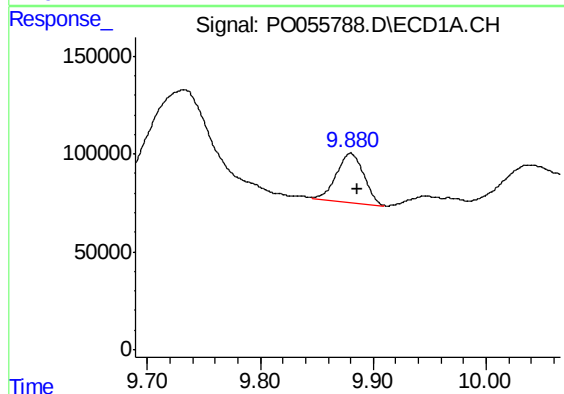

#2 Decachlorobiphenyl

R.T.: 9.880 min
Delta R.T.: -0.007 min
Response: 428450
Conc: 10.03 ng/ml m

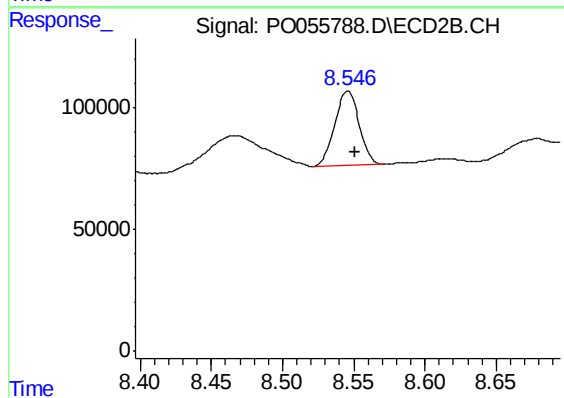

#2 Decachlorobiphenyl

R.T.: 8.546 min
Delta R.T.: -0.005 min
Response: 357937
Conc: 11.27 ng/ml m