

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050420\
 Data File : P0068144.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2020 12:21
 Operator : DD\AJ
 Sample : L2456-01 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 207

Manual Integrations
 APPROVED

Sohil
 5/6/2020 12:18:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 13:25:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.936	116152	148890	4.854m	4.659
2) SA Decachlor...	10.886	9.221	124925	137837	3.310m	3.571

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050420\
Data File : P0068144.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2020 12:21
Operator : DD\AJ
Sample : L2456-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
207


Manual Integrations
APPROVED

Sohil
5/6/2020 12:18:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 13:25:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

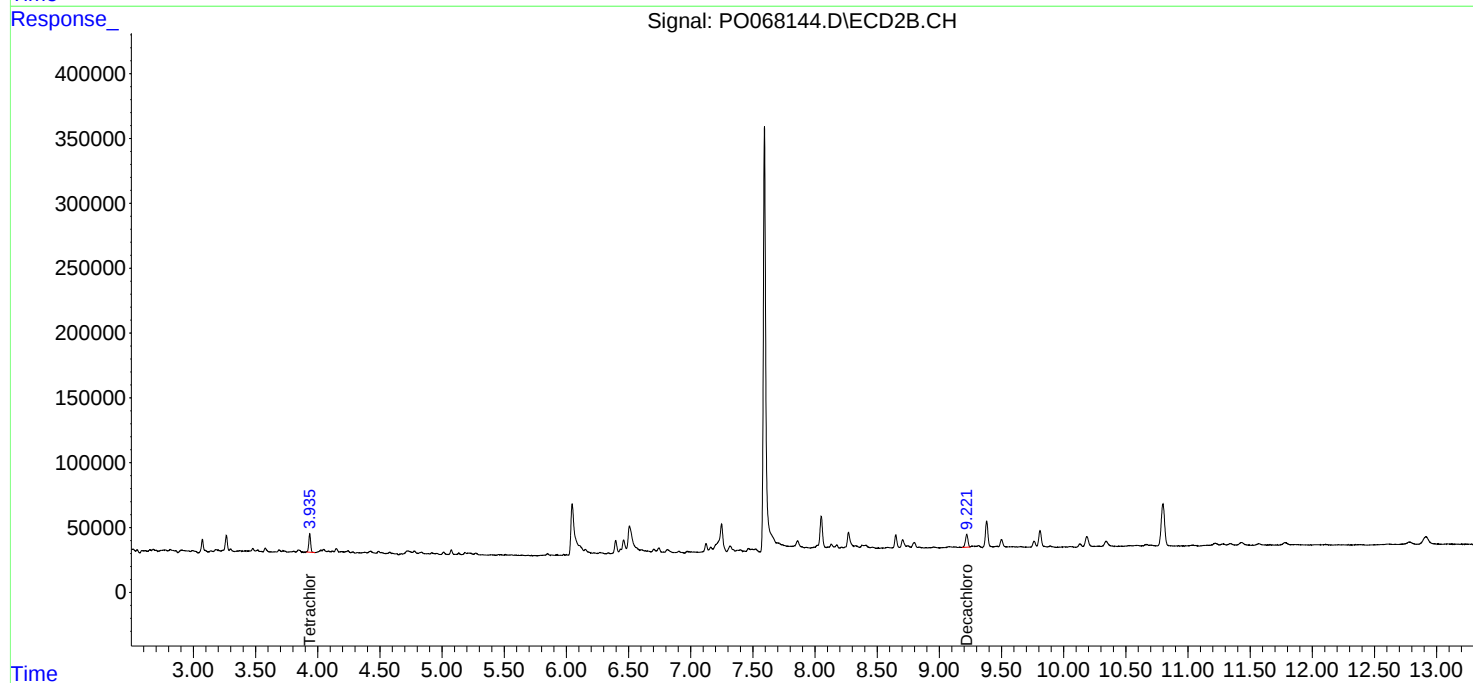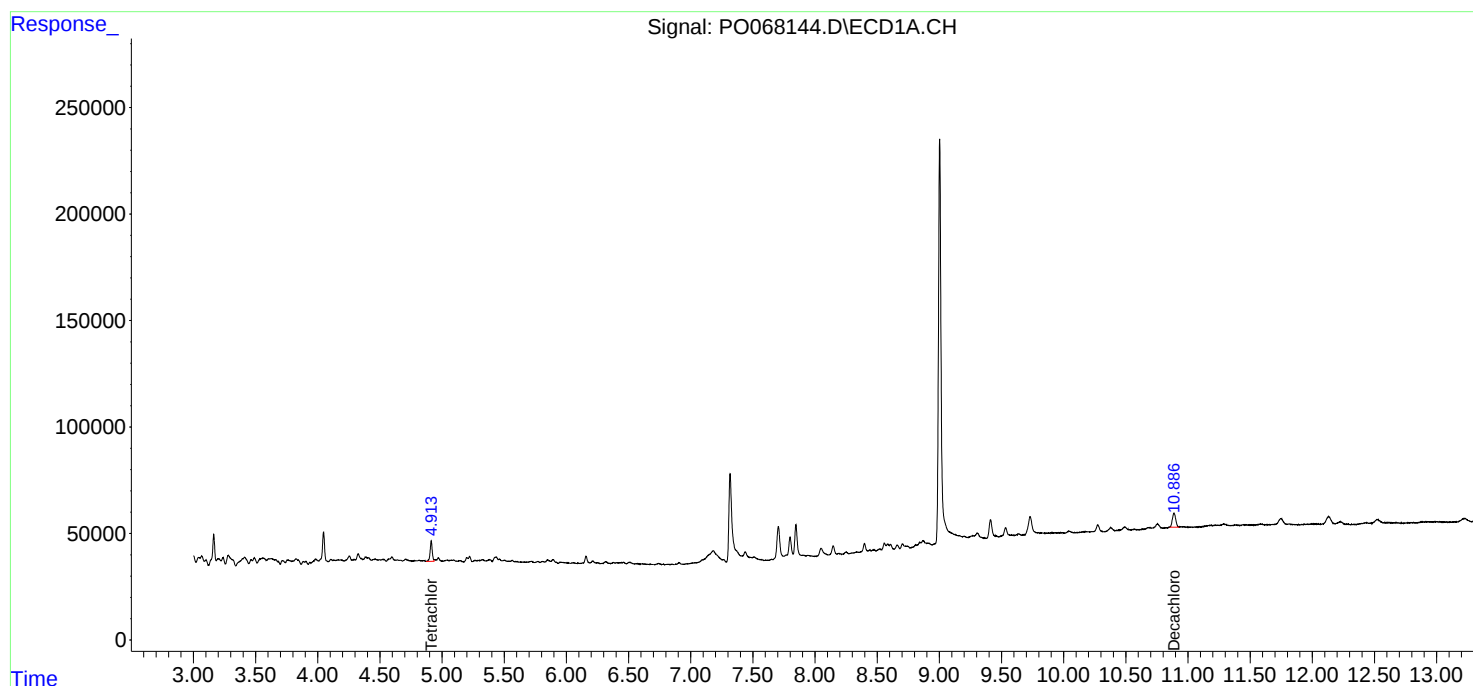

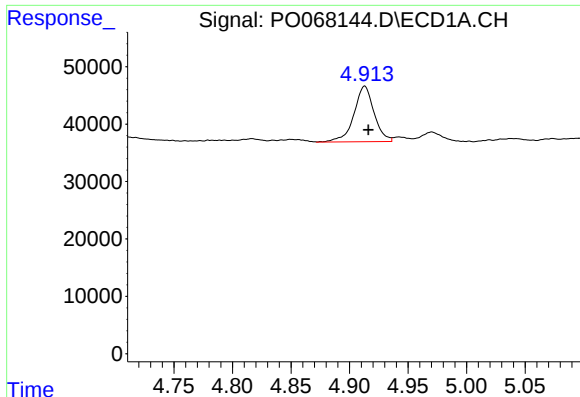


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: -0.003 min
Response: 116152
Conc: 4.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
207


Manual Integrations
APPROVED

Sohil
5/6/2020 12:18:11 PM

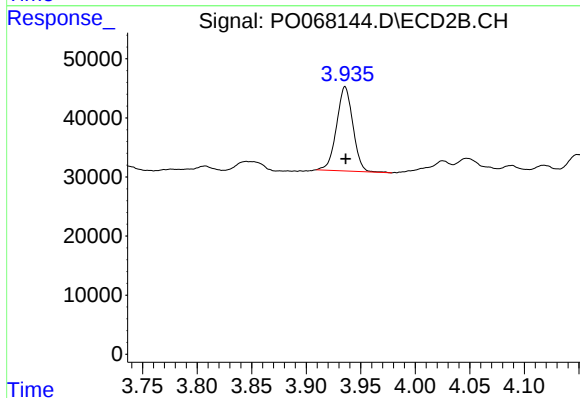


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 148890
Conc: 4.66 ng/ml

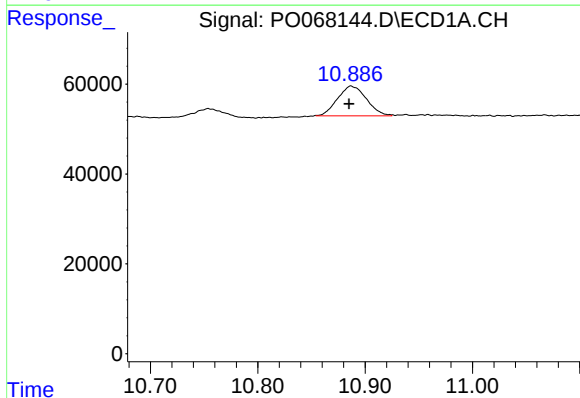

#2 Decachlorobiphenyl

R.T.: 10.886 min
Delta R.T.: 0.001 min
Response: 124925
Conc: 3.31 ng/ml m

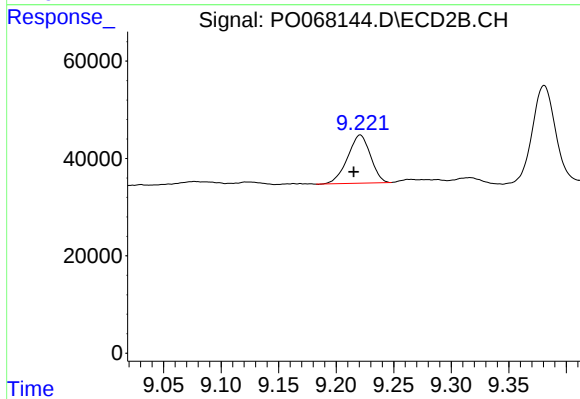

#2 Decachlorobiphenyl

R.T.: 9.221 min
Delta R.T.: 0.006 min
Response: 137837
Conc: 3.57 ng/ml