

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050420\
 Data File : P0068151.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2020 15:21
 Operator : DD\AJ
 Sample : L2464-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRE-50028

Manual Integrations
 APPROVED

Sohil
 5/6/2020 12:18:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 15:36:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.913	3.935	406717	566863	16.996	17.739m
2) SA Decachlor...	10.878	9.211	514437	528364	13.632m	13.690

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050420\
Data File : P0068151.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2020 15:21
Operator : DD\AJ
Sample : L2464-05
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRE-50028


Manual Integrations
APPROVED

Sohil
5/6/2020 12:18:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 15:36:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

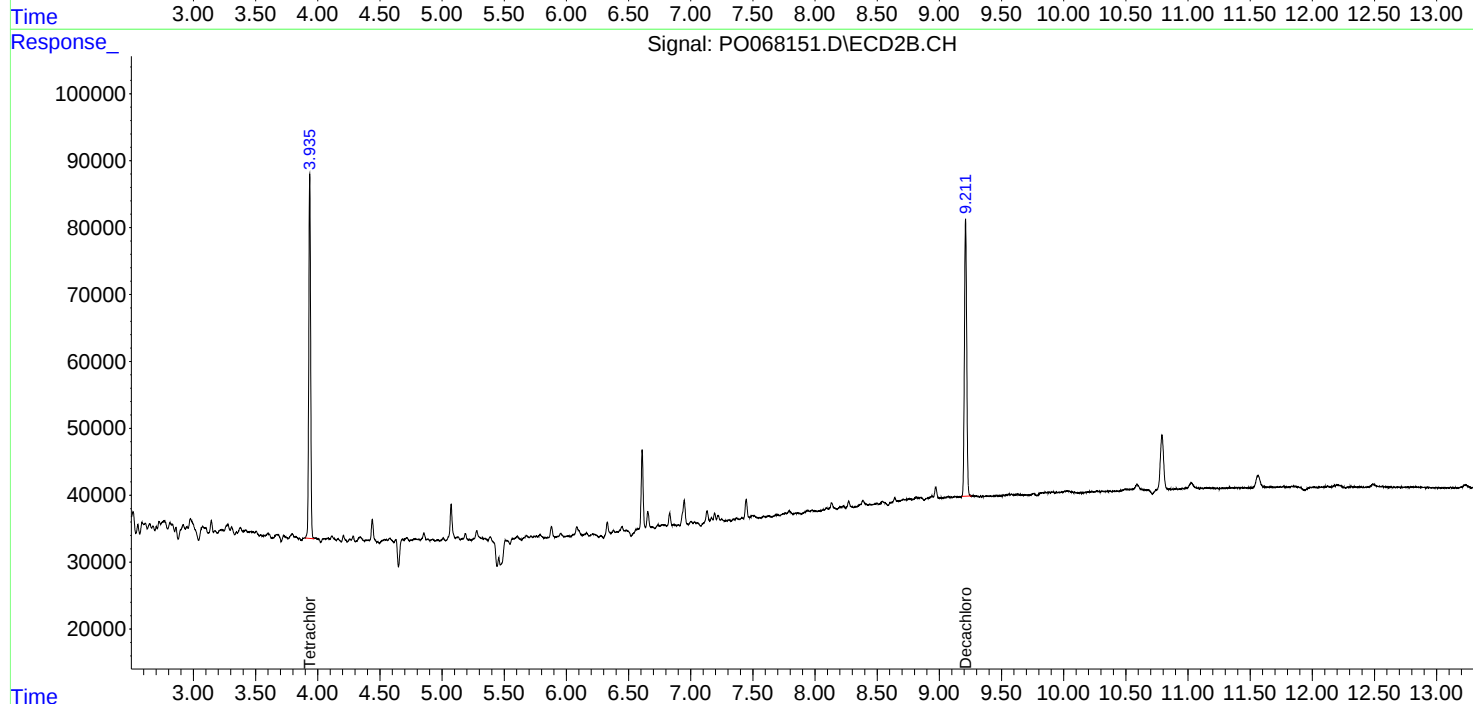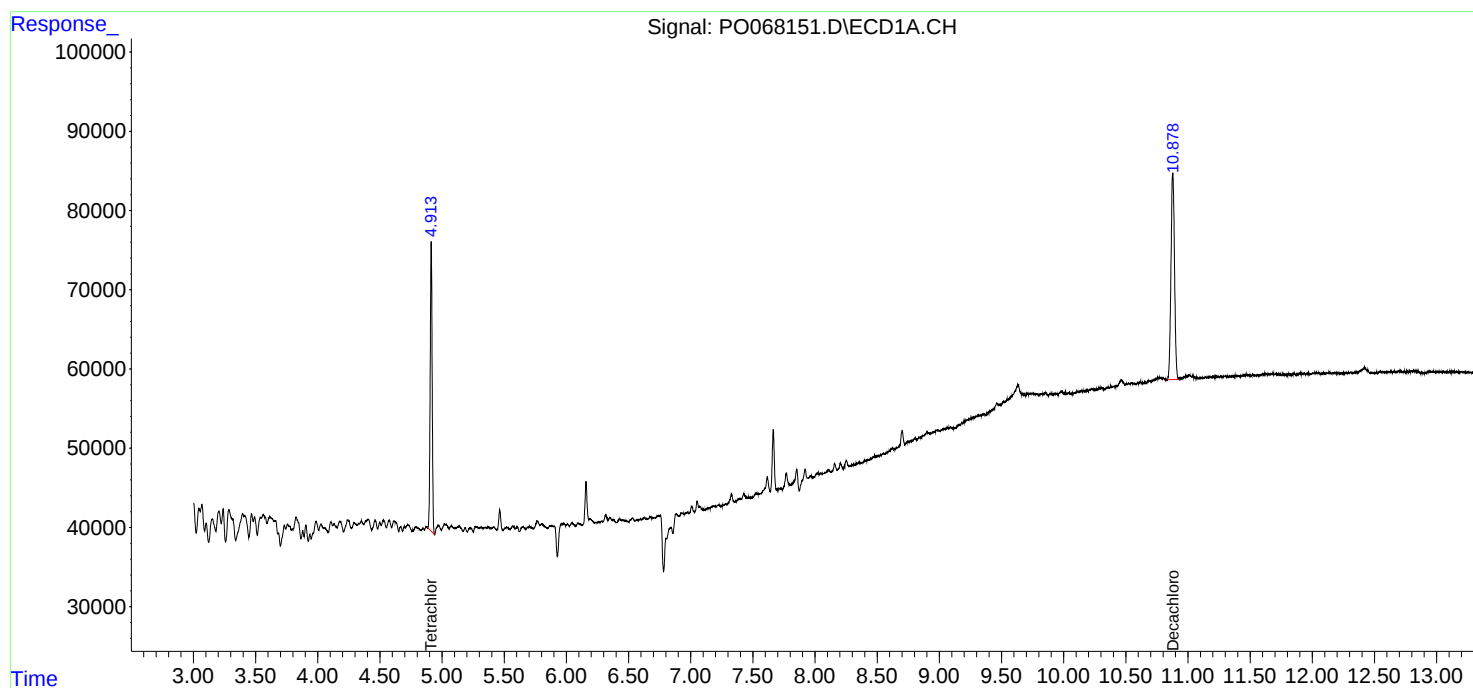

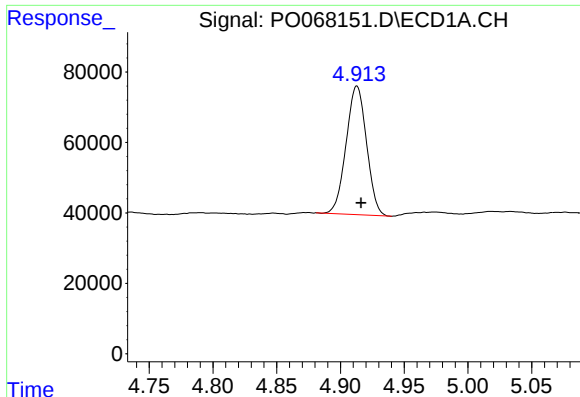


#1 Tetrachloro-m-xylene

R.T.: 4.913 min
Delta R.T.: -0.003 min
Response: 406717
Conc: 17.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-50028


Manual Integrations
APPROVED

Sohil
5/6/2020 12:18:17 PM

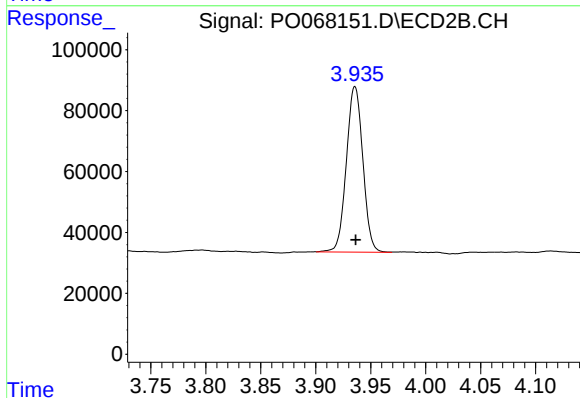


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 566863
Conc: 17.74 ng/ml m

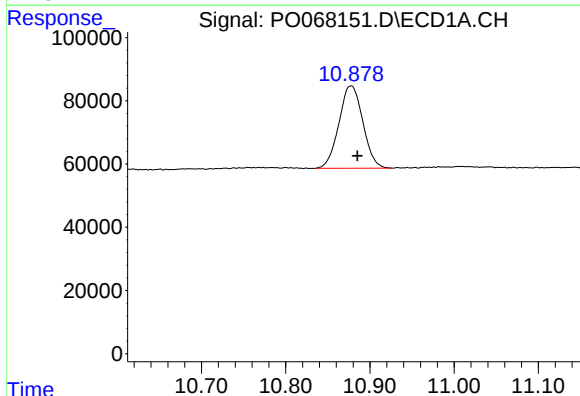

#2 Decachlorobiphenyl

R.T.: 10.878 min
Delta R.T.: -0.007 min
Response: 514437
Conc: 13.63 ng/ml m

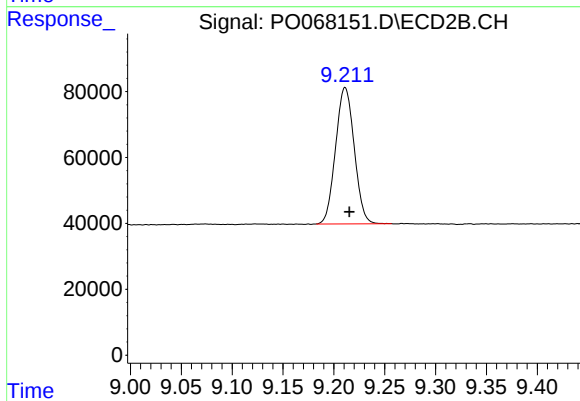

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.004 min
Response: 528364
Conc: 13.69 ng/ml