

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050420\
 Data File : P0068155.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2020 16:30
 Operator : DD\AJ
 Sample : L2477-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-0D015-03-012

Manual Integrations
 APPROVED

Sohil
 5/6/2020 12:18:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 16:53:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.911	3.933	409318	555057	17.105	17.370
2) SA Decachlor...	10.876	9.210	658683	693693	17.454m	17.974m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050420\
Data File : P0068155.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2020 16:30
Operator : DD\AJ
Sample : L2477-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-012


Manual Integrations
APPROVED

Sohil
5/6/2020 12:18:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 16:53:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

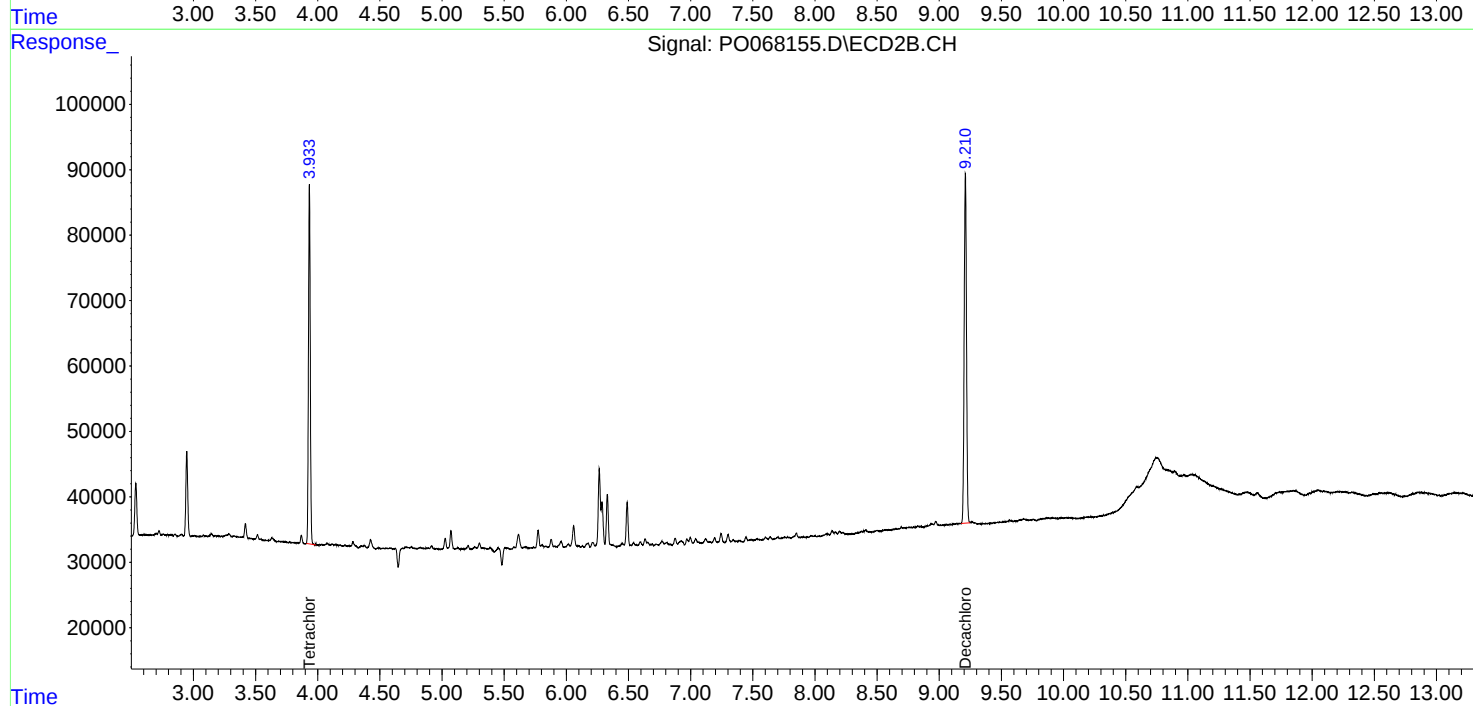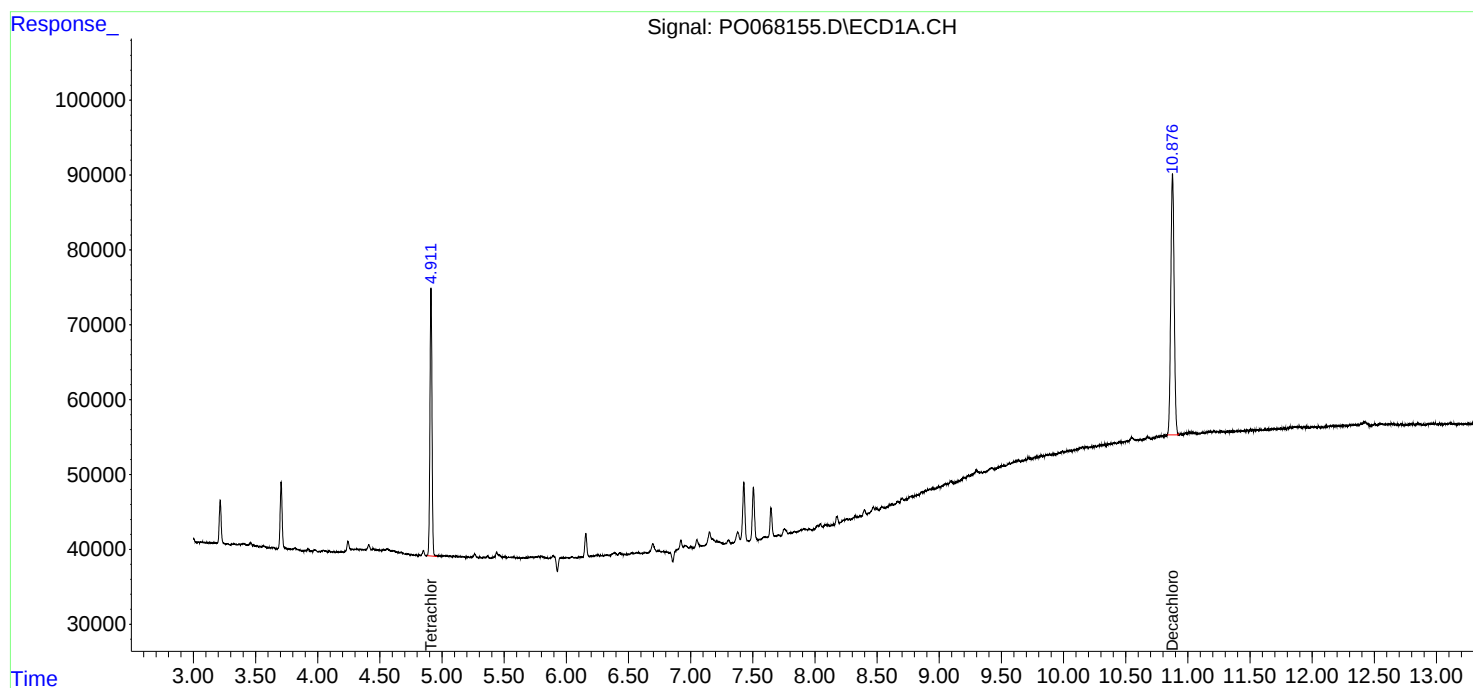

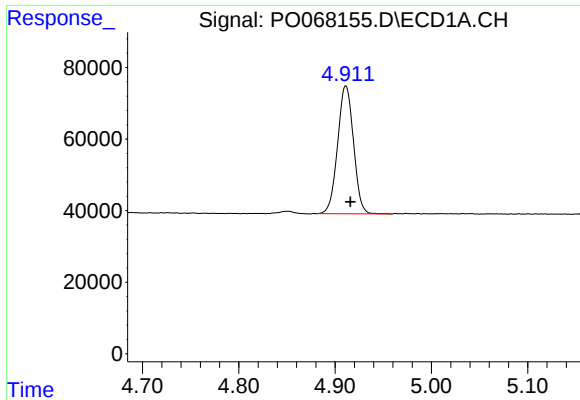


#1 Tetrachloro-m-xylene

R.T.: 4.911 min
Delta R.T.: -0.005 min
Response: 409318
Conc: 17.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-012


Manual Integrations
APPROVED

Sohil
5/6/2020 12:18:20 PM

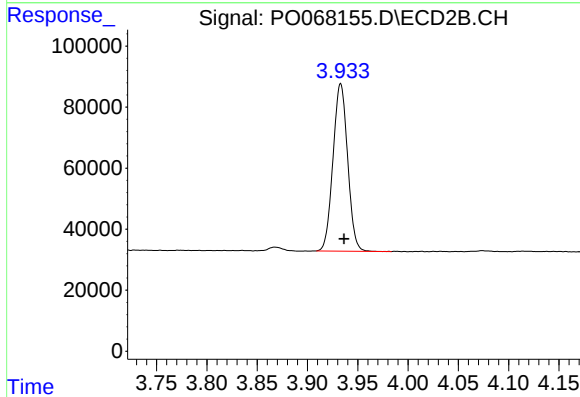


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 555057
Conc: 17.37 ng/ml

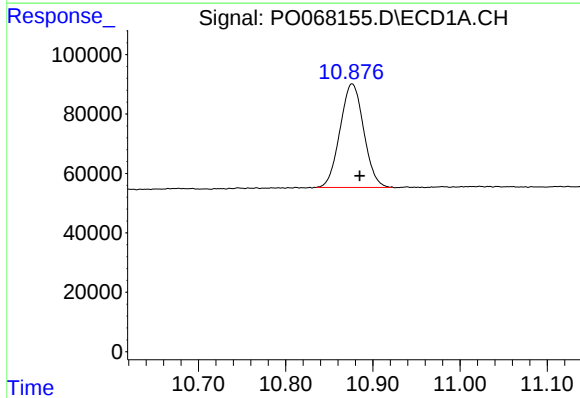

#2 Decachlorobiphenyl

R.T.: 10.876 min
Delta R.T.: -0.009 min
Response: 658683
Conc: 17.45 ng/ml m

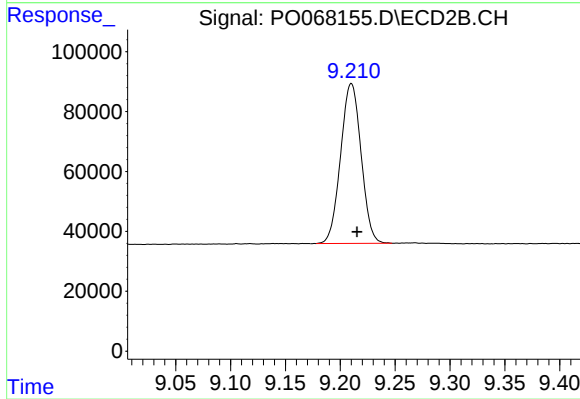

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: -0.006 min
Response: 693693
Conc: 17.97 ng/ml m