

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050520\
 Data File : P0068165.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2020 10:24
 Operator : DD\AJ
 Sample : L2476-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-03-008-B

Manual Integrations
 APPROVED

Sohil
 5/6/2020 12:23:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 10:58:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.910	3.934	673002	899951	28.124	28.163
2) SA Decachlor...	10.875	9.208	888524	823078	23.544m	21.326m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050520\
Data File : P0068165.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2020 10:24
Operator : DD\AJ
Sample : L2476-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-GF-03-008-B


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 10:58:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

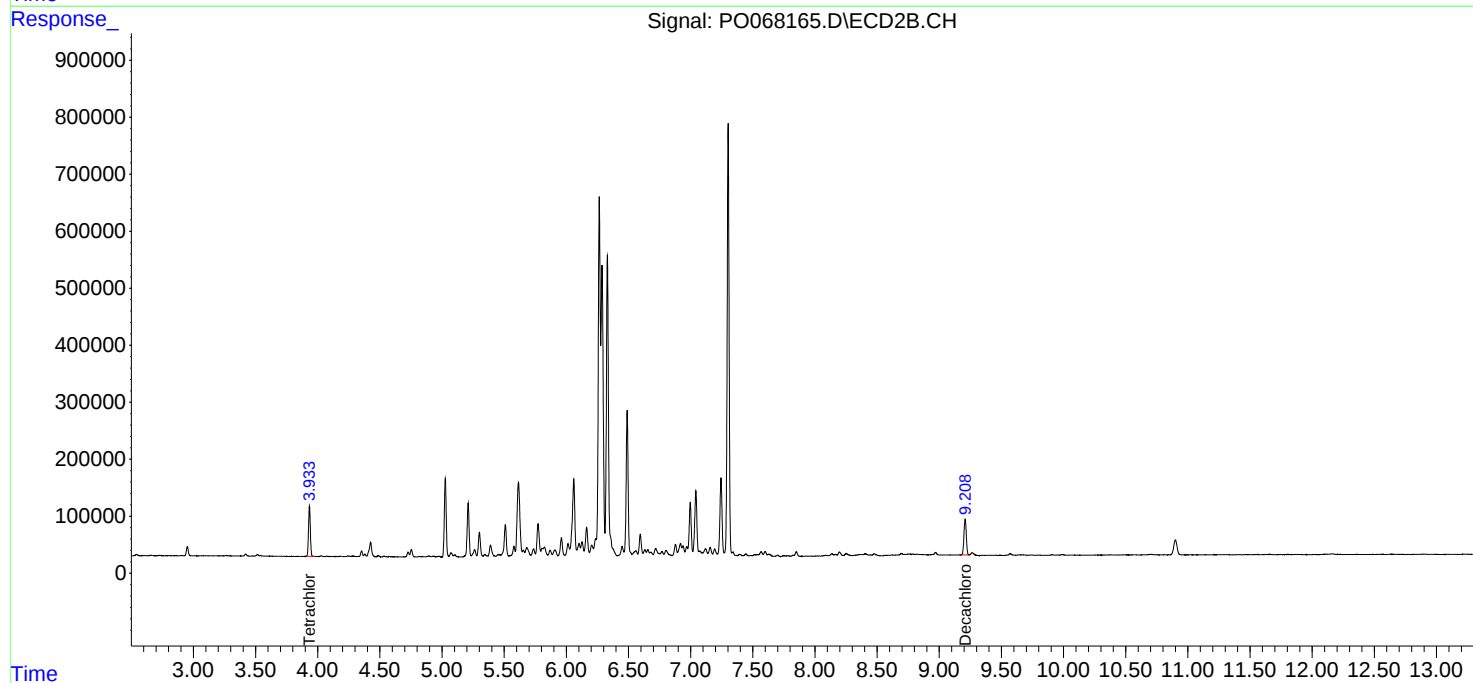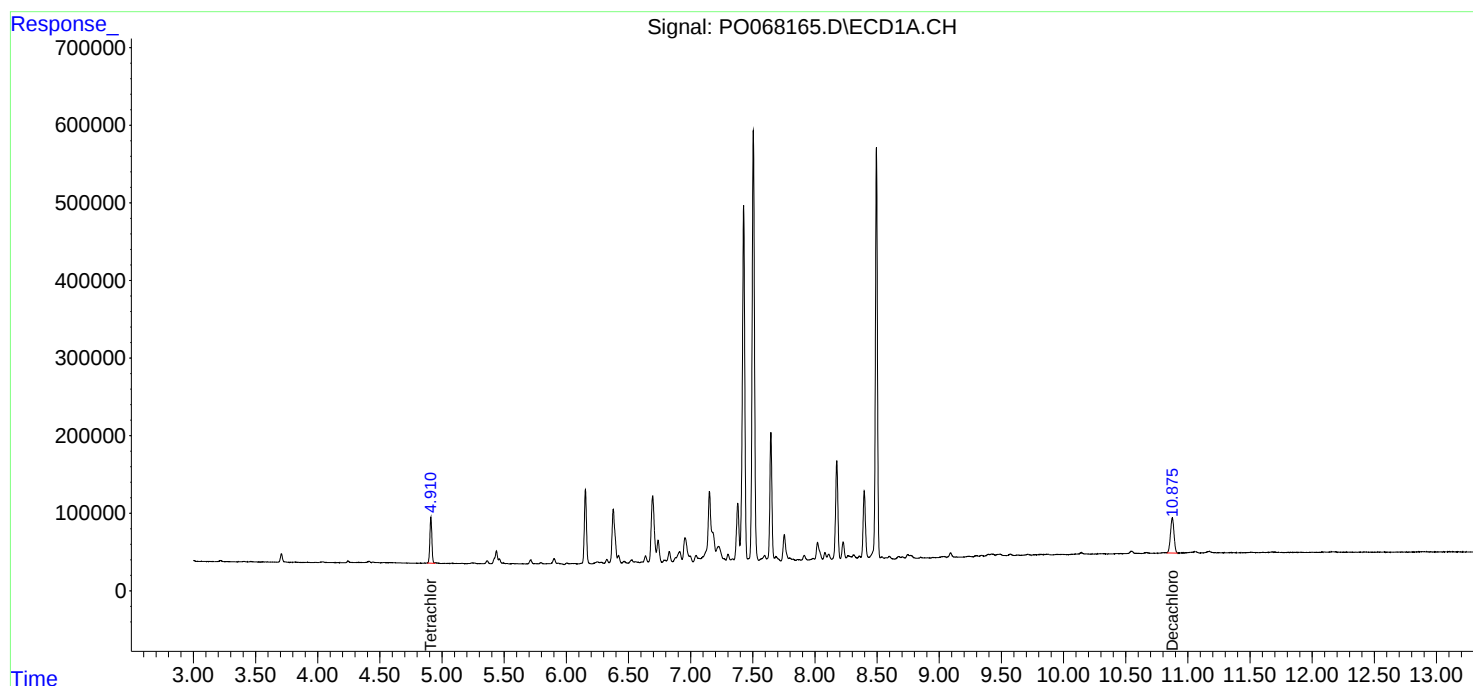

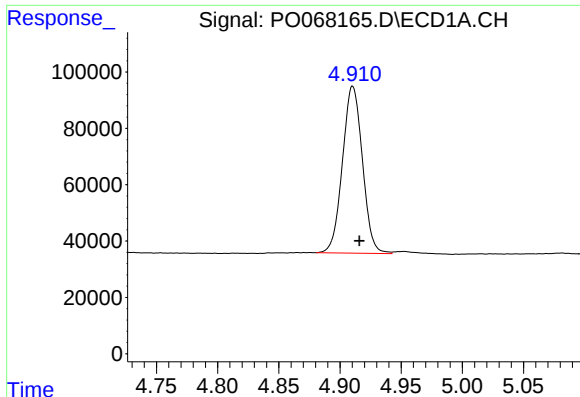


#1 Tetrachloro-m-xylene

R.T.: 4.910 min
Delta R.T.: -0.006 min
Response: 673002
Conc: 28.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-03-008-B


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:16 PM

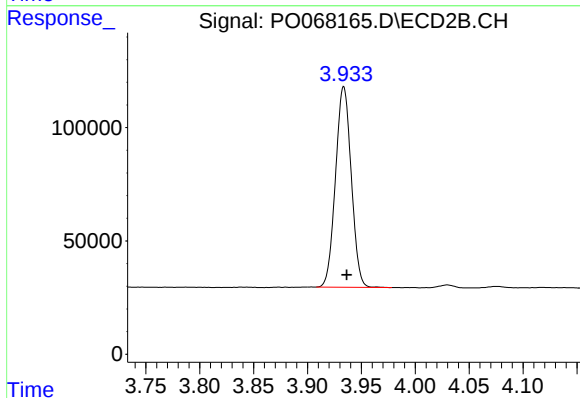


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.003 min
Response: 899951
Conc: 28.16 ng/ml

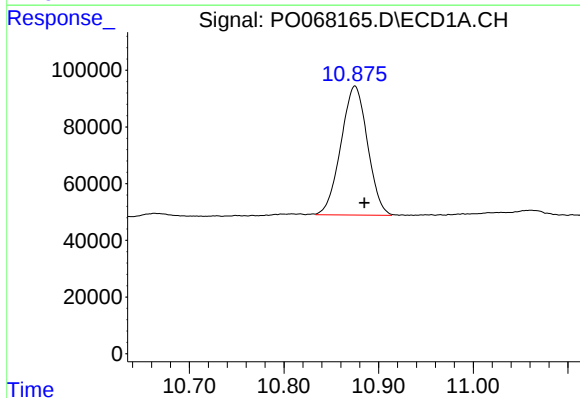

#2 Decachlorobiphenyl

R.T.: 10.875 min
Delta R.T.: -0.010 min
Response: 888524
Conc: 23.54 ng/ml m

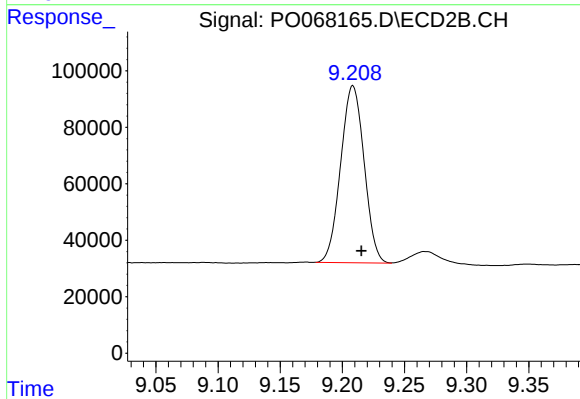

#2 Decachlorobiphenyl

R.T.: 9.208 min
Delta R.T.: -0.007 min
Response: 823078
Conc: 21.33 ng/ml m