

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050520\
 Data File : P0068166.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2020 10:41
 Operator : DD\AJ
 Sample : L2478-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-0D015-03-013

Manual Integrations
 APPROVED

Sohil
 5/6/2020 12:23:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 12:23:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.910	3.933	440763	607383	18.419m	19.007m
2) SA Decachlor...	10.872	9.208	635570	598505	16.841m	15.507m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050520\
Data File : P0068166.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2020 10:41
Operator : DD\AJ
Sample : L2478-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-013


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 12:23:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

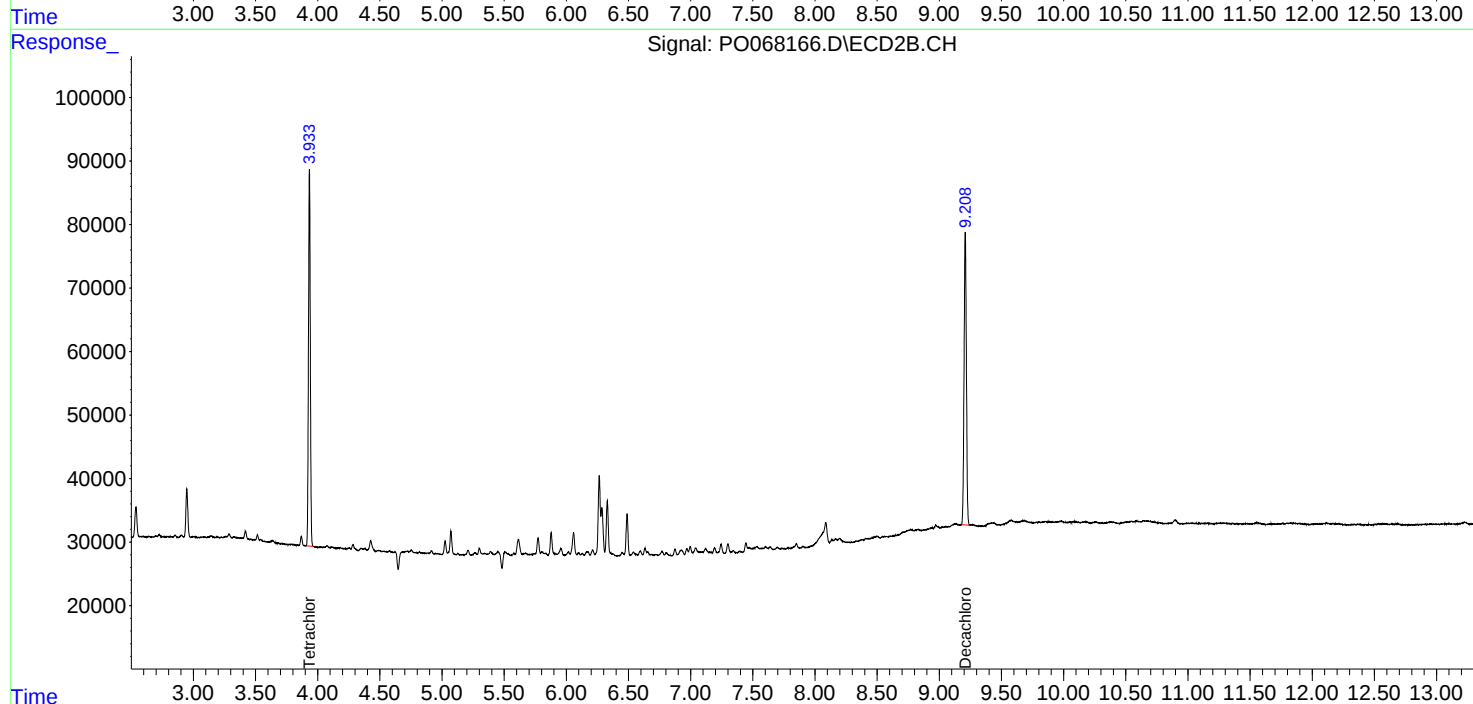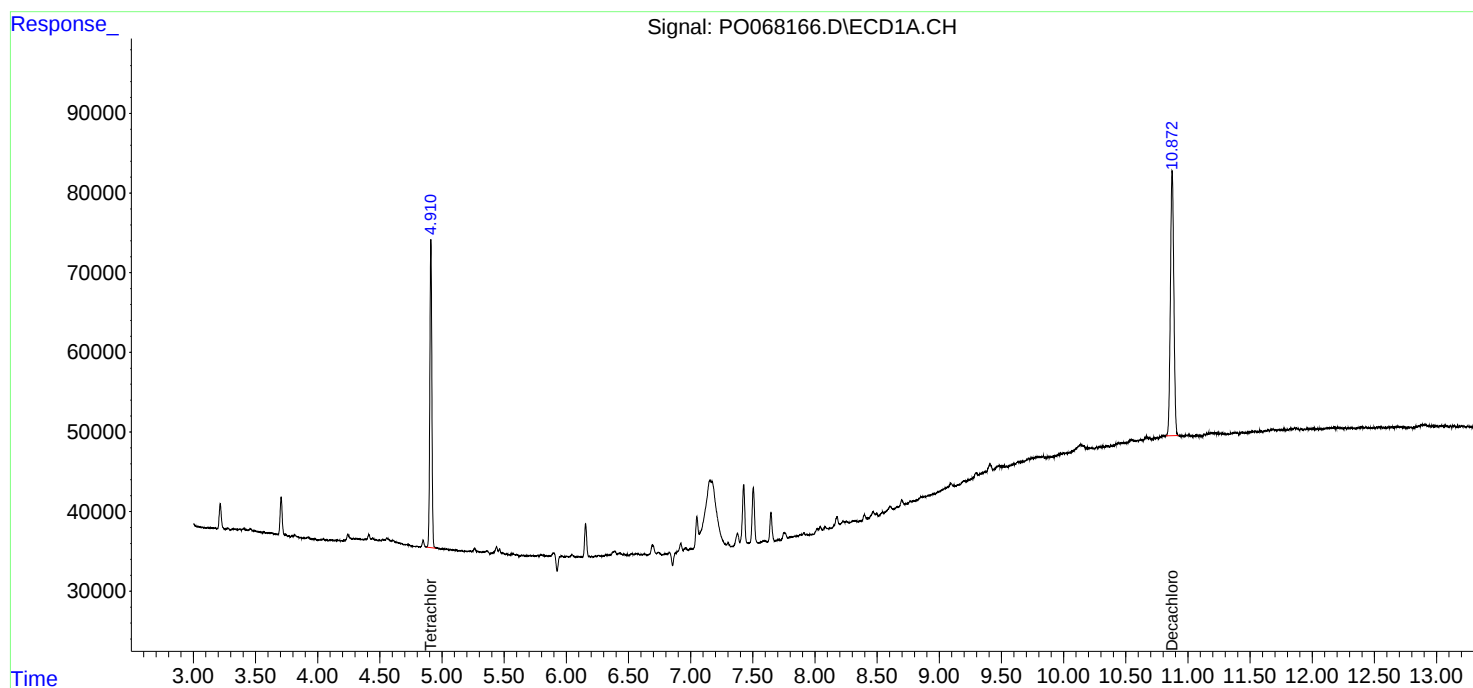

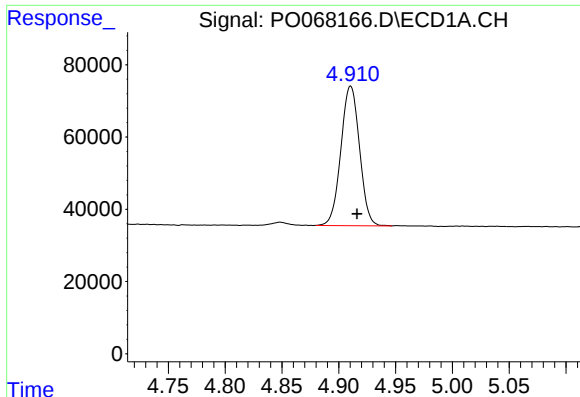


#1 Tetrachloro-m-xylene

R.T.: 4.910 min
Delta R.T.: -0.006 min
Response: 440763
Conc: 18.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-013


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:18 PM

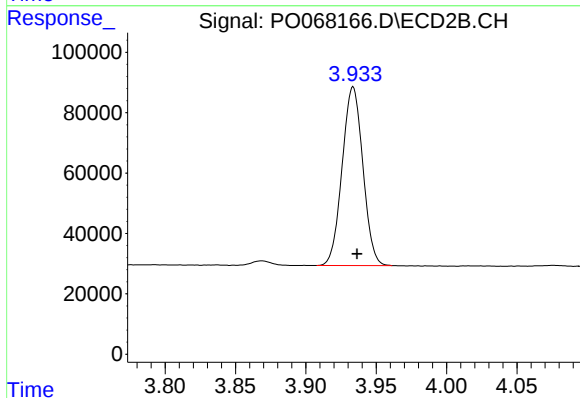


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 607383
Conc: 19.01 ng/ml m

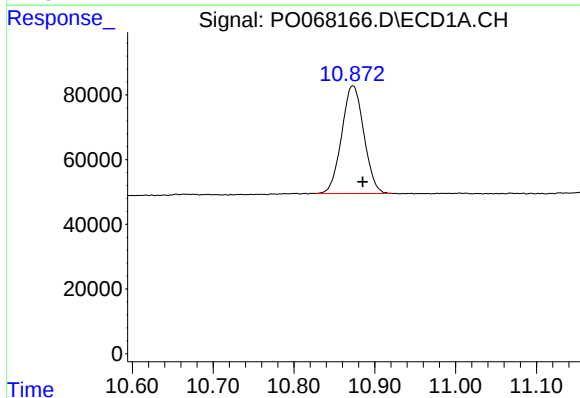

#2 Decachlorobiphenyl

R.T.: 10.872 min
Delta R.T.: -0.013 min
Response: 635570
Conc: 16.84 ng/ml m

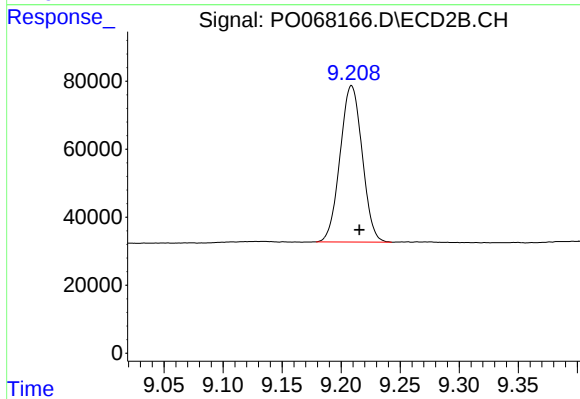

#2 Decachlorobiphenyl

R.T.: 9.208 min
Delta R.T.: -0.007 min
Response: 598505
Conc: 15.51 ng/ml m