

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050520\
 Data File : P0068169.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2020 11:32
 Operator : DD\AJ
 Sample : L2480-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-0D015-03-015

Manual Integrations
 APPROVED

Sohil
 5/6/2020 12:23:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 12:24:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.910	3.933	418085	564242	17.471	17.657
2) SA Decachlor...	10.873	9.209	599155	585534	15.876	15.171m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050520\
Data File : P0068169.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2020 11:32
Operator : DD\AJ
Sample : L2480-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-015


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 12:24:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

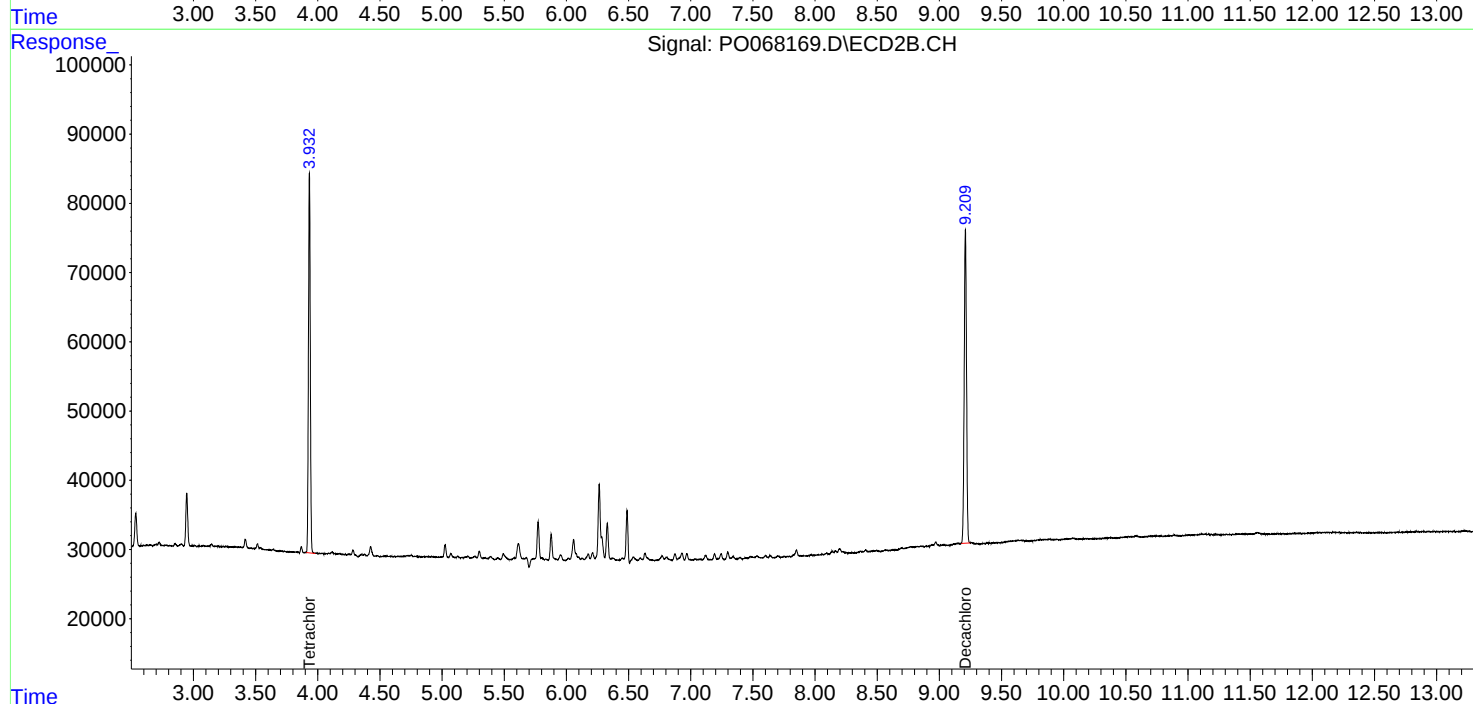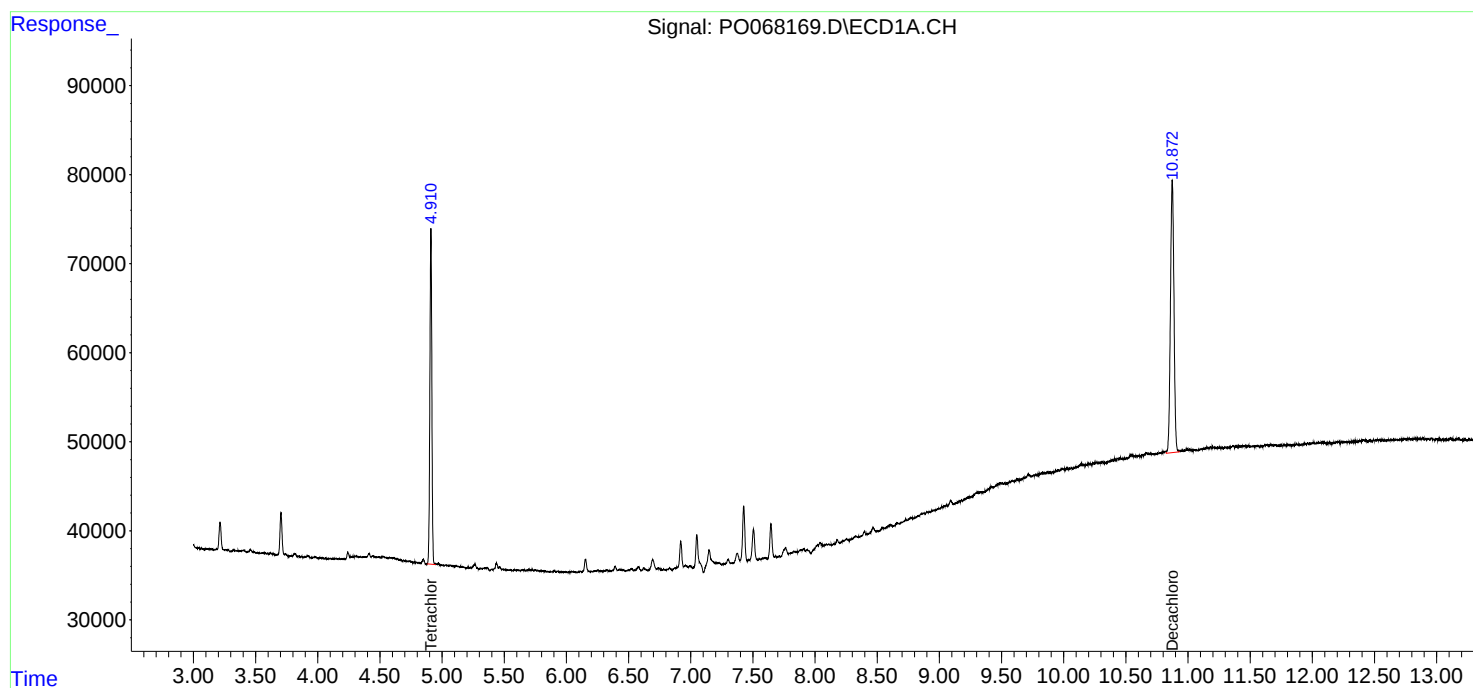

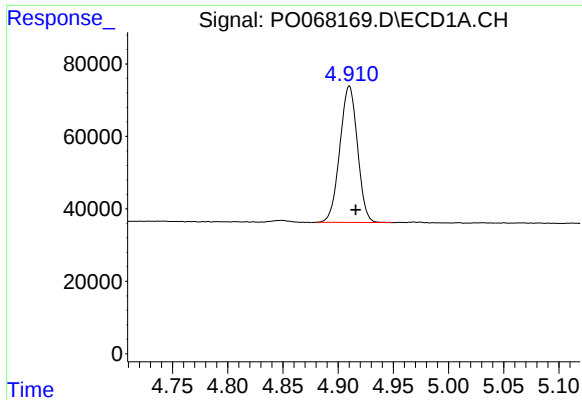


#1 Tetrachloro-m-xylene

R.T.: 4.910 min
Delta R.T.: -0.006 min
Response: 418085
Conc: 17.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-015


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:21 PM

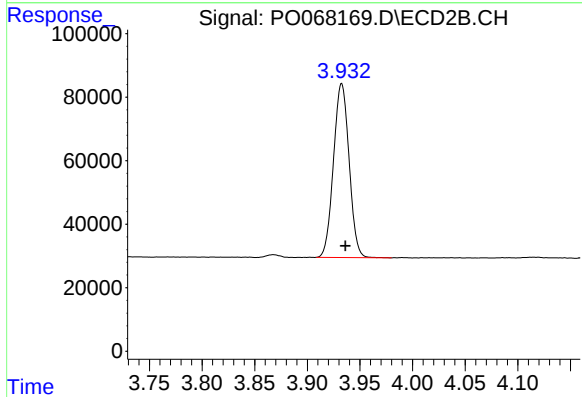


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.004 min
Response: 564242
Conc: 17.66 ng/ml

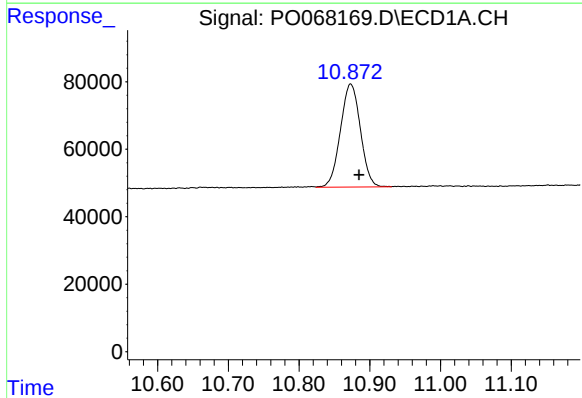

#2 Decachlorobiphenyl

R.T.: 10.873 min
Delta R.T.: -0.012 min
Response: 599155
Conc: 15.88 ng/ml

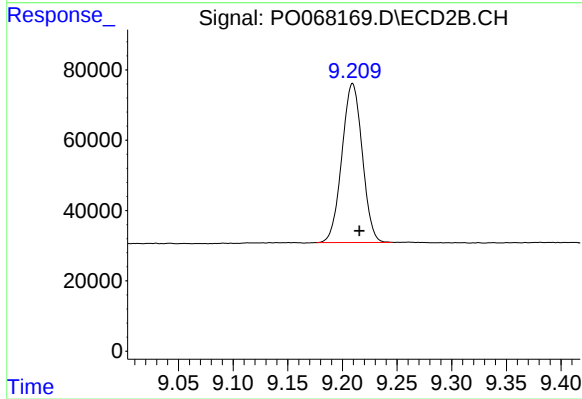

#2 Decachlorobiphenyl

R.T.: 9.209 min
Delta R.T.: -0.006 min
Response: 585534
Conc: 15.17 ng/ml m