

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050520\
 Data File : P0068172.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 May 2020 12:23
 Operator : DD\AJ
 Sample : L2464-01 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRE-50006

Manual Integrations
 APPROVED

Sohil
 5/6/2020 12:23:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 13:49:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.911	3.934	78677	111094	3.288	3.477
2) SA Decachlor...	10.876	9.212	99814	95624	2.645m	2.478

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050520\
Data File : PO068172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 May 2020 12:23
Operator : DD\AJ
Sample : L2464-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TRE-50006


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 13:49:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

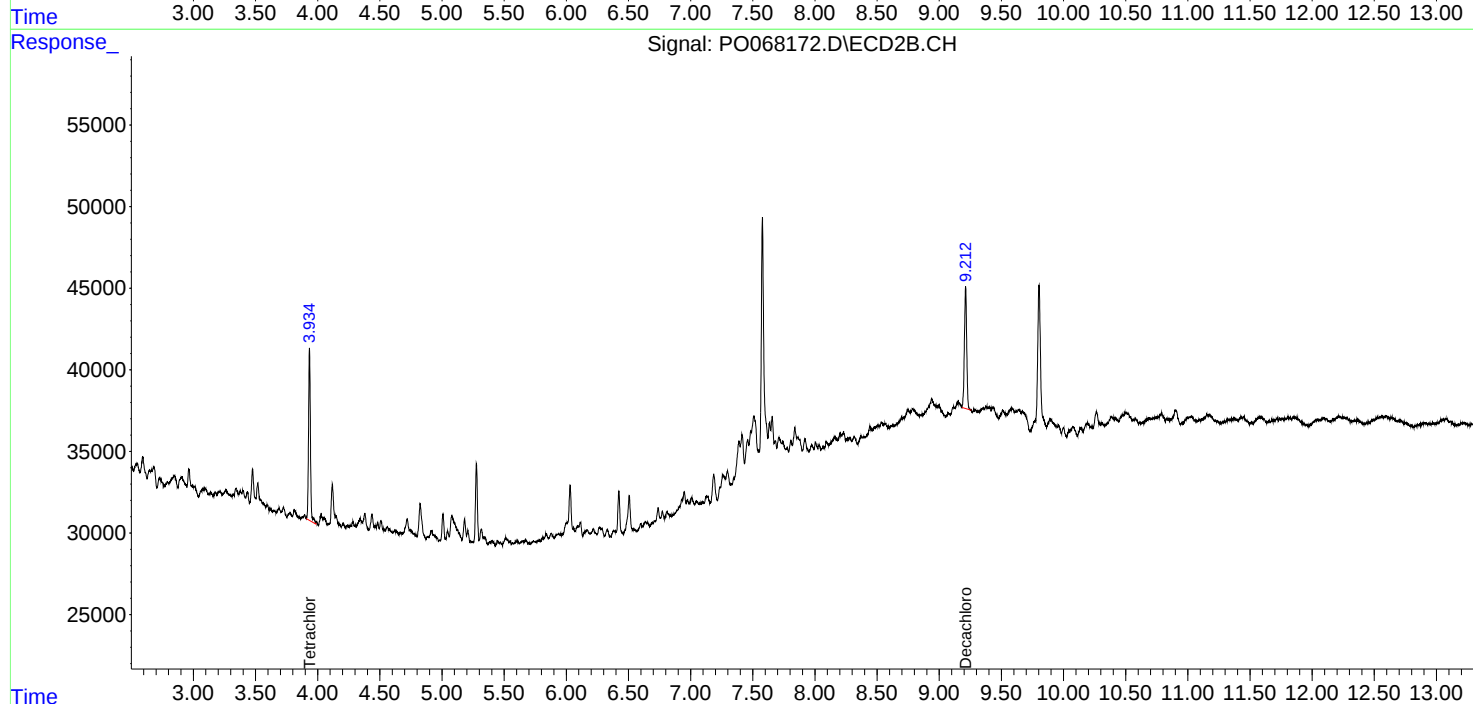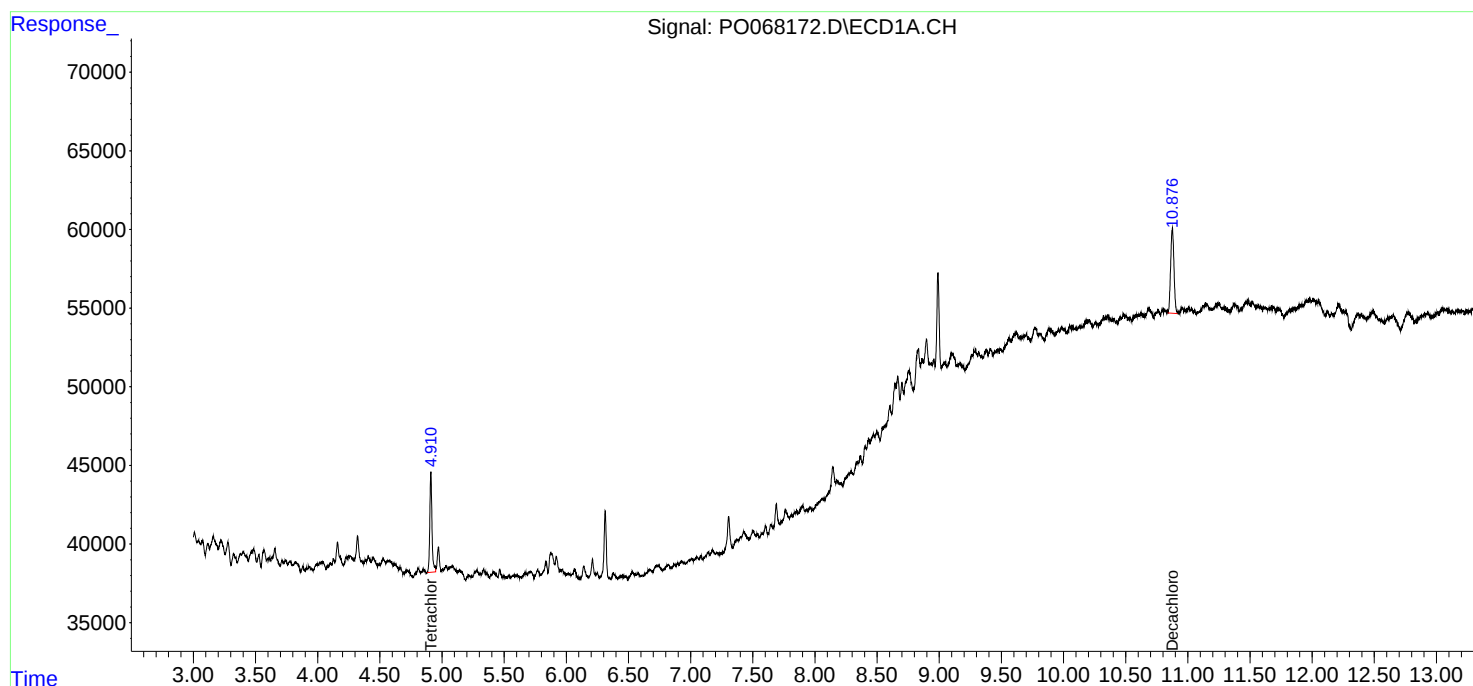

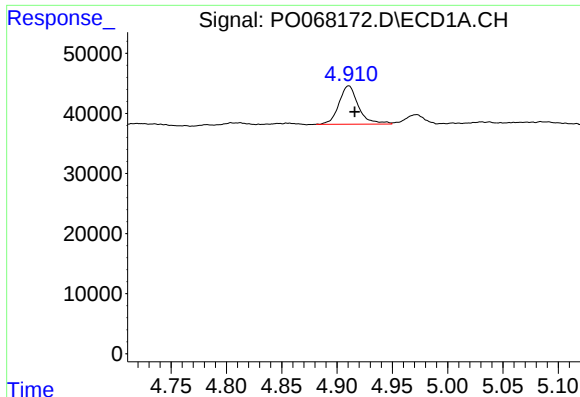


#1 Tetrachloro-m-xylene

R.T.: 4.911 min
Delta R.T.: -0.005 min
Response: 78677
Conc: 3.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-50006


Manual Integrations
APPROVED

Sohil
5/6/2020 12:23:23 PM

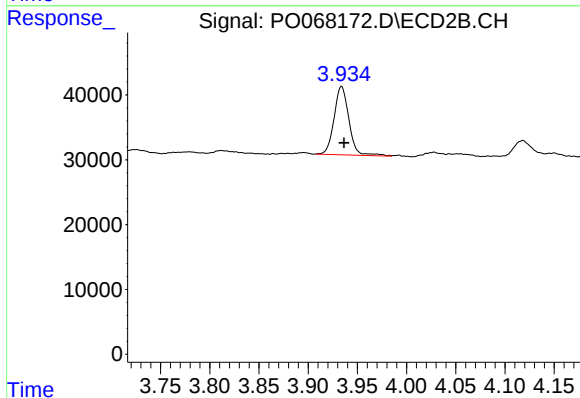


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 111094
Conc: 3.48 ng/ml

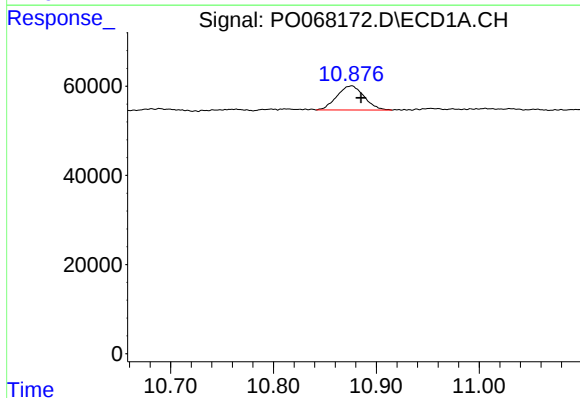

#2 Decachlorobiphenyl

R.T.: 10.876 min
Delta R.T.: -0.009 min
Response: 99814
Conc: 2.64 ng/ml m

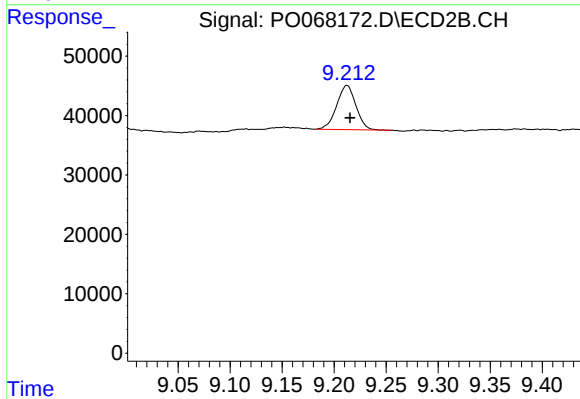

#2 Decachlorobiphenyl

R.T.: 9.212 min
Delta R.T.: -0.003 min
Response: 95624
Conc: 2.48 ng/ml