

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050620\
 Data File : P0068190.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 May 2020 10:18
 Operator : DD\AJ
 Sample : L2483-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 6FT-TP-1

Manual Integrations
 APPROVED

Sohil
 5/7/2020 8:14:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 10:51:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.911	3.934	564789	746067	23.602	23.347
2) SA Decachlor...	10.873	9.211	825982	819903	21.887m	21.244

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050620\
Data File : P0068190.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 May 2020 10:18
Operator : DD\AJ
Sample : L2483-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
6FT-TP-1


Manual Integrations
APPROVED

Sohil
5/7/2020 8:14:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 10:51:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

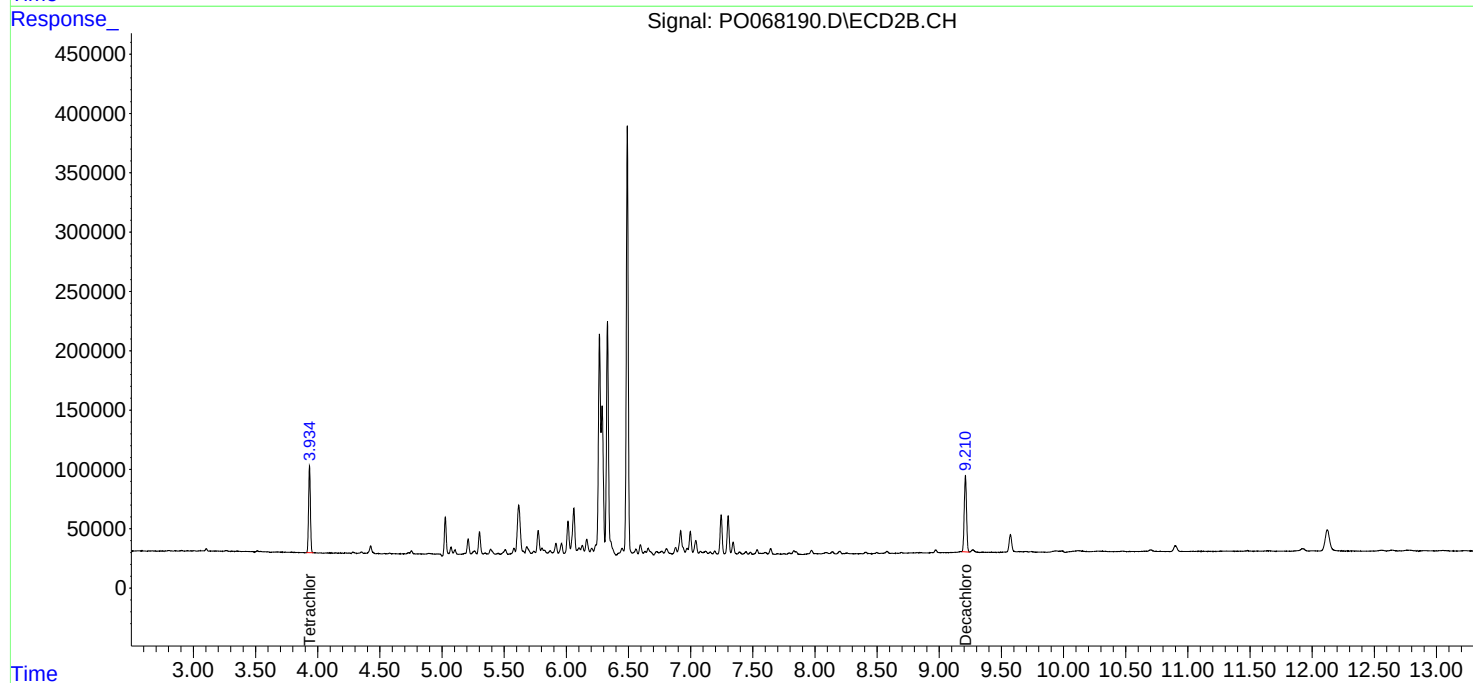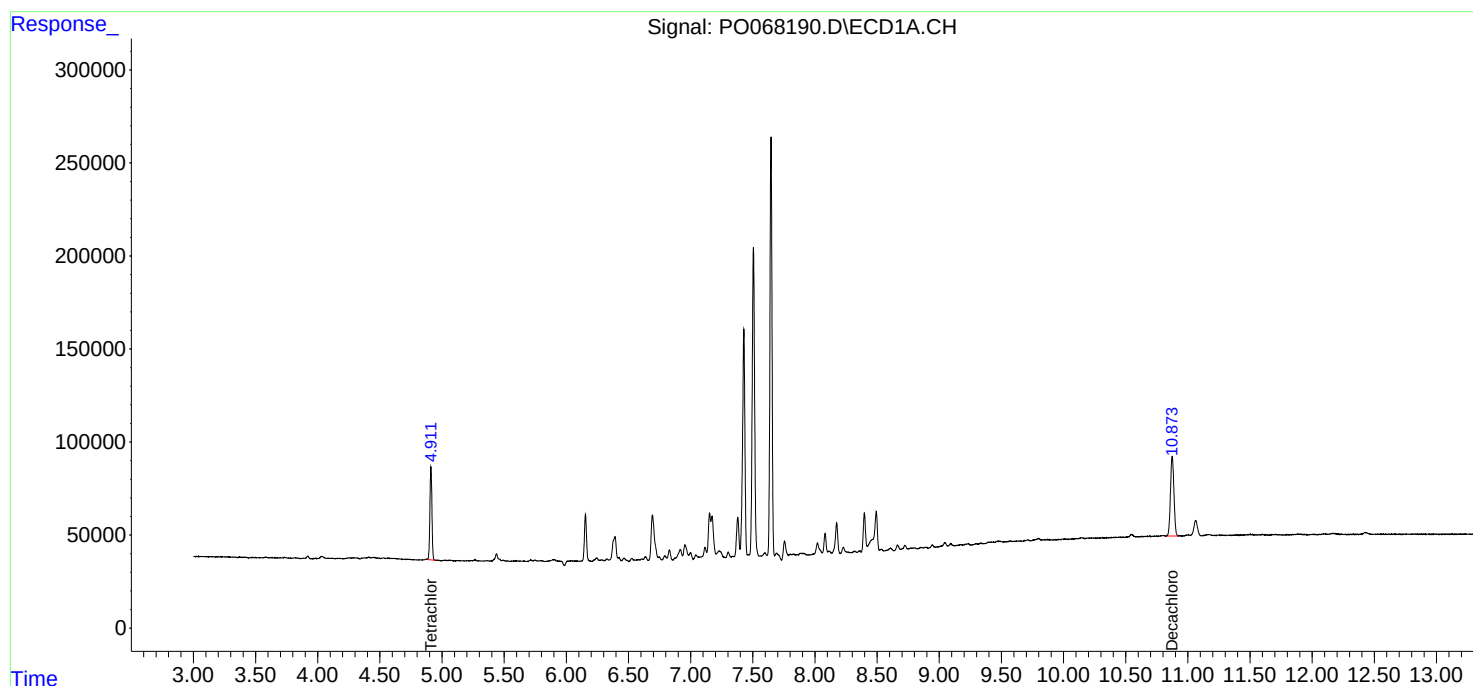

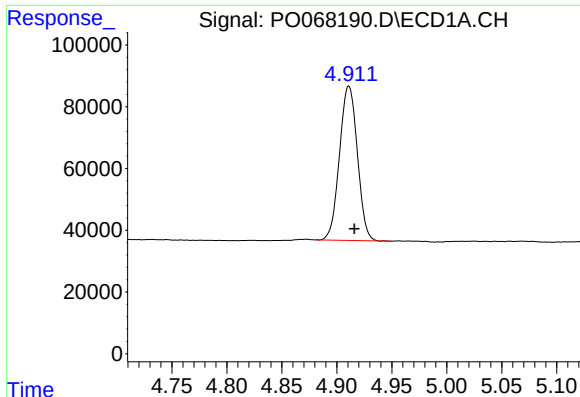


#1 Tetrachloro-m-xylene

R.T.: 4.911 min
Delta R.T.: -0.005 min
Response: 564789
Conc: 23.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
6FT-TP-1


Manual Integrations
APPROVED

Sohil
5/7/2020 8:14:15 AM

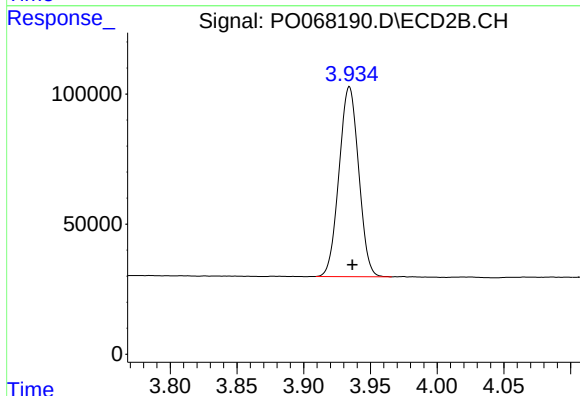


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 746067
Conc: 23.35 ng/ml

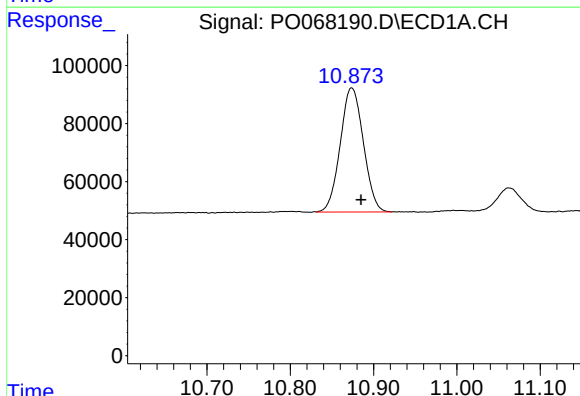

#2 Decachlorobiphenyl

R.T.: 10.873 min
Delta R.T.: -0.012 min
Response: 825982
Conc: 21.89 ng/ml m

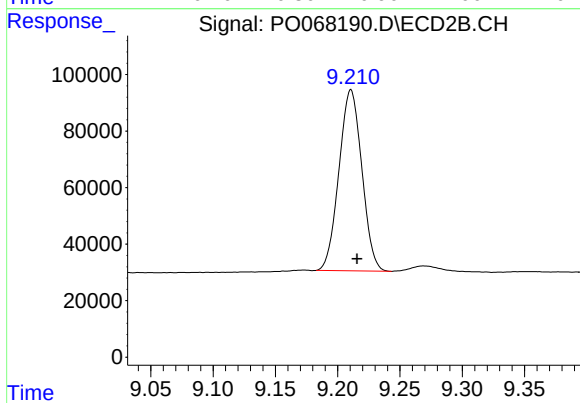

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.005 min
Response: 819903
Conc: 21.24 ng/ml