

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
 Data File : P0055943.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 17:56
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 04:07:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.273	3.589	721020	778029	24.094	27.547
2)	SA Decachlor...	9.867	8.536	507701	377691	13.569	13.966
Target Compounds							
7)	L1 AR-1016-5	0.000	5.108	0	1676	N.D.	1.522 #
15)	L3 AR-1232-5	0.000	5.108	0	1676	N.D.	3.458 #
20)	L4 AR-1242-5	6.283	0.000	39716	0	36.305	N.D. #
24)	L5 AR-1248-4	6.283	5.108	39716	1676	22.777	1.194 #
25)	L5 AR-1248-5	6.283	0.000	39716	0	23.777	N.D. #
26)	L6 AR-1254-1	6.283	0.000	39716	0	18.914	N.D. #
28)	L6 AR-1254-3	6.875	0.000	23129	0	6.362	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
Data File : P0055943.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 17:56
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 04:07:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

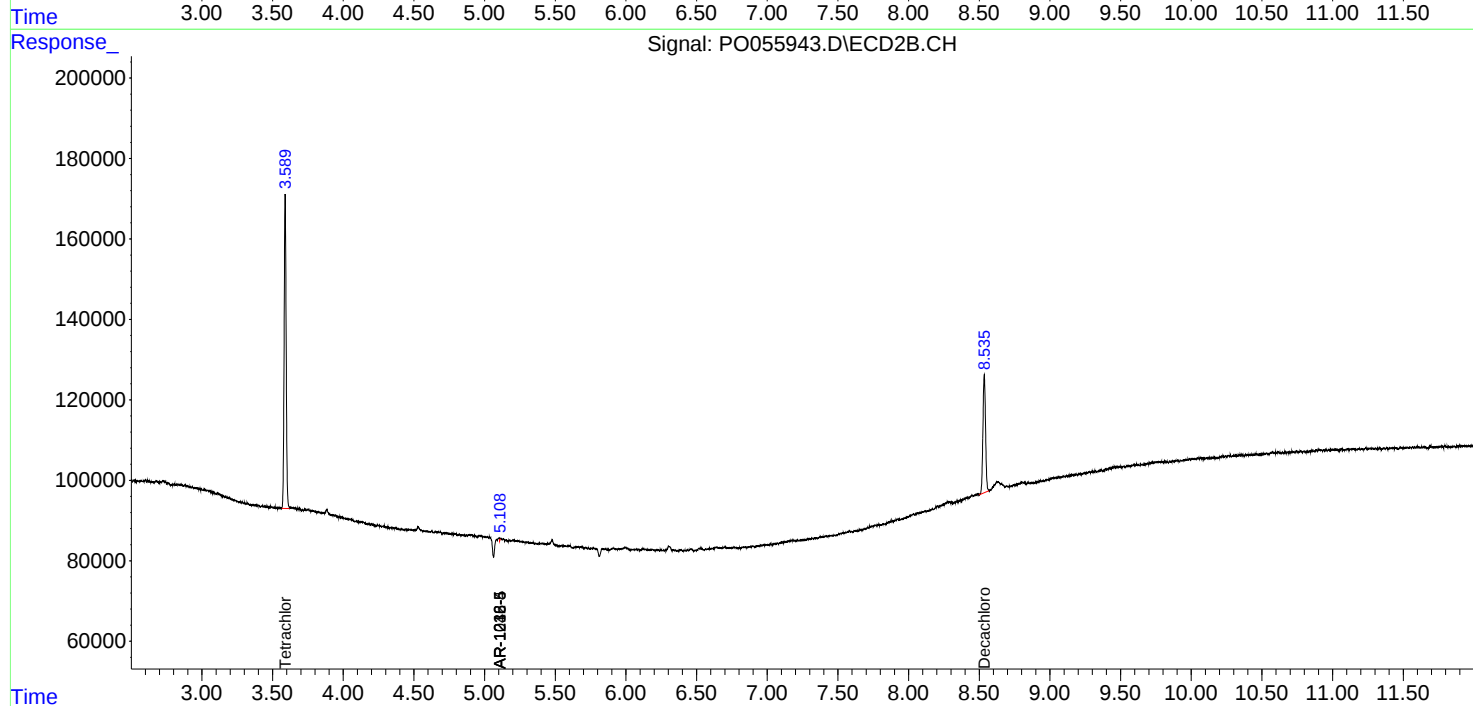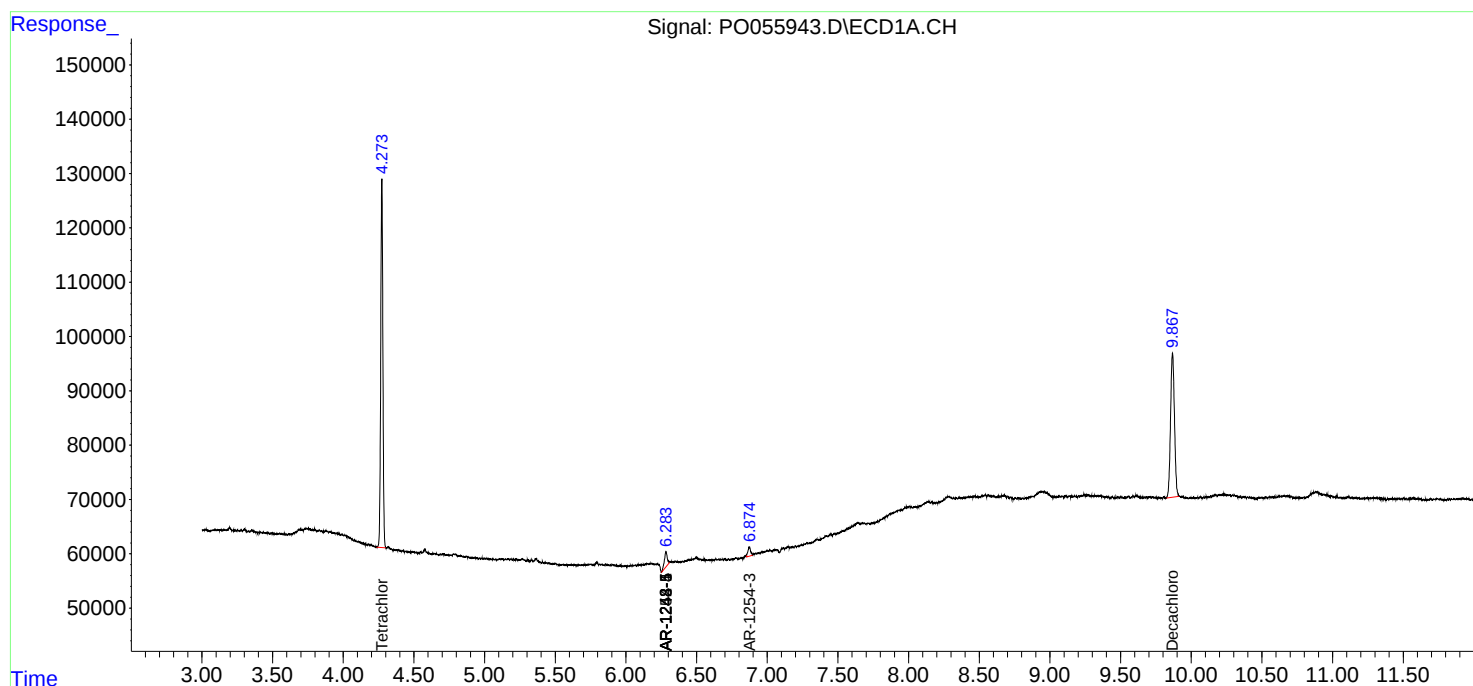


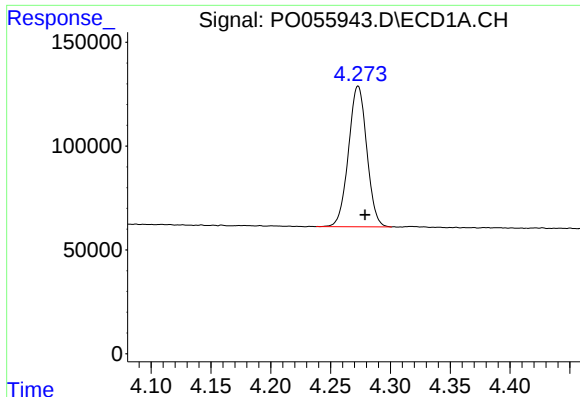

#1 Tetrachloro-m-xylene


R.T.: 4.273 min
Delta R.T.: -0.006 min
Response: 721020
Conc: 24.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

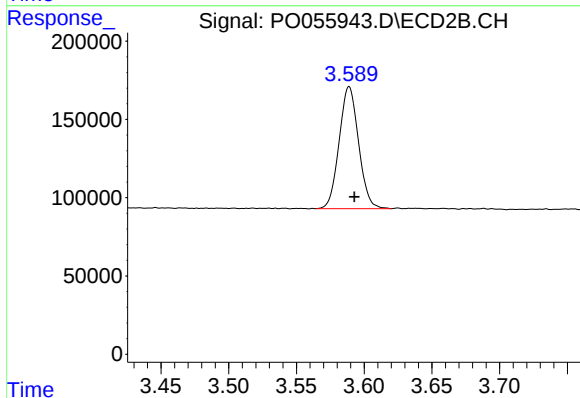


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 778029
Conc: 27.55 ng/ml

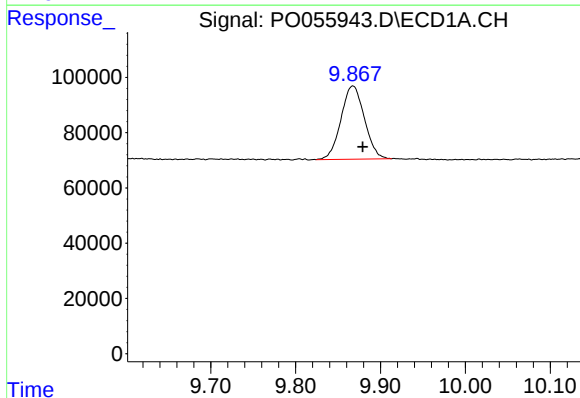


#2 Decachlorobiphenyl

R.T.: 9.867 min
Delta R.T.: -0.012 min
Response: 507701
Conc: 13.57 ng/ml

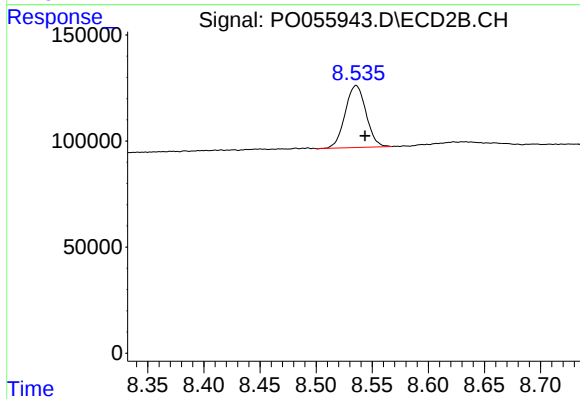

#2 Decachlorobiphenyl


R.T.: 8.536 min
Delta R.T.: -0.008 min
Response: 377691
Conc: 13.97 ng/ml

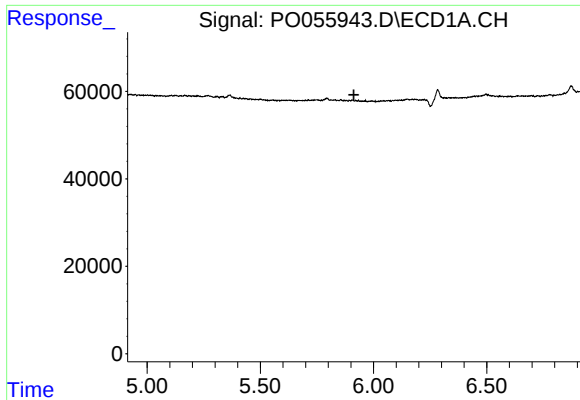

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

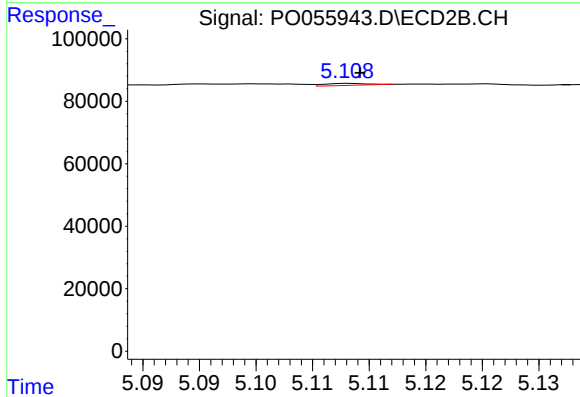


#7 AR-1016-5

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 1676
Conc: 1.52 ng/ml

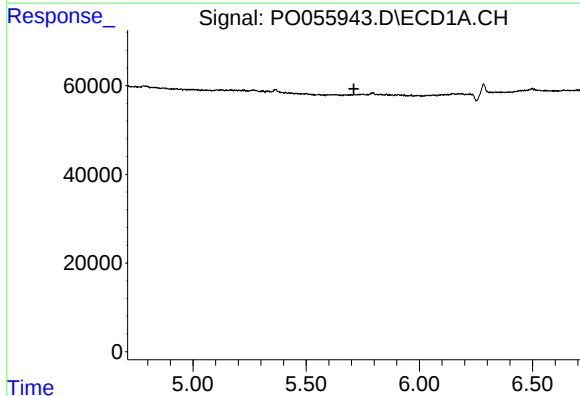


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.711 min
Response: 0
Conc: N.D.

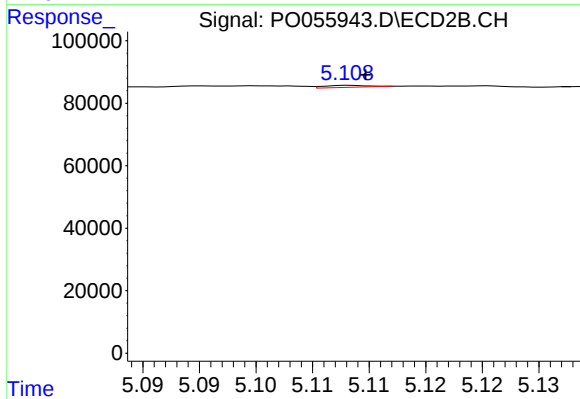

#15 AR-1232-5


R.T.: 5.108 min
Delta R.T.: -0.001 min
Response: 1676
Conc: 3.46 ng/ml

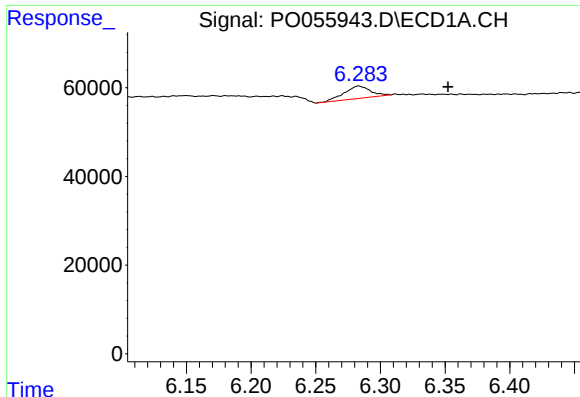

#20 AR-1242-5


R.T.: 6.283 min
Delta R.T.: -0.069 min
Response: 39716
Conc: 36.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

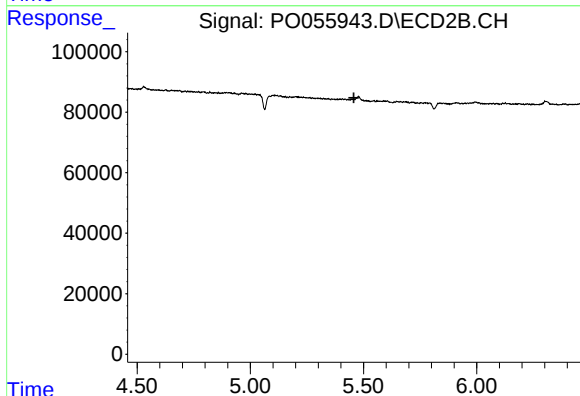


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.457 min
Response: 0
Conc: N.D.

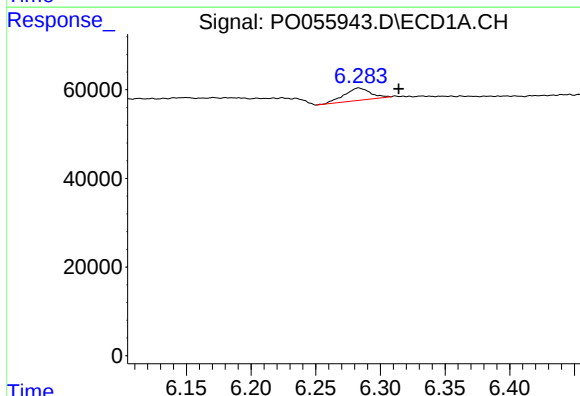


#24 AR-1248-4

R.T.: 6.283 min
Delta R.T.: -0.031 min
Response: 39716
Conc: 22.78 ng/ml

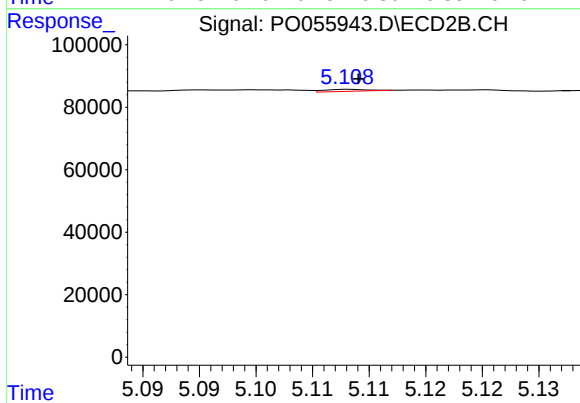

#24 AR-1248-4


R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 1676
Conc: 1.19 ng/ml

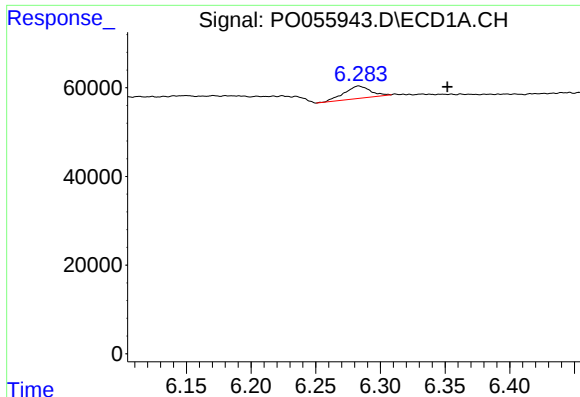

#25 AR-1248-5


R.T.: 6.283 min
Delta R.T.: -0.068 min
Response: 39716
Conc: 23.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

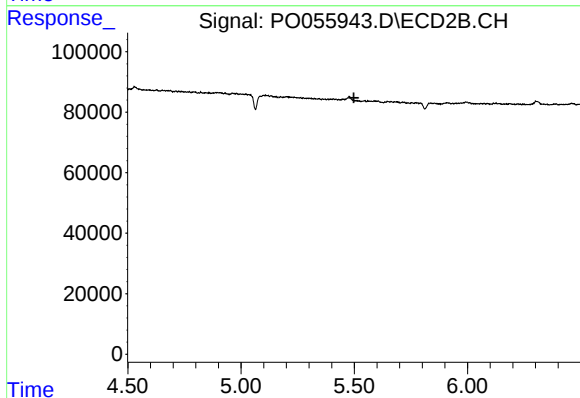


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.498 min
Response: 0
Conc: N.D.

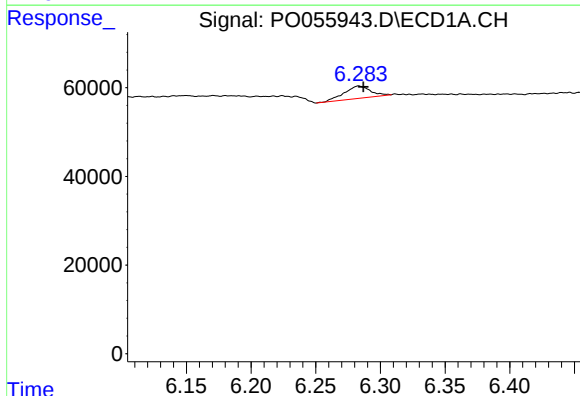


#26 AR-1254-1

R.T.: 6.283 min
Delta R.T.: -0.004 min
Response: 39716
Conc: 18.91 ng/ml

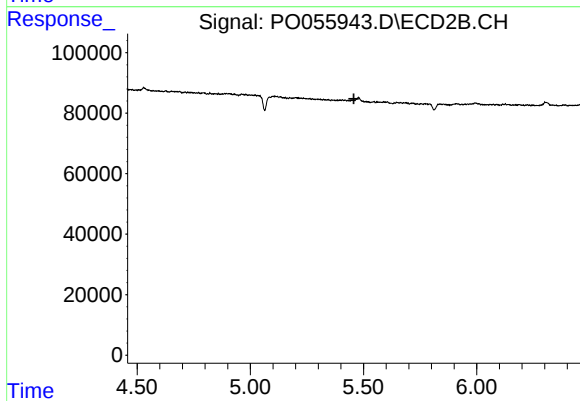

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.457 min
Response: 0
Conc: N.D.

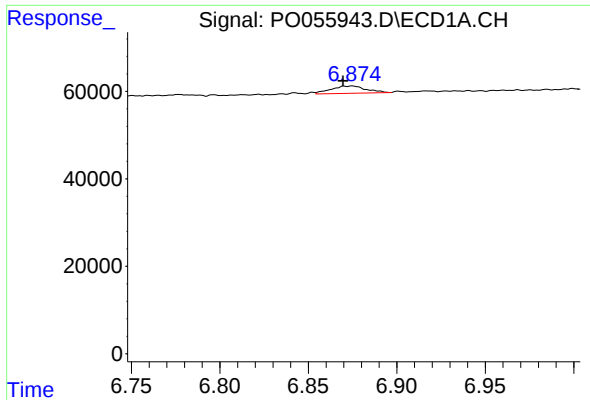

#28 AR-1254-3

R.T.: 6.875 min
Delta R.T.: 0.005 min
Response: 23129
Conc: 6.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

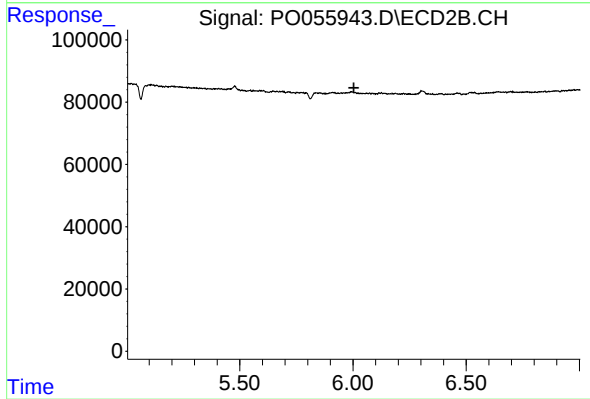

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.