

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0050719\
 Data File : P0055928.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 12:34
 Operator : SM/SJ
 Sample : K2672-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SB-02-COMP

Manual Integrations
 APPROVED

Ankita
 5/8/2019 4:15:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 03:59:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.274	3.589	751885	772048	25.125	27.336
2)	SA Decachlor...	9.867	8.536	1291996	816470	34.530	30.191m
Target Compounds							
31)	L7 AR-1260-1	7.025	6.128	372768	337241	172.618	153.070
32)	L7 AR-1260-2	7.278	6.313	1270028	411849	484.950	134.874m#
33)	L7 AR-1260-3	7.637	6.467	219555	287239	109.778	115.263m
34)	L7 AR-1260-4	7.858	6.935	334135	158279	144.484	76.705 #
35)	L7 AR-1260-5	8.171	7.175	360788	364548	85.045	72.586m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050719\
Data File : PO055928.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 12:34
Operator : SM/SJ
Sample : K2672-04
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-02-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:15:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 03:59:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

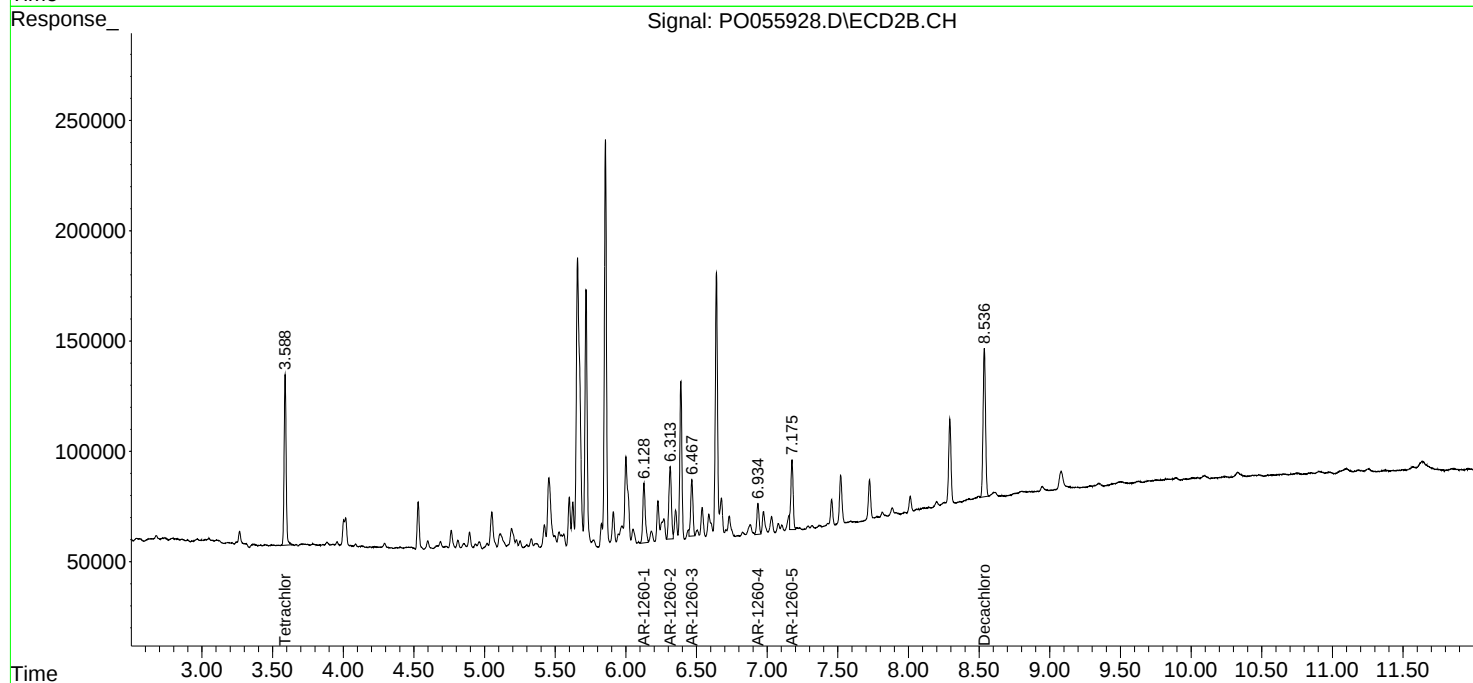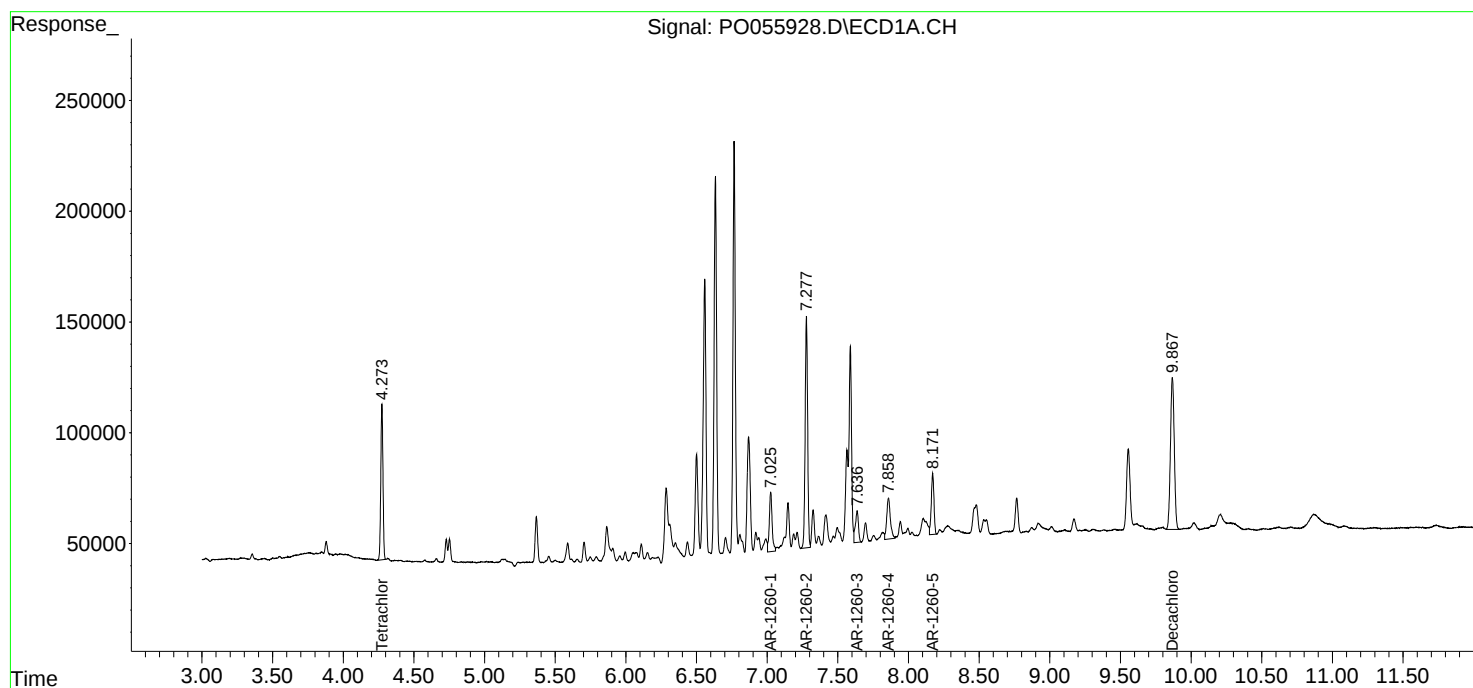

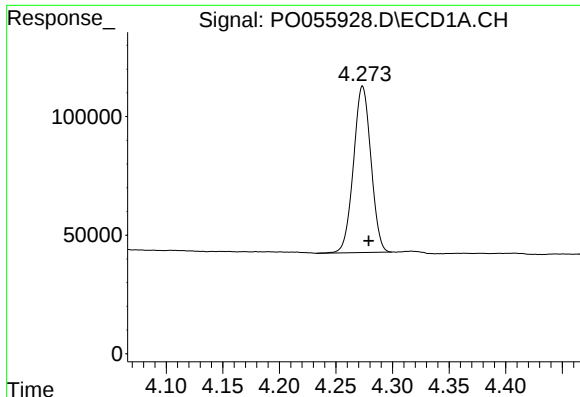


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 751885
Conc: 25.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:15:50 PM

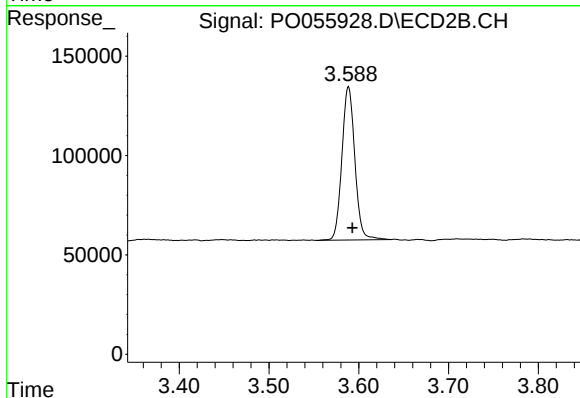


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 772048
Conc: 27.34 ng/ml

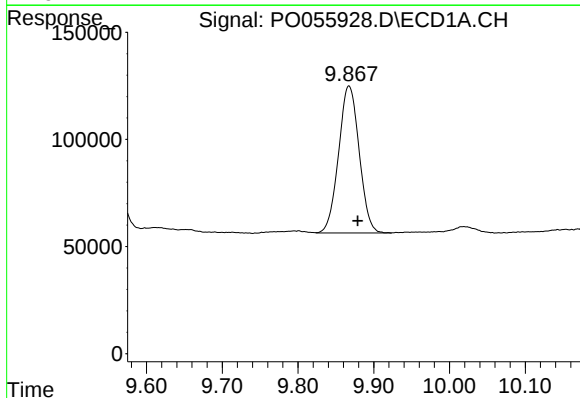


#2 Decachlorobiphenyl

R.T.: 9.867 min
Delta R.T.: -0.012 min
Response: 1291996
Conc: 34.53 ng/ml

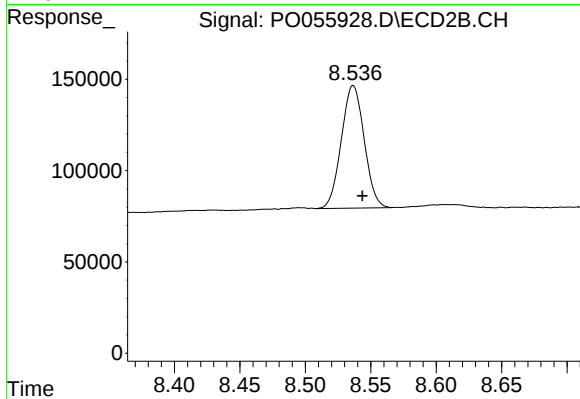

#2 Decachlorobiphenyl

R.T.: 8.536 min
Delta R.T.: -0.008 min
Response: 816470
Conc: 30.19 ng/ml m

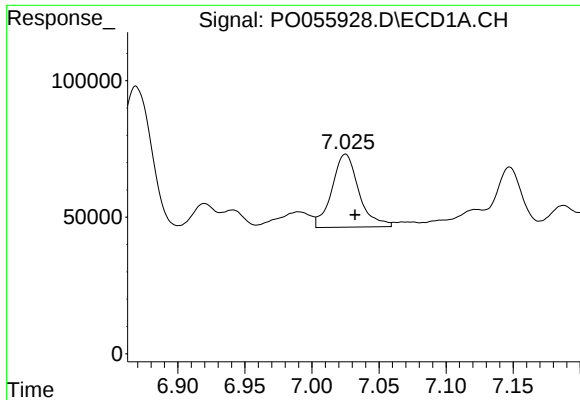


#31 AR-1260-1

R.T.: 7.025 min
Delta R.T.: -0.007 min
Response: 372768
Conc: 172.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:15:50 PM

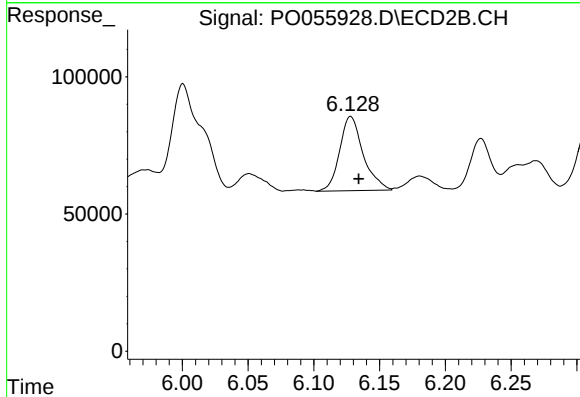


#31 AR-1260-1

R.T.: 6.128 min
Delta R.T.: -0.006 min
Response: 337241
Conc: 153.07 ng/ml

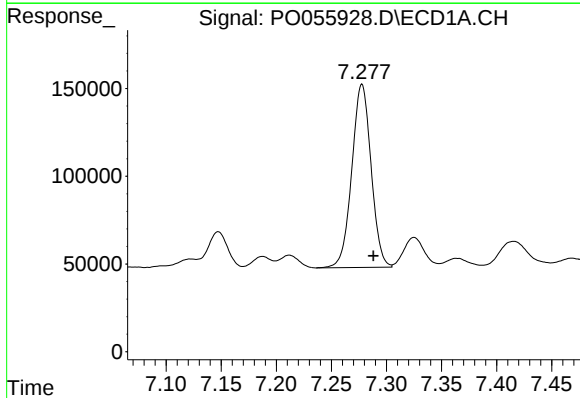


#32 AR-1260-2

R.T.: 7.278 min
Delta R.T.: -0.011 min
Response: 1270028
Conc: 484.95 ng/ml

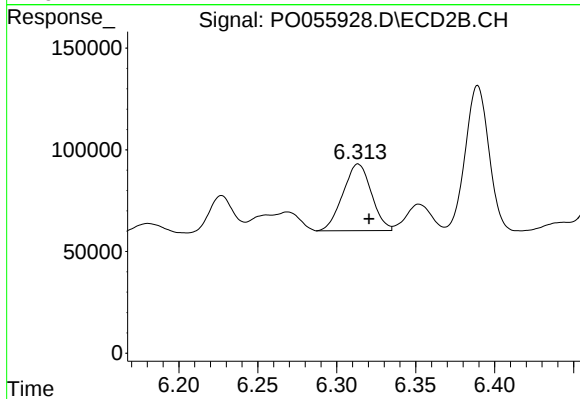

#32 AR-1260-2

R.T.: 6.313 min
Delta R.T.: -0.007 min
Response: 411849
Conc: 134.87 ng/ml m

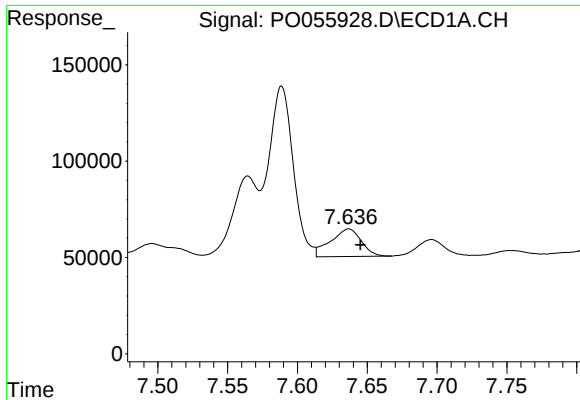


#33 AR-1260-3

R.T.: 7.637 min
Delta R.T.: -0.008 min
Response: 219555
Conc: 109.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:15:50 PM

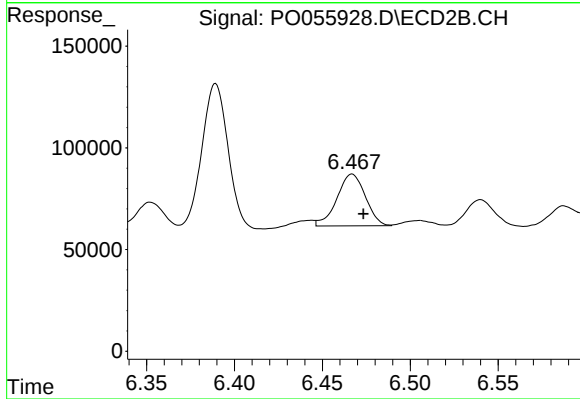


#33 AR-1260-3

R.T.: 6.467 min
Delta R.T.: -0.007 min
Response: 287239
Conc: 115.26 ng/ml m

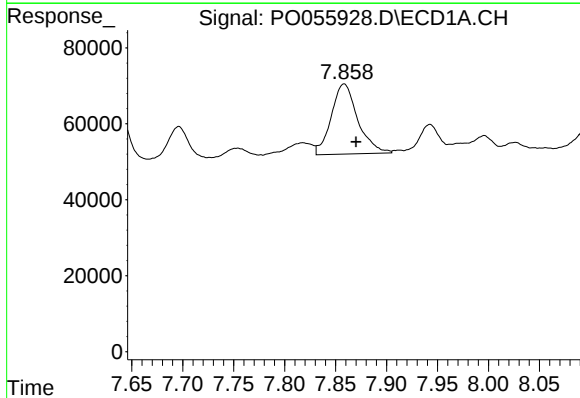


#34 AR-1260-4

R.T.: 7.858 min
Delta R.T.: -0.012 min
Response: 334135
Conc: 144.48 ng/ml

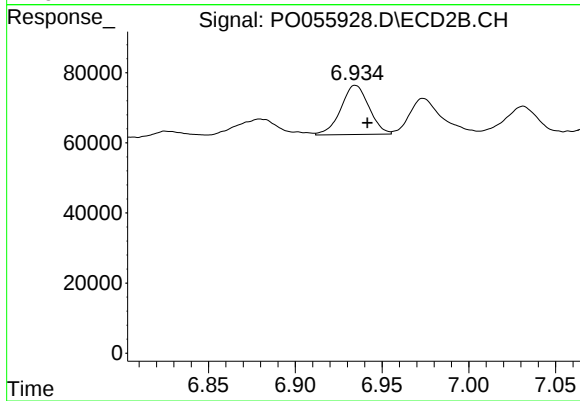

#34 AR-1260-4

R.T.: 6.935 min
Delta R.T.: -0.007 min
Response: 158279
Conc: 76.71 ng/ml

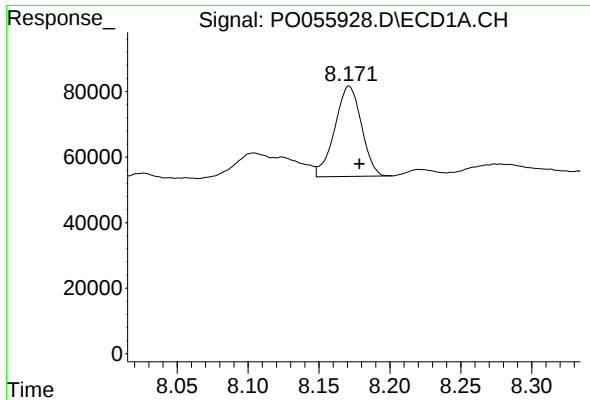


#35 AR-1260-5

R.T.: 8.171 min
Delta R.T.: -0.007 min
Response: 360788
Conc: 85.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-COMP

Manual Integrations
APPROVED

Ankita
5/8/2019 4:15:50 PM

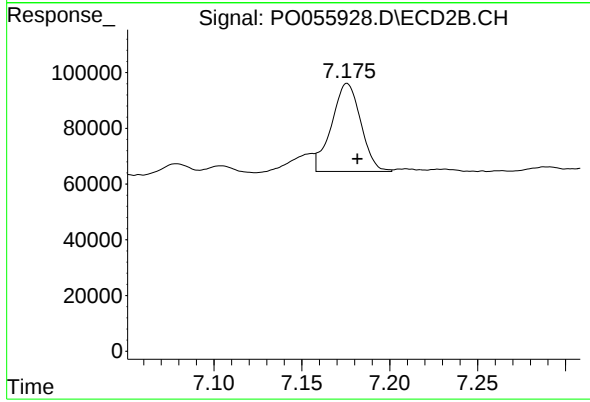

#35 AR-1260-5

R.T.: 7.175 min
Delta R.T.: -0.006 min
Response: 364548
Conc: 72.59 ng/ml m