

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
 Data File : P0055929.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 12:51
 Operator : SM/SJ
 Sample : K2672-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-03-COMP

Manual Integrations
 APPROVED

Ankita
 5/8/2019 4:15:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 03:59:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.589	829652	830198	27.724	29.394
2) SA Decachlor...	9.869	8.538	642608	3857898	17.174	142.658m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
Data File : P0055929.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 12:51
Operator : SM/SJ
Sample : K2672-06
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:15:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 03:59:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

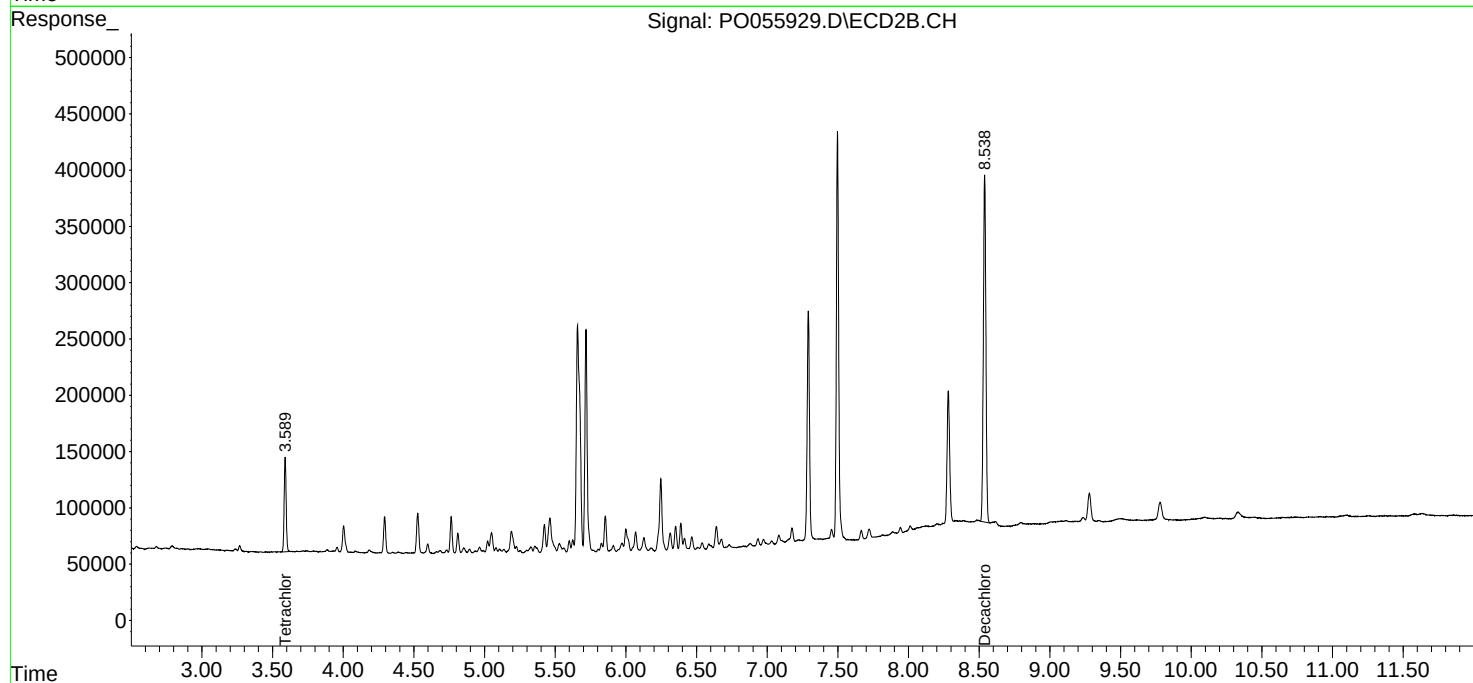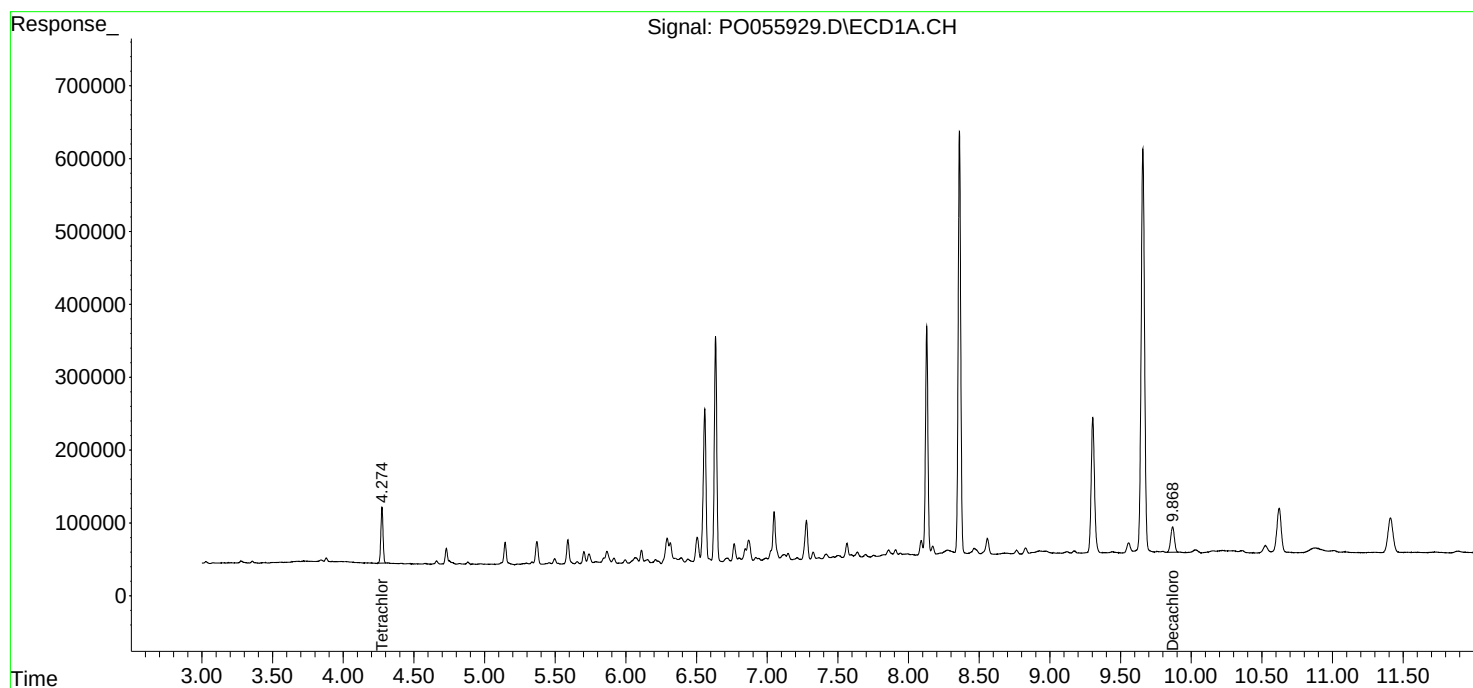

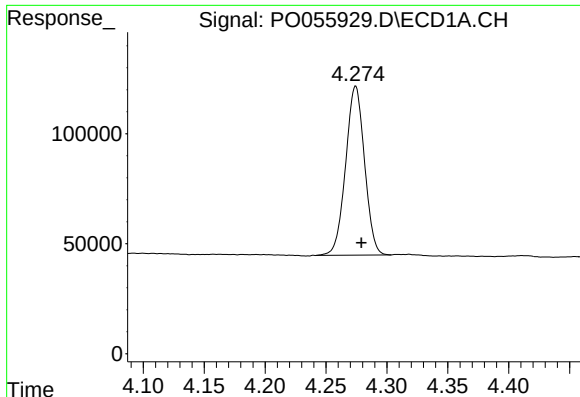


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 829652
Conc: 27.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:15:51 PM

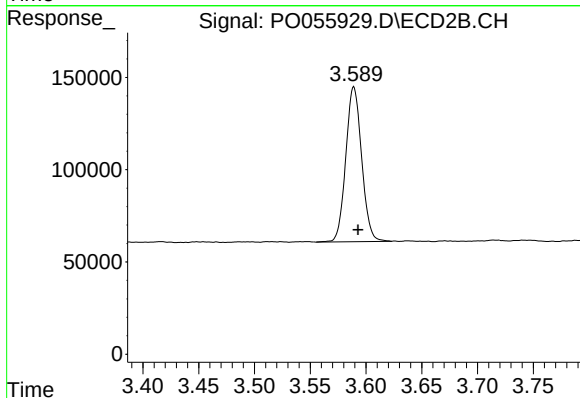


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 830198
Conc: 29.39 ng/ml

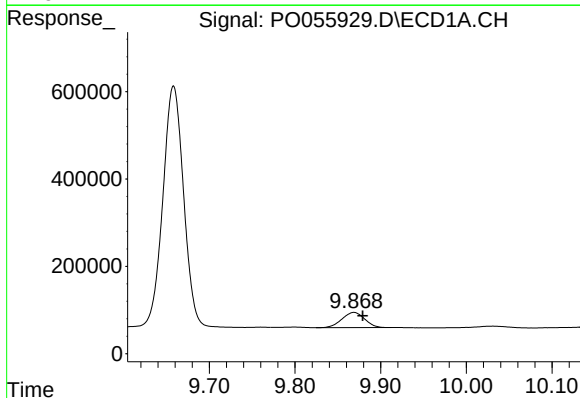

#2 Decachlorobiphenyl

R.T.: 9.869 min
Delta R.T.: -0.010 min
Response: 642608
Conc: 17.17 ng/ml

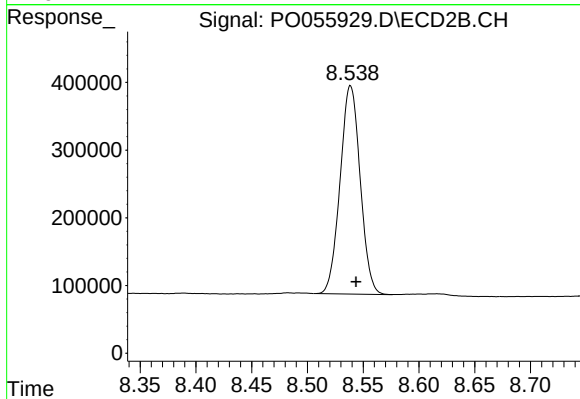

#2 Decachlorobiphenyl

R.T.: 8.538 min
Delta R.T.: -0.006 min
Response: 3857898
Conc: 142.66 ng/ml m