

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
 Data File : P0055941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 17:23
 Operator : SM/SJ
 Sample : K2673-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-12-COMP

Manual Integrations
 APPROVED

Ankita
 5/8/2019 4:16:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 04:06:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.589	859065	853283	28.707	30.212
2) SA Decachlor...	9.869	8.537	1478601	1023115	39.517	37.833m
Target Compounds						
31) L7 AR-1260-1	7.025	6.128	159659	149275	73.933	67.754
32) L7 AR-1260-2	7.278	6.314	4804276	115954	1834.473	37.973m#
33) L7 AR-1260-3	7.638	6.466	134555	125231	67.278	50.253m#
34) L7 AR-1260-4	7.861	6.934	143077	93357	61.868	45.243 #
35) L7 AR-1260-5	8.171	7.176	190557	212946	44.918	42.400m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050719\
Data File : PO055941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 17:23
Operator : SM/SJ
Sample : K2673-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-12-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 04:06:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

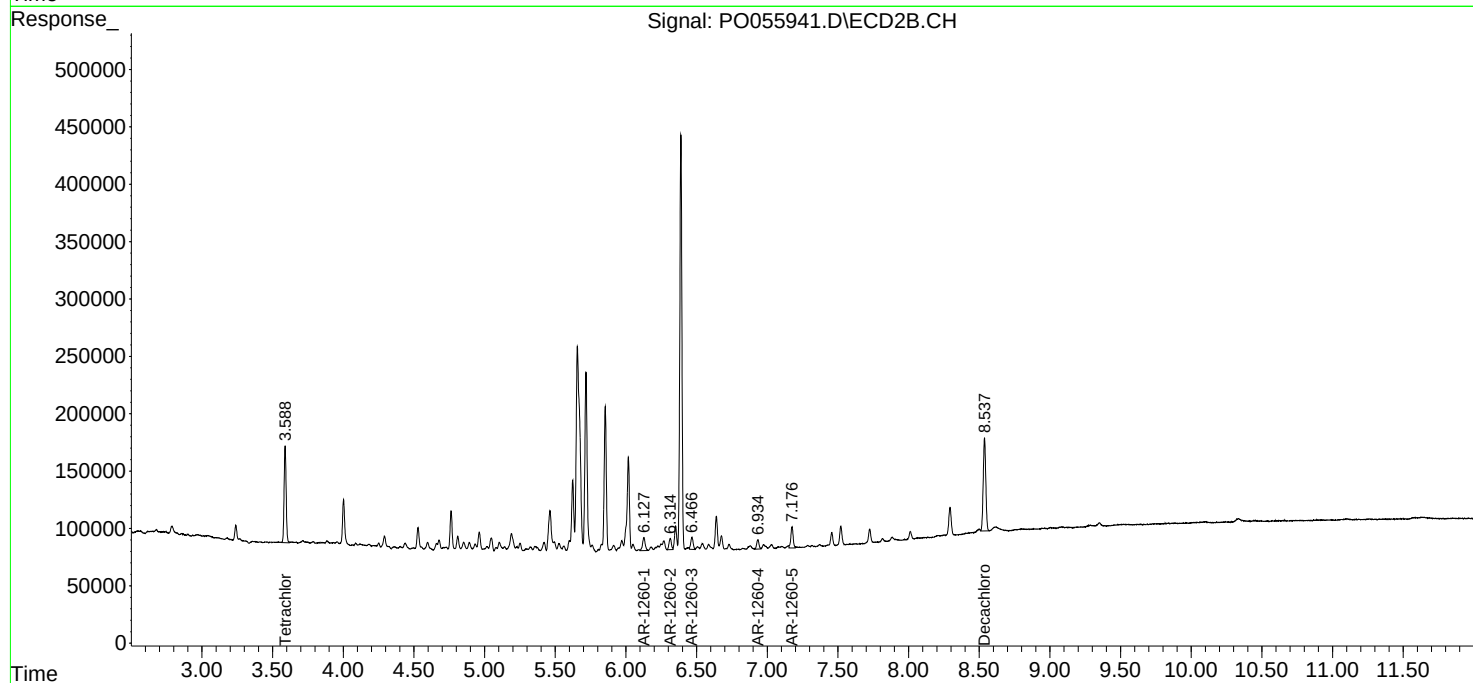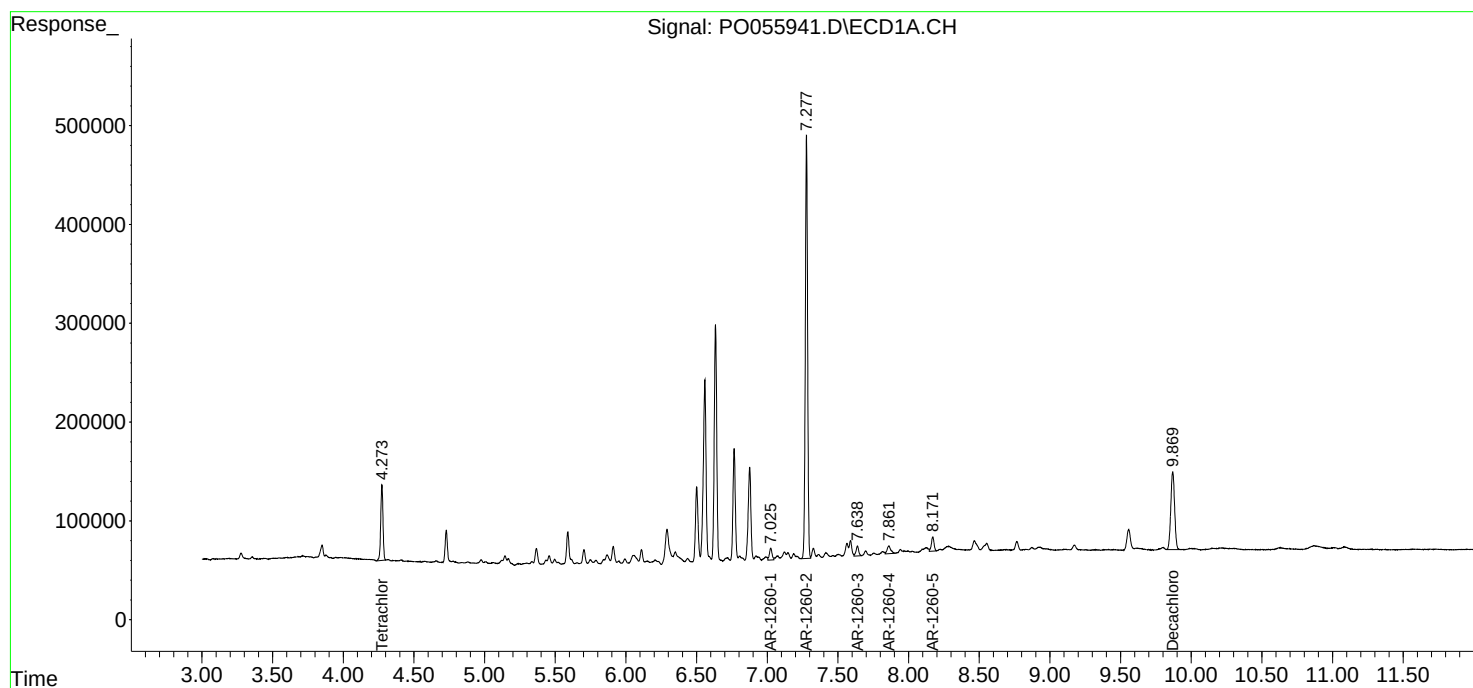

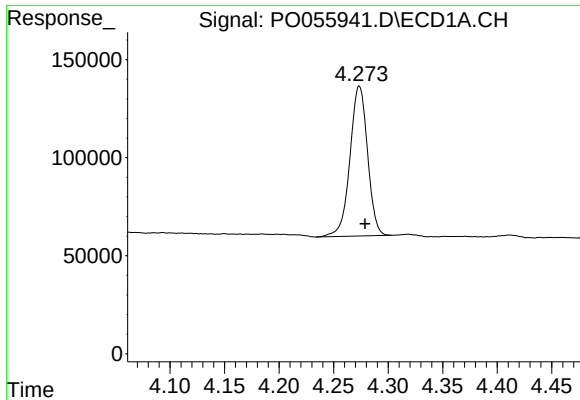


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 859065
Conc: 28.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-12-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:35 PM

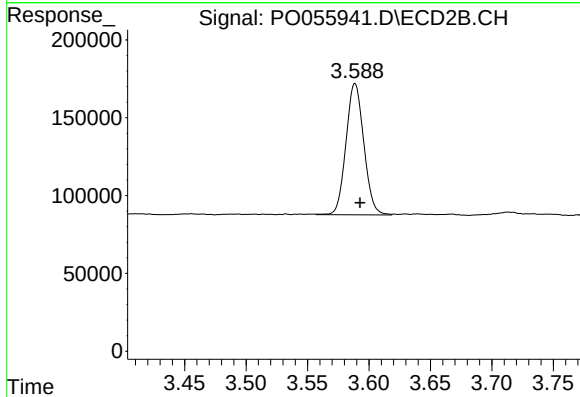


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 853283
Conc: 30.21 ng/ml

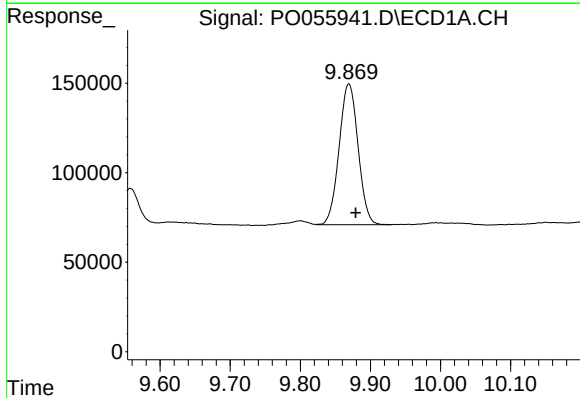


#2 Decachlorobiphenyl

R.T.: 9.869 min
Delta R.T.: -0.010 min
Response: 1478601
Conc: 39.52 ng/ml

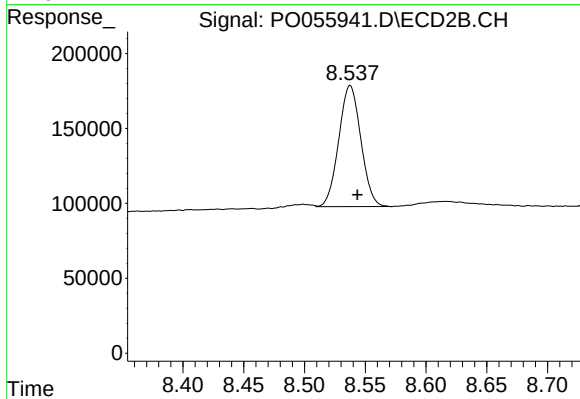

#2 Decachlorobiphenyl

R.T.: 8.537 min
Delta R.T.: -0.006 min
Response: 1023115
Conc: 37.83 ng/ml m

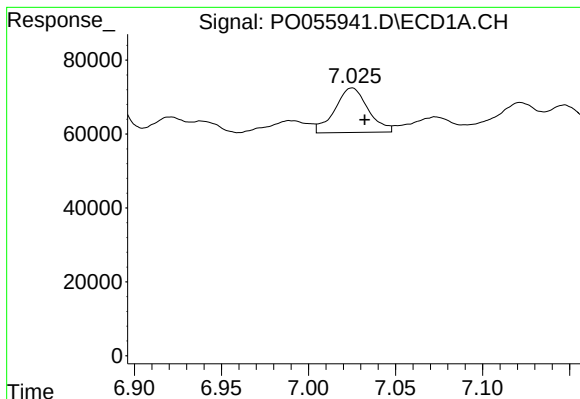


#31 AR-1260-1

R.T.: 7.025 min
Delta R.T.: -0.007 min
Response: 159659
Conc: 73.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-12-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:35 PM

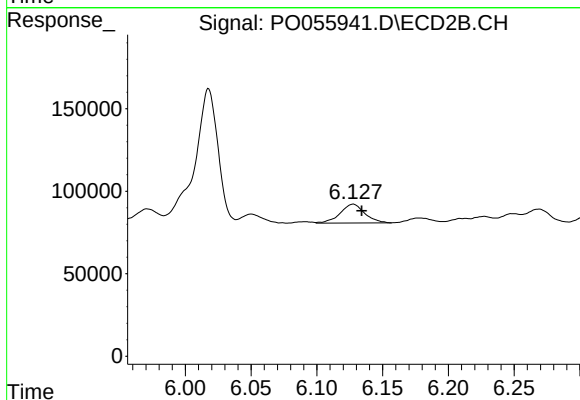


#31 AR-1260-1

R.T.: 6.128 min
Delta R.T.: -0.006 min
Response: 149275
Conc: 67.75 ng/ml

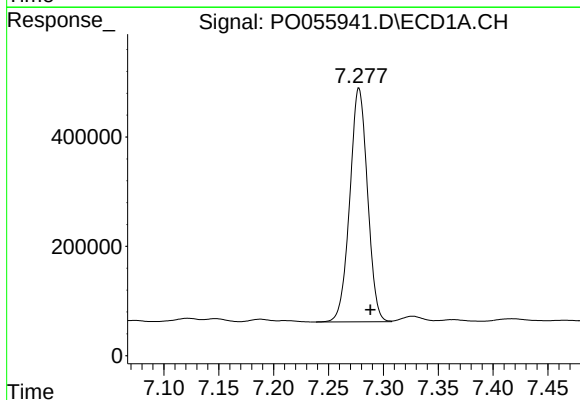


#32 AR-1260-2

R.T.: 7.278 min
Delta R.T.: -0.011 min
Response: 4804276
Conc: 1834.47 ng/ml

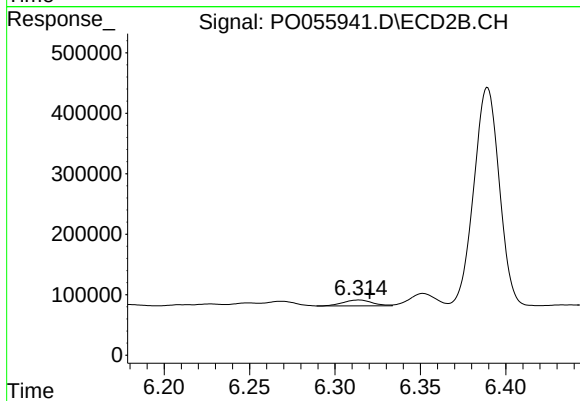

#32 AR-1260-2

R.T.: 6.314 min
Delta R.T.: -0.007 min
Response: 115954
Conc: 37.97 ng/ml m

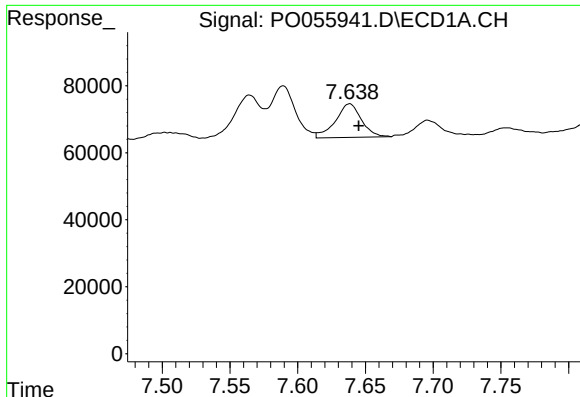


#33 AR-1260-3

R.T.: 7.638 min
Delta R.T.: -0.007 min
Response: 134555
Conc: 67.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-12-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:35 PM

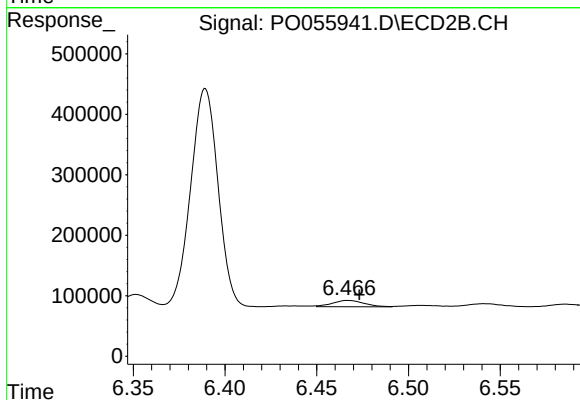


#33 AR-1260-3

R.T.: 6.466 min
Delta R.T.: -0.007 min
Response: 125231
Conc: 50.25 ng/ml m

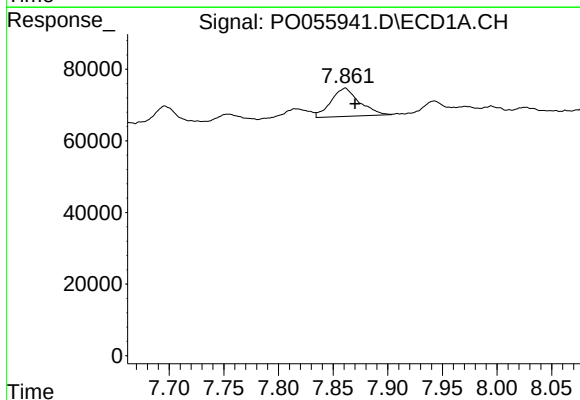


#34 AR-1260-4

R.T.: 7.861 min
Delta R.T.: -0.009 min
Response: 143077
Conc: 61.87 ng/ml

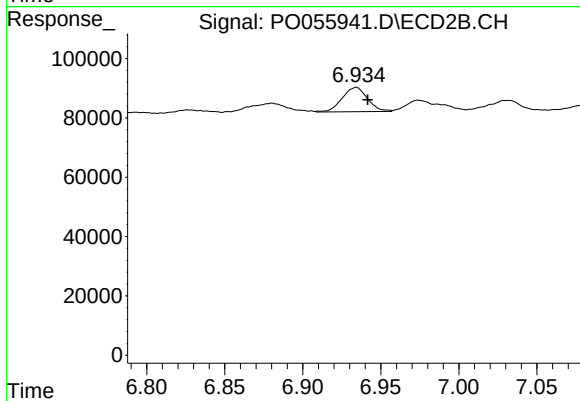

#34 AR-1260-4

R.T.: 6.934 min
Delta R.T.: -0.007 min
Response: 93357
Conc: 45.24 ng/ml

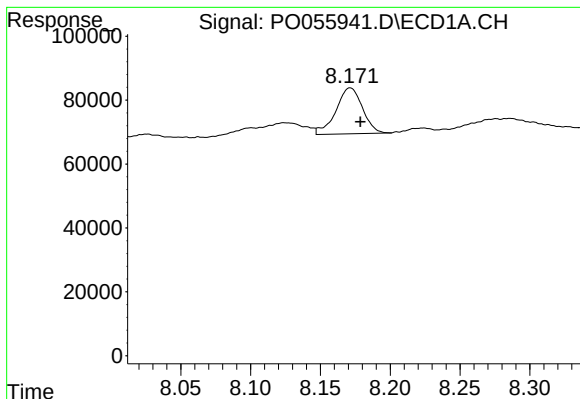


#35 AR-1260-5

R.T.: 8.171 min
Delta R.T.: -0.007 min
Response: 190557
Conc: 44.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-12-COMP

Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:35 PM

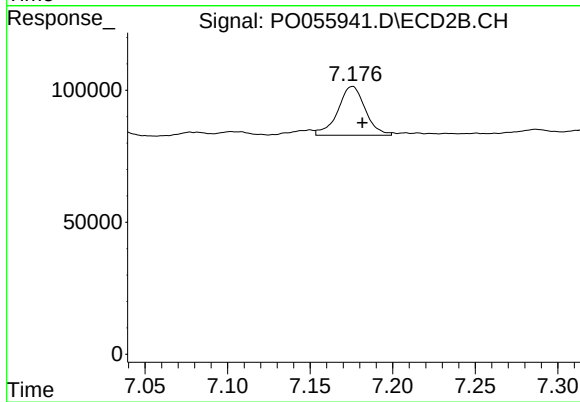

#35 AR-1260-5

R.T.: 7.176 min
Delta R.T.: -0.006 min
Response: 212946
Conc: 42.40 ng/ml m