

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0050719\
 Data File : P0055945.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 18:30
 Operator : SM/SJ
 Sample : K2673-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SB-14-COMP

Manual Integrations
 APPROVED

Ankita
 5/8/2019 4:16:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 04:08:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.273	3.589	989881	1041937	33.078m	36.891m
2) SA Decachlor...	9.868	8.535	723136	534916	19.326	19.780m
Target Compounds						
31) L7 AR-1260-1	7.024	6.126	107219	152541	49.650	69.237m#
32) L7 AR-1260-2	7.278	6.314	4556396	129680	1739.822	42.468m#
33) L7 AR-1260-3	7.637	6.466	73751	110481	36.875	44.334m
34) L7 AR-1260-4	7.860	6.933	100953	57415	43.653	27.825 #
35) L7 AR-1260-5	8.171	7.174	106217	144262	25.037	28.724m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
Data File : P0055945.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 18:30
Operator : SM/SJ
Sample : K2673-08
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-14-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 04:08:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

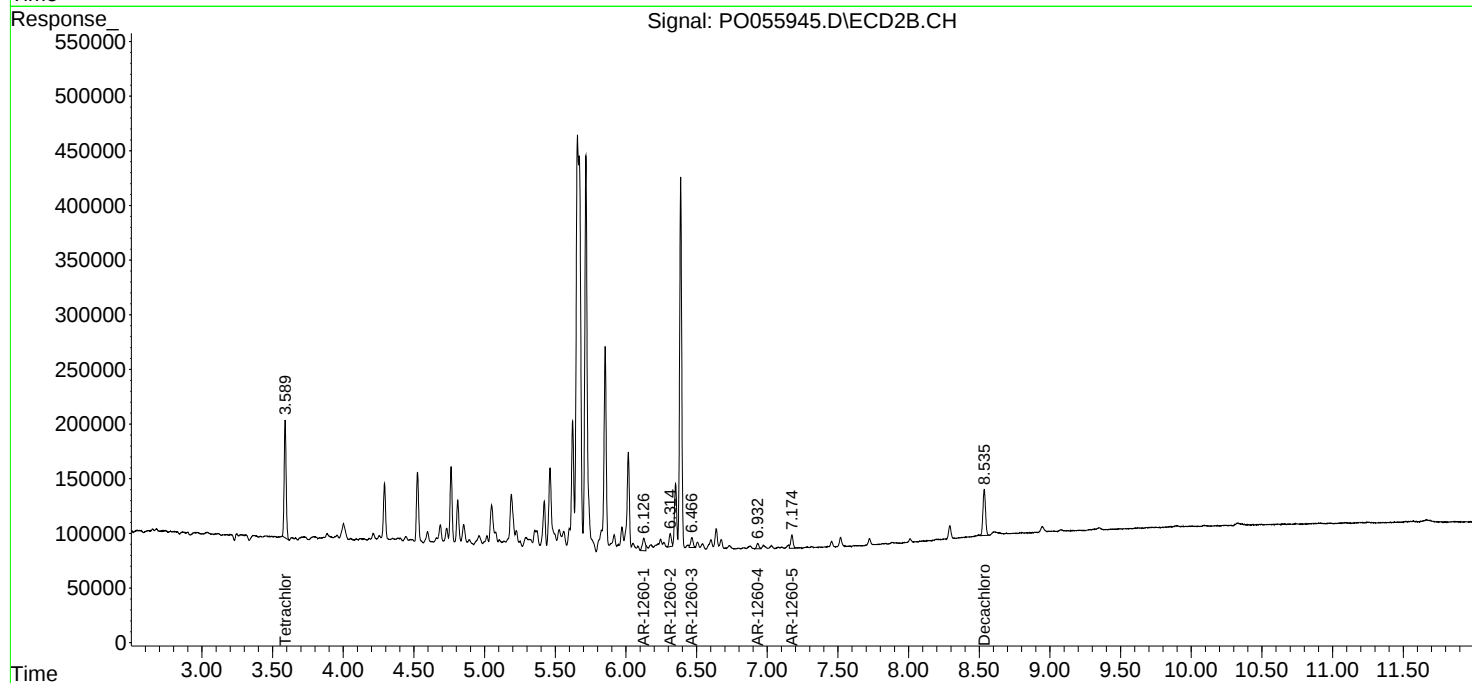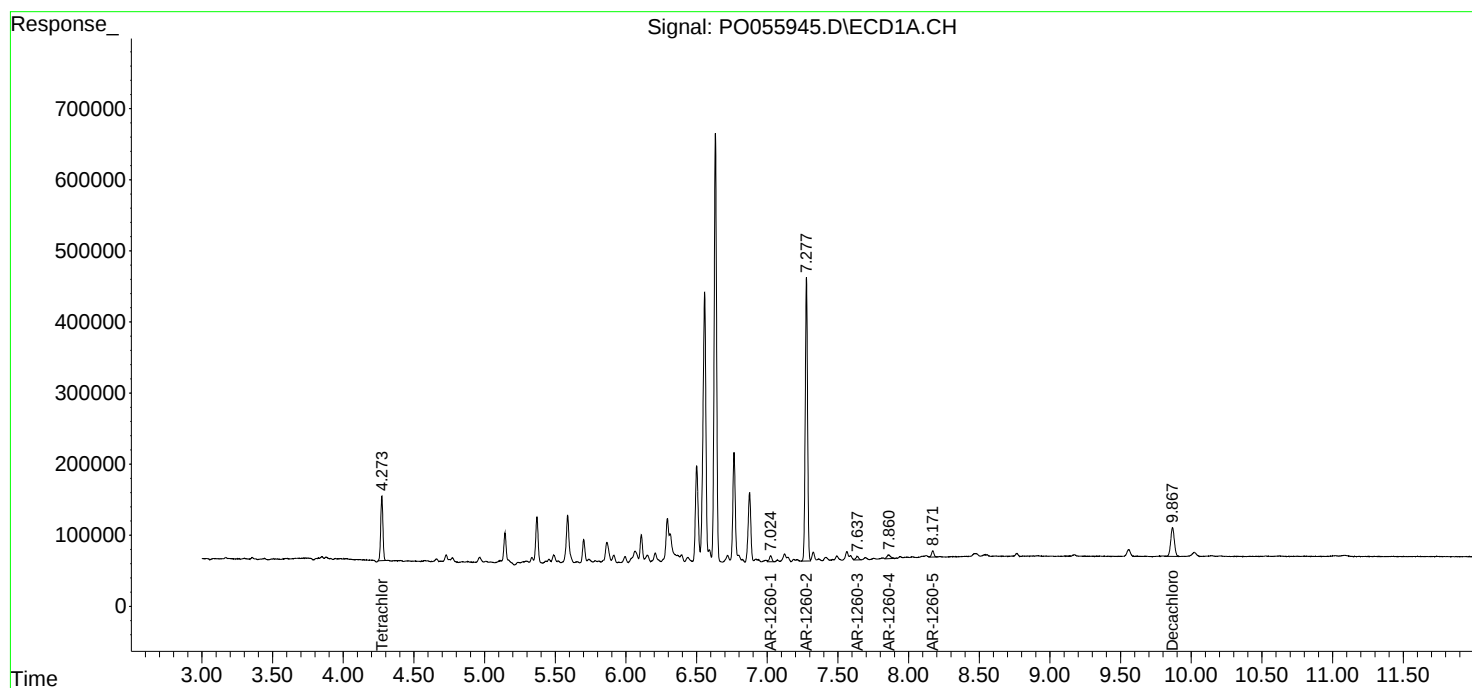

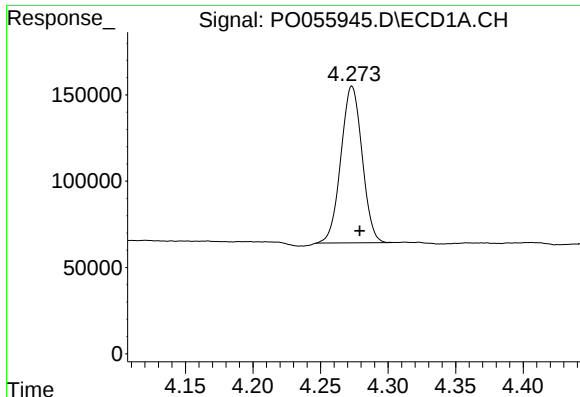


#1 Tetrachloro-m-xylene

R.T.: 4.273 min
Delta R.T.: -0.006 min
Response: 989881
Conc: 33.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-14-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:43 PM

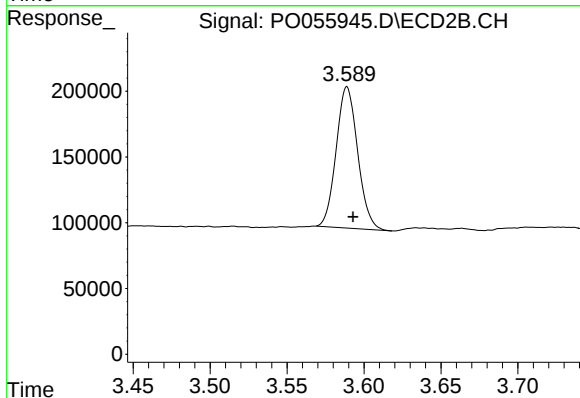


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 1041937
Conc: 36.89 ng/ml m

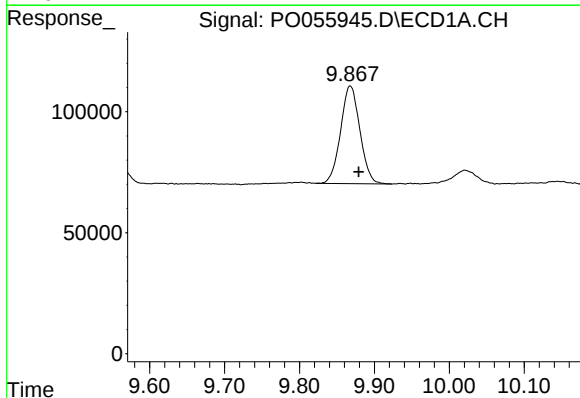


#2 Decachlorobiphenyl

R.T.: 9.868 min
Delta R.T.: -0.011 min
Response: 723136
Conc: 19.33 ng/ml

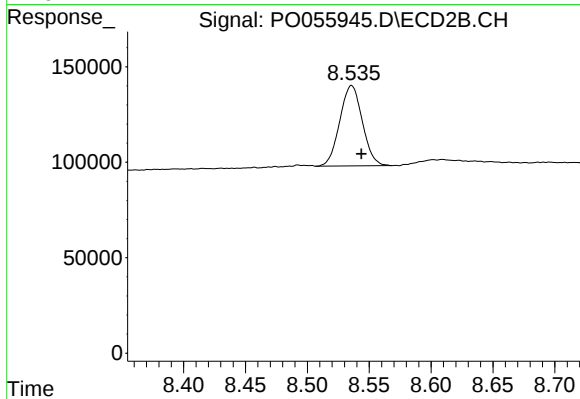

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.008 min
Response: 534916
Conc: 19.78 ng/ml m

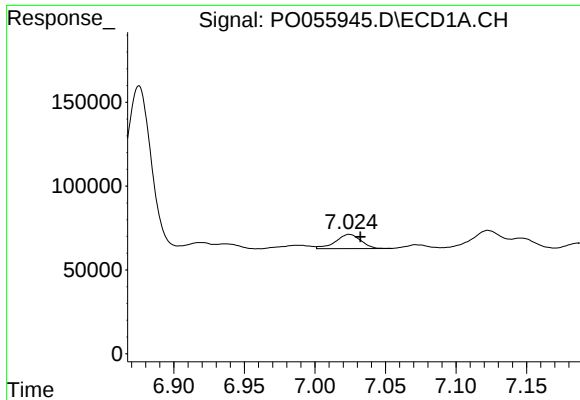


#31 AR-1260-1

R.T.: 7.024 min
Delta R.T.: -0.008 min
Response: 107219
Conc: 49.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-14-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:43 PM

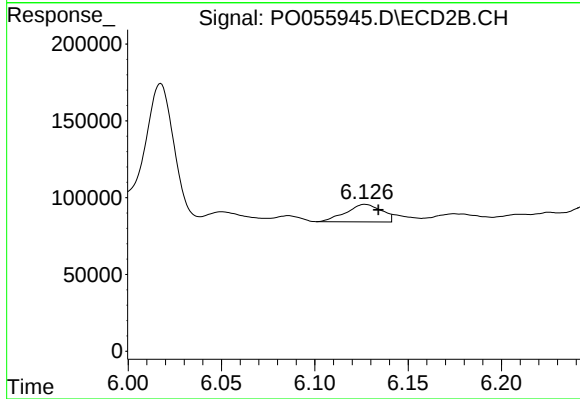


#31 AR-1260-1

R.T.: 6.126 min
Delta R.T.: -0.008 min
Response: 152541
Conc: 69.24 ng/ml m

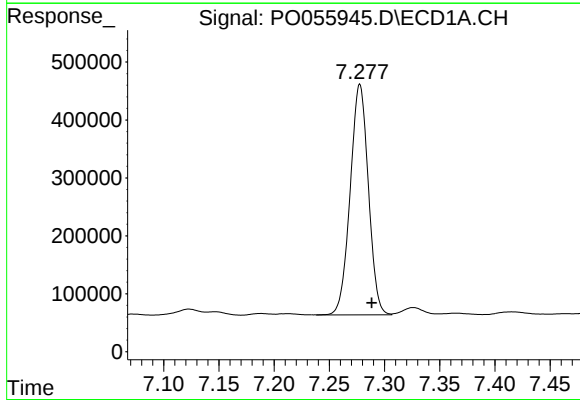


#32 AR-1260-2

R.T.: 7.278 min
Delta R.T.: -0.011 min
Response: 4556396
Conc: 1739.82 ng/ml

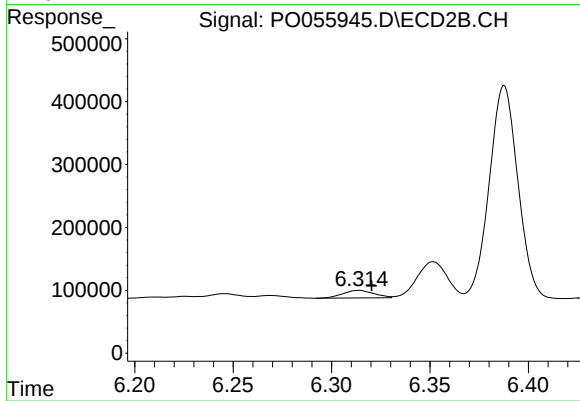

#32 AR-1260-2

R.T.: 6.314 min
Delta R.T.: -0.007 min
Response: 129680
Conc: 42.47 ng/ml m

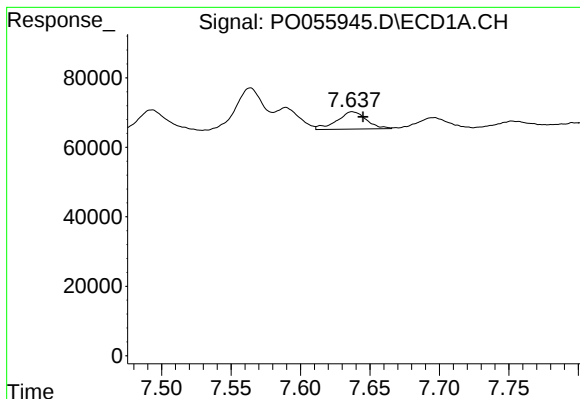


#33 AR-1260-3

R.T.: 7.637 min
Delta R.T.: -0.008 min
Response: 73751
Conc: 36.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-14-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:43 PM

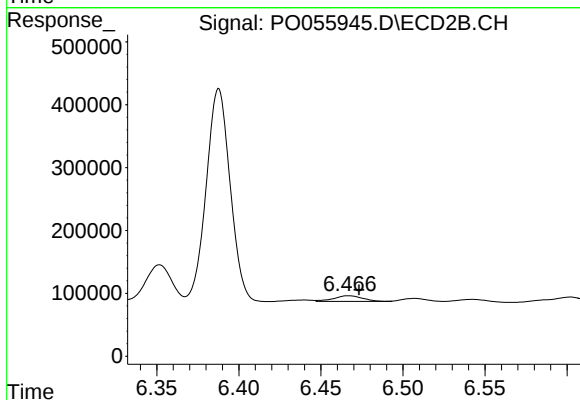


#33 AR-1260-3

R.T.: 6.466 min
Delta R.T.: -0.007 min
Response: 110481
Conc: 44.33 ng/ml m

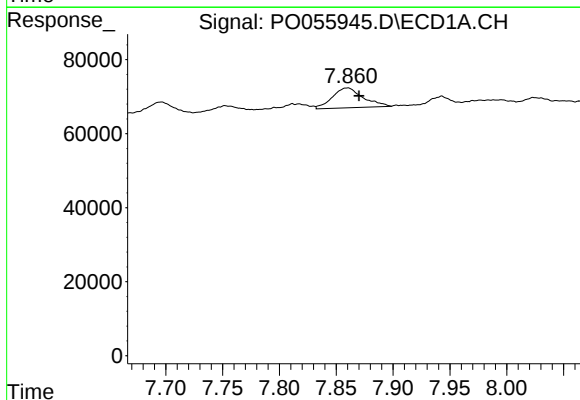


#34 AR-1260-4

R.T.: 7.860 min
Delta R.T.: -0.010 min
Response: 100953
Conc: 43.65 ng/ml

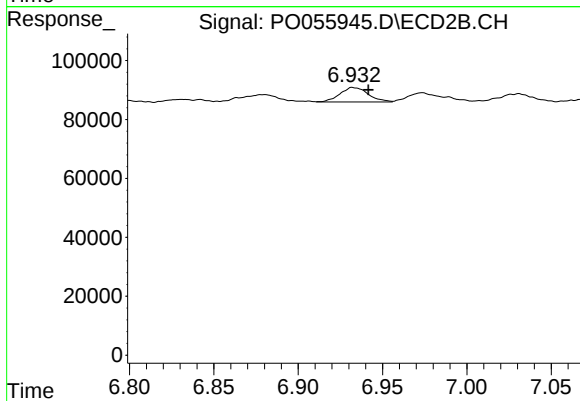

#34 AR-1260-4

R.T.: 6.933 min
Delta R.T.: -0.009 min
Response: 57415
Conc: 27.82 ng/ml

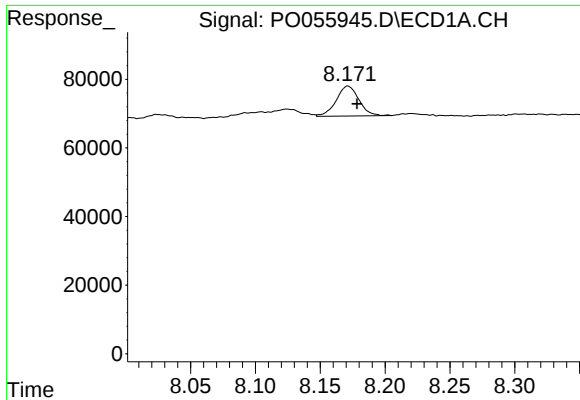


#35 AR-1260-5

R.T.: 8.171 min
Delta R.T.: -0.007 min
Response: 106217
Conc: 25.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-14-COMP

Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:43 PM

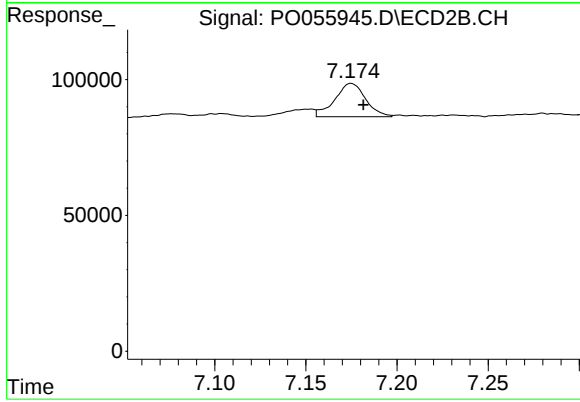

#35 AR-1260-5

R.T.: 7.174 min
Delta R.T.: -0.007 min
Response: 144262
Conc: 28.72 ng/ml m