

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0050719\
 Data File : P0055949.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 19:38
 Operator : SM/SJ
 Sample : K2673-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SP-01-COMP

Manual Integrations
 APPROVED

Ankita
 5/8/2019 4:16:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 04:11:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.273	3.589	891735	1004539	29.798	35.567
2) SA Decachlor...	9.867	8.535	553264	406677	14.786	15.038m
Target Compounds						
31) L7 AR-1260-1	7.024	6.126	157509	209299	72.938	94.998m#
32) L7 AR-1260-2	7.277	6.314	319797	109557	122.112	35.878m#
33) L7 AR-1260-3	7.637	6.466	155731	129843	77.866	52.104m#
34) L7 AR-1260-4	7.861	6.933	192474	114064	83.228m	55.278 #
35) L7 AR-1260-5	8.170	7.175	266688	318113	62.864	63.340

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
Data File : P0055949.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 19:38
Operator : SM/SJ
Sample : K2673-15
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SP-01-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 04:11:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

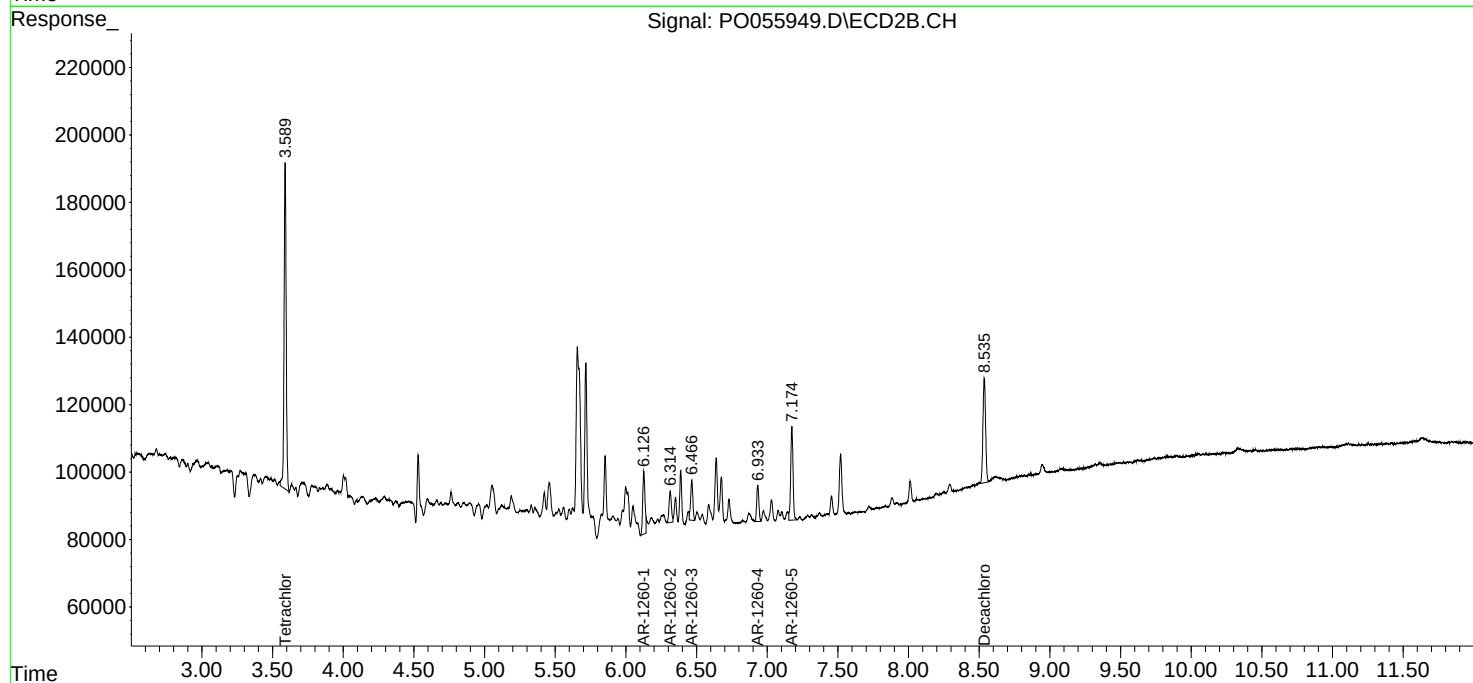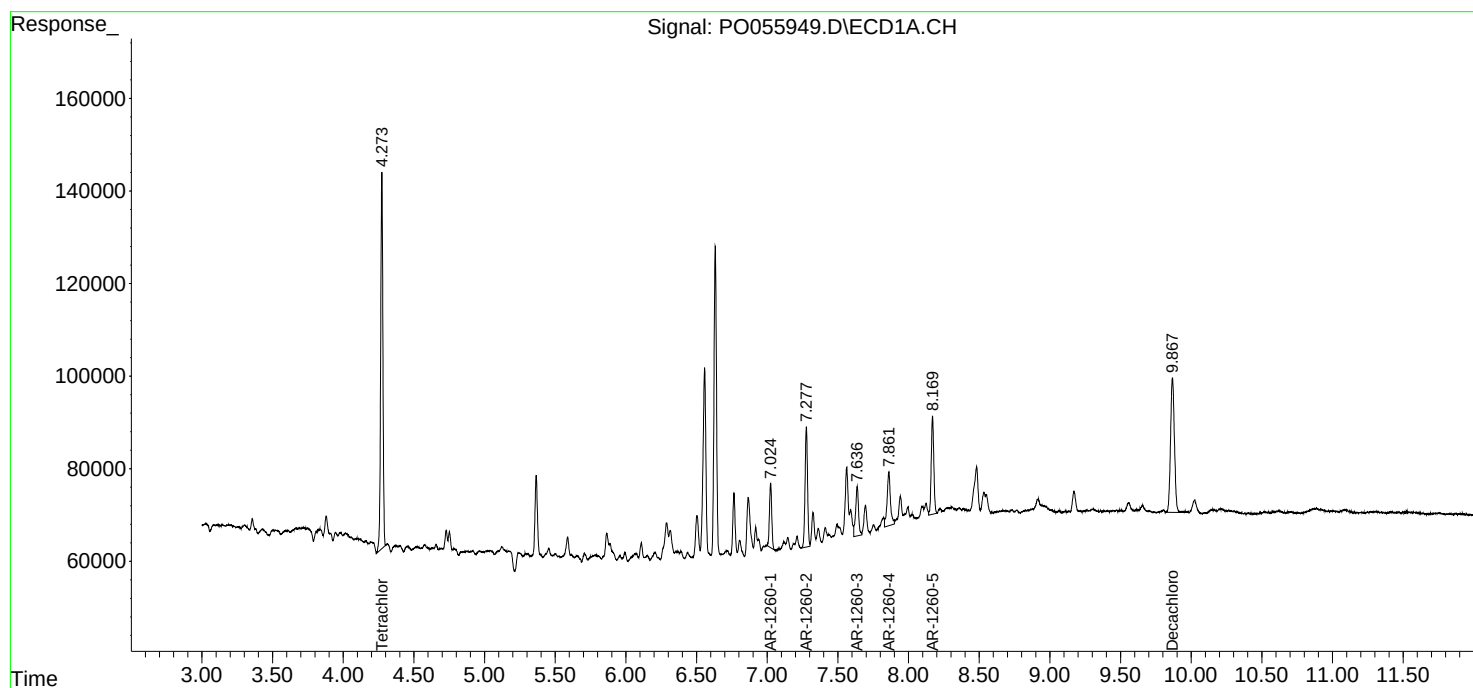

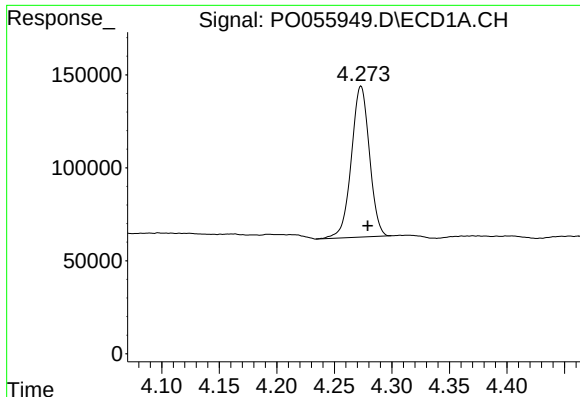


#1 Tetrachloro-m-xylene

R.T.: 4.273 min
Delta R.T.: -0.006 min
Response: 891735
Conc: 29.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-01-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:50 PM

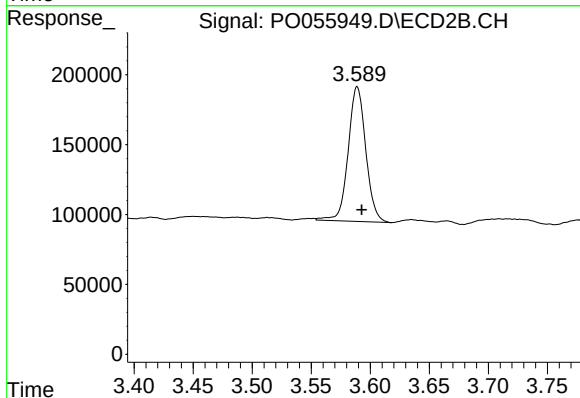


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 1004539
Conc: 35.57 ng/ml

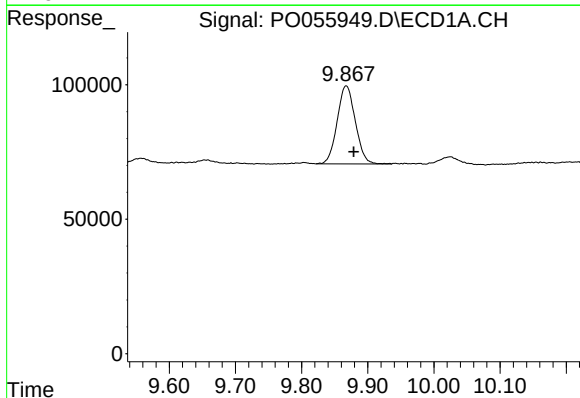


#2 Decachlorobiphenyl

R.T.: 9.867 min
Delta R.T.: -0.011 min
Response: 553264
Conc: 14.79 ng/ml

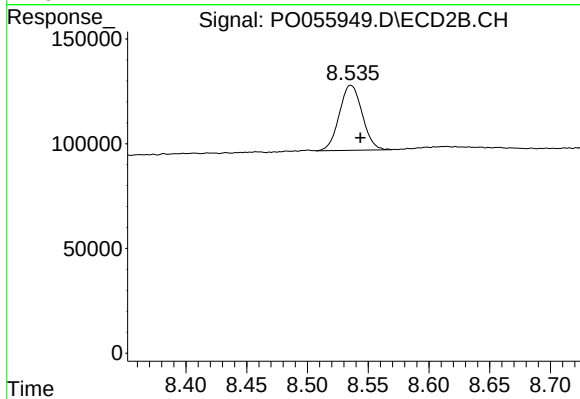

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.008 min
Response: 406677
Conc: 15.04 ng/ml m

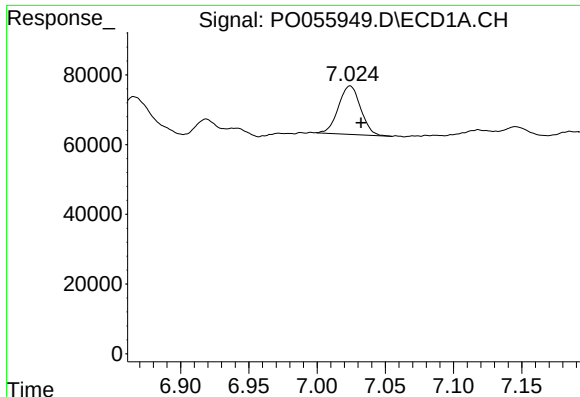


#31 AR-1260-1

R.T.: 7.024 min
Delta R.T.: -0.008 min
Response: 157509
Conc: 72.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-01-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:50 PM

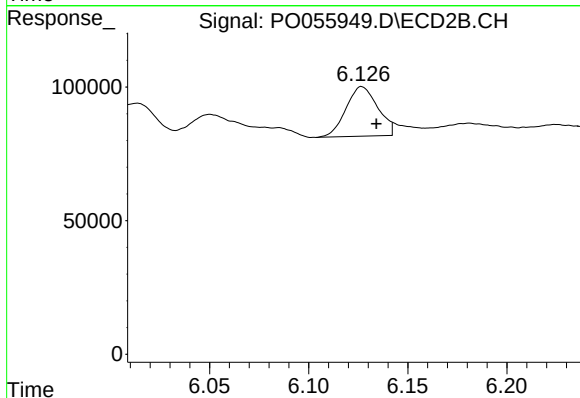


#31 AR-1260-1

R.T.: 6.126 min
Delta R.T.: -0.008 min
Response: 209299
Conc: 95.00 ng/ml m

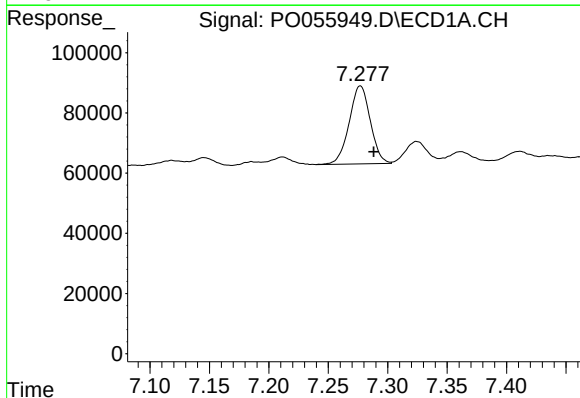


#32 AR-1260-2

R.T.: 7.277 min
Delta R.T.: -0.011 min
Response: 319797
Conc: 122.11 ng/ml

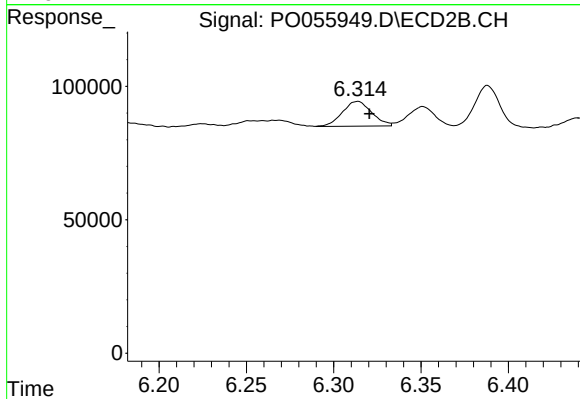

#32 AR-1260-2

R.T.: 6.314 min
Delta R.T.: -0.007 min
Response: 109557
Conc: 35.88 ng/ml m

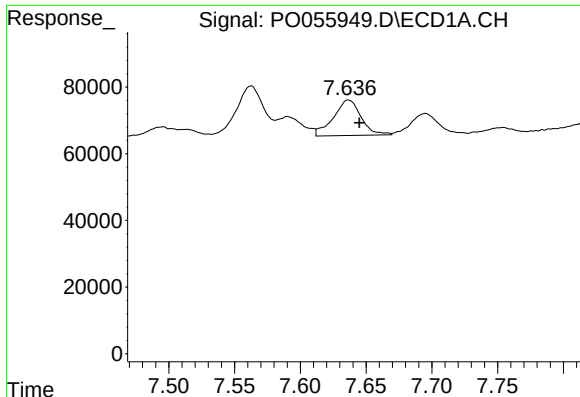


#33 AR-1260-3

R.T.: 7.637 min
Delta R.T.: -0.008 min
Response: 155731
Conc: 77.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-01-COMP


Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:50 PM

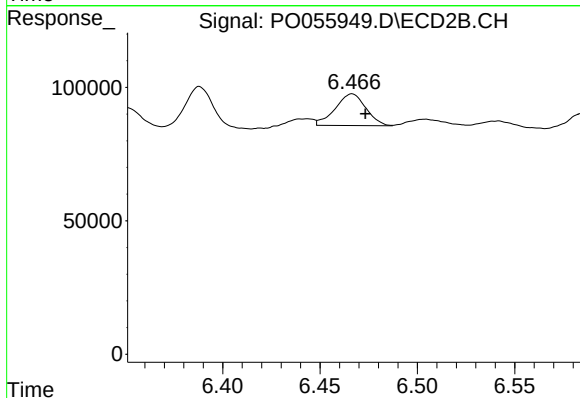


#33 AR-1260-3

R.T.: 6.466 min
Delta R.T.: -0.007 min
Response: 129843
Conc: 52.10 ng/ml m

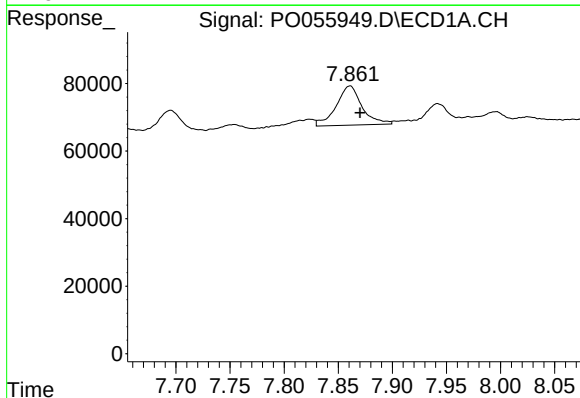


#34 AR-1260-4

R.T.: 7.861 min
Delta R.T.: -0.009 min
Response: 192474
Conc: 83.23 ng/ml m

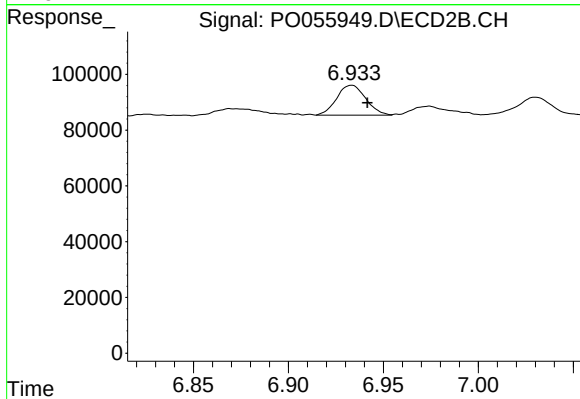

#34 AR-1260-4

R.T.: 6.933 min
Delta R.T.: -0.008 min
Response: 114064
Conc: 55.28 ng/ml

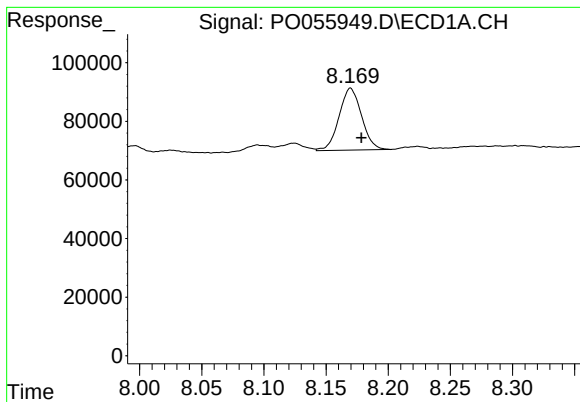


#35 AR-1260-5

R.T.: 8.170 min
Delta R.T.: -0.009 min
Response: 266688
Conc: 62.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-01-COMP

Manual Integrations
APPROVED

Ankita
5/8/2019 4:16:50 PM

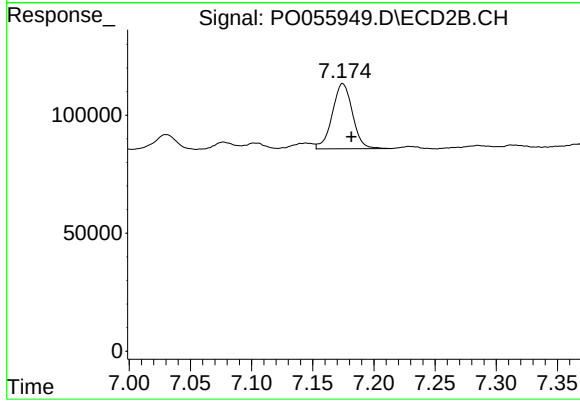

#35 AR-1260-5

R.T.: 7.175 min
Delta R.T.: -0.007 min
Response: 318113
Conc: 63.34 ng/ml