

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
 Data File : P0055957.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2019 21:54
 Operator : SM/SJ
 Sample : K2675-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OUTFALL001-WK-1

Manual Integrations
 APPROVED

Ankita
 5/8/2019 4:17:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 04:19:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.589	1137329	1139899	38.005	40.360
2) SA Decachlor...	9.866	8.535	718518	566859	19.203m	20.961

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050719\
Data File : P0055957.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2019 21:54
Operator : SM/SJ
Sample : K2675-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OUTFALL001-WK-1


Manual Integrations
APPROVED

Ankita
5/8/2019 4:17:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 04:19:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

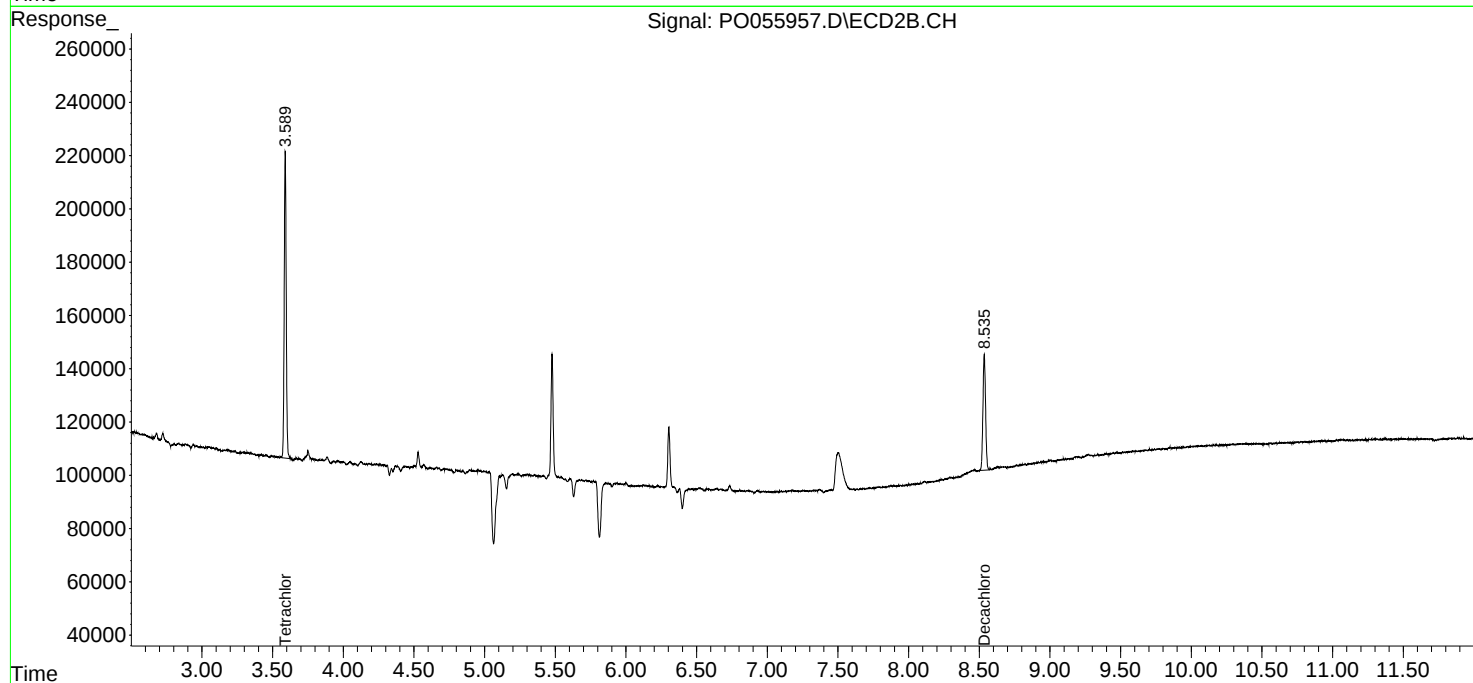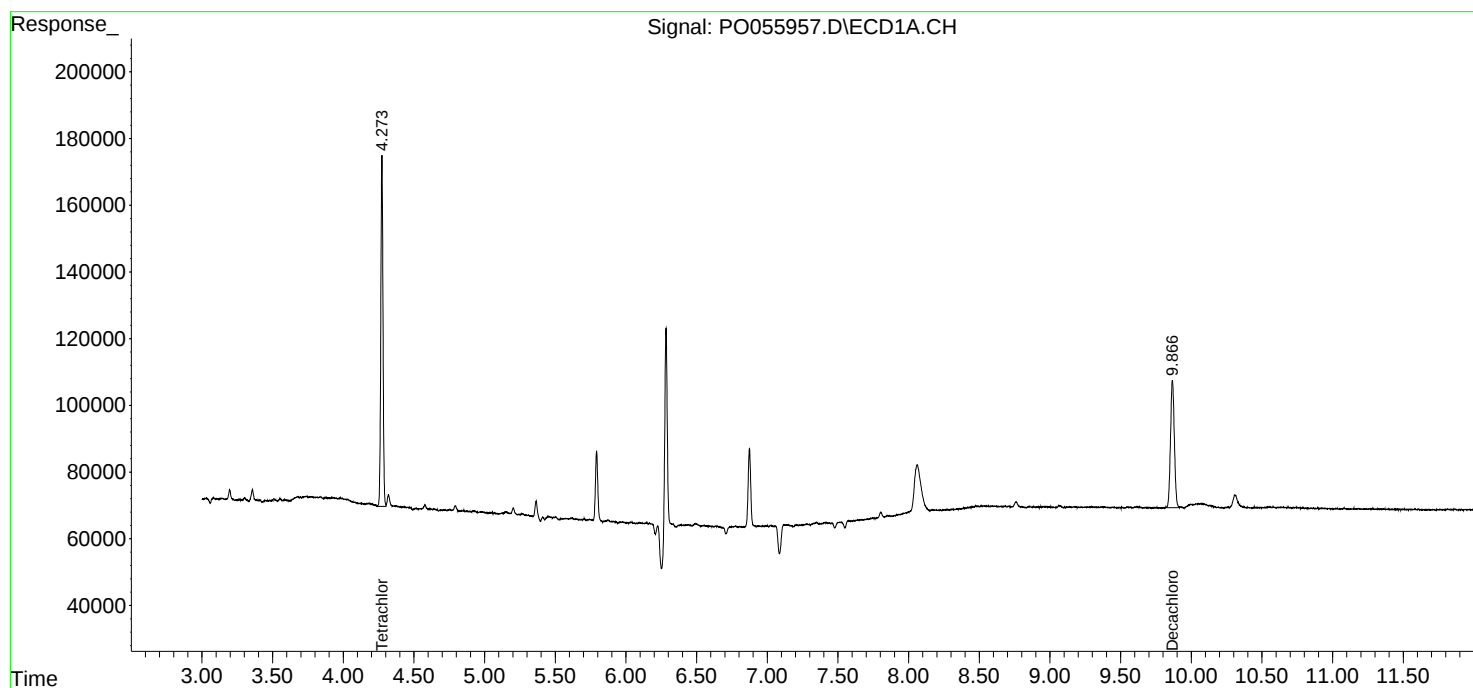

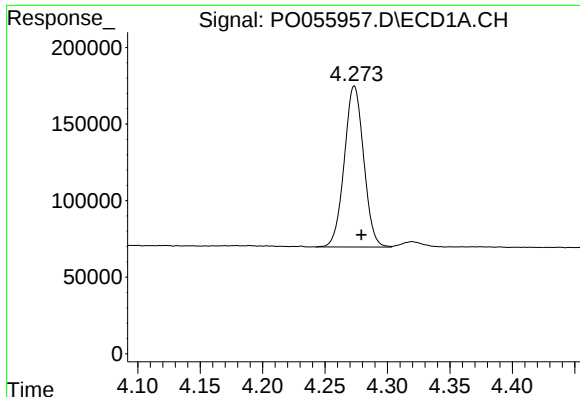


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 1137329
Conc: 38.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
OUTFALL001-WK-1


Manual Integrations
APPROVED

Ankita
5/8/2019 4:17:12 PM

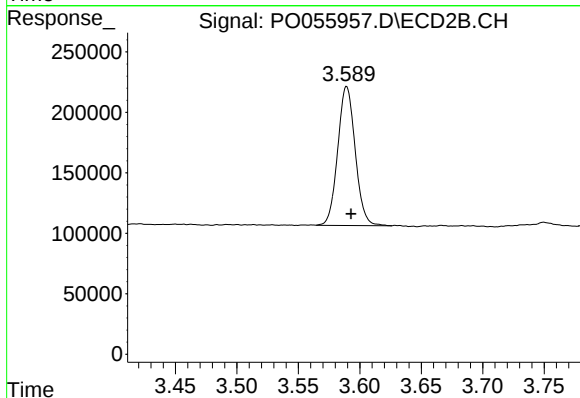


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 1139899
Conc: 40.36 ng/ml

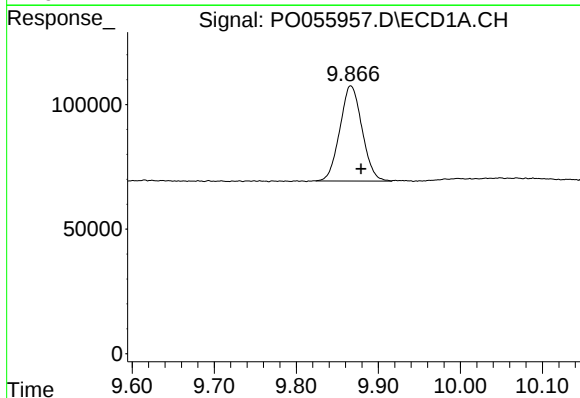

#2 Decachlorobiphenyl

R.T.: 9.866 min
Delta R.T.: -0.013 min
Response: 718518
Conc: 19.20 ng/ml m

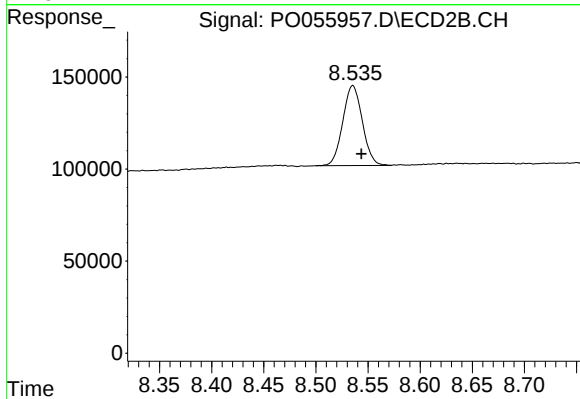

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.008 min
Response: 566859
Conc: 20.96 ng/ml