

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050720\
 Data File : P0068213.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 May 2020 14:21
 Operator : DD\AJ
 Sample : L2498-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-050620

Manual Integrations
 APPROVED

Sohil
 5/8/2020 7:55:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 15:16:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 28 07:12:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.909	3.934	789193	1004602	32.979m	31.438m
2) SA Decachlor...	10.873	9.211	1011547	934348	26.804m	24.209

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050720\
Data File : P0068213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 May 2020 14:21
Operator : DD\AJ
Sample : L2498-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-050620


Manual Integrations
APPROVED

Sohil
5/8/2020 7:55:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 15:16:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 28 07:12:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

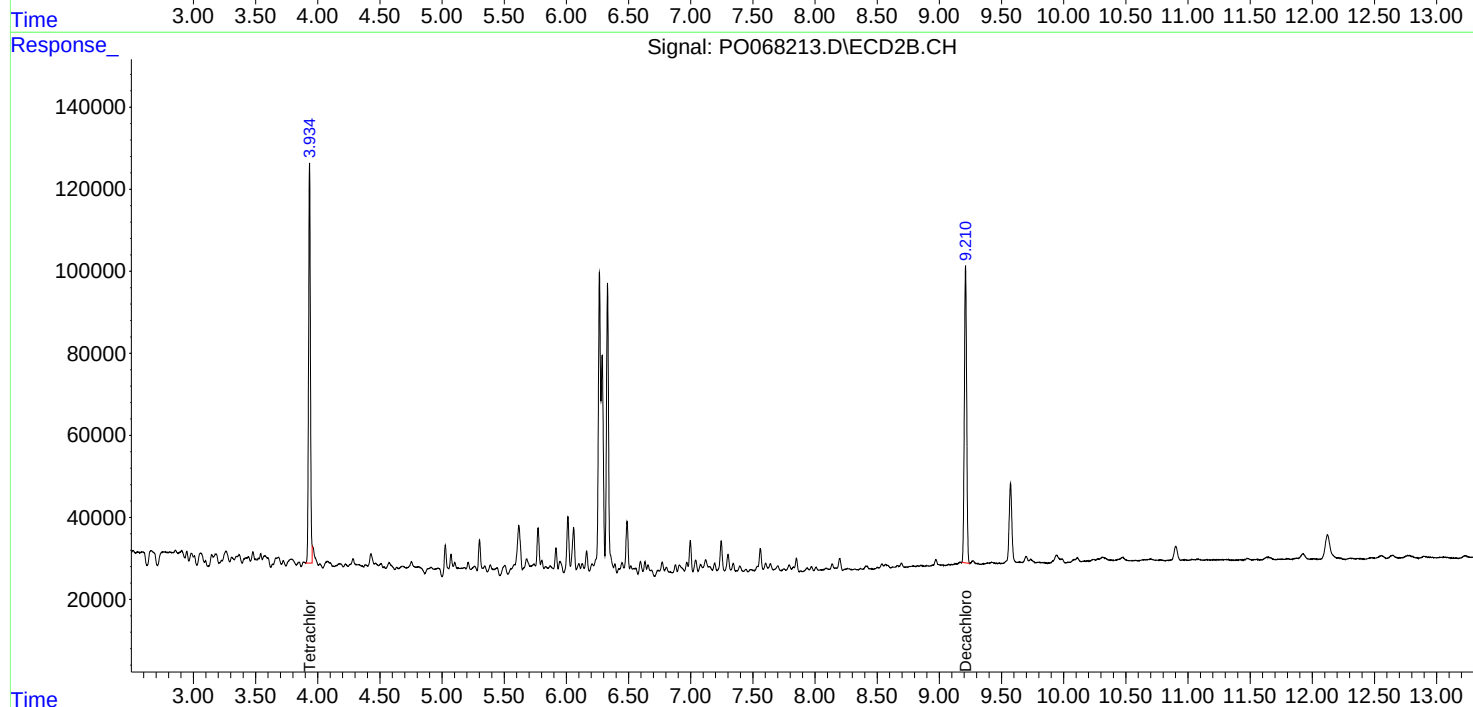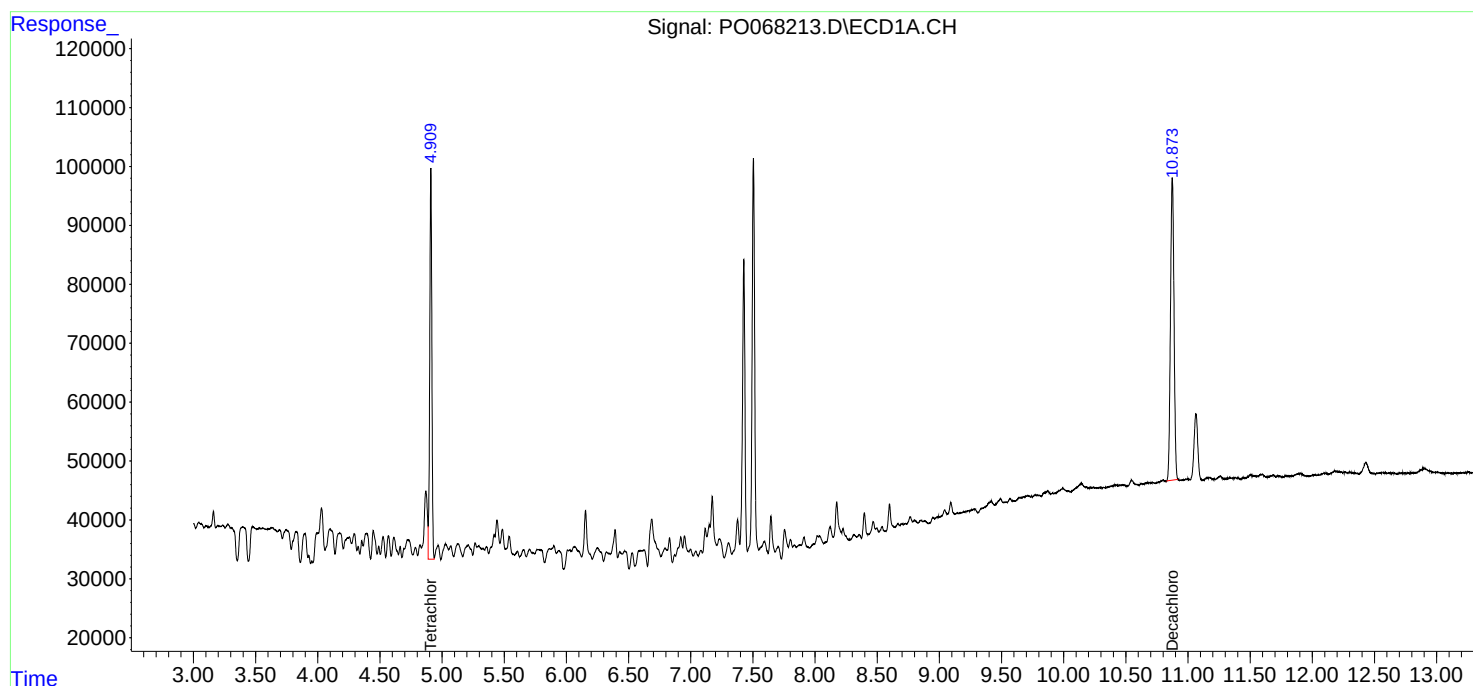

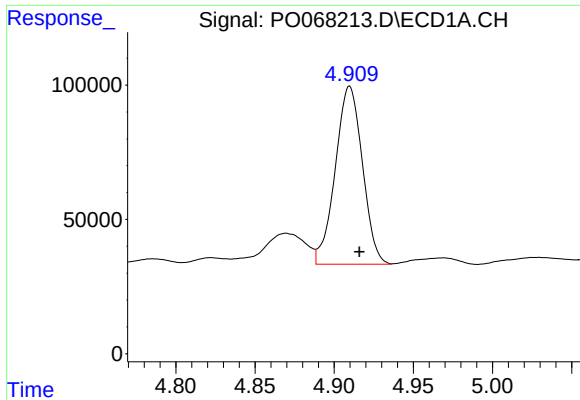


#1 Tetrachloro-m-xylene

R.T.: 4.909 min
Delta R.T.: -0.007 min
Response: 789193
Conc: 32.98 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-02-050620


Manual Integrations
APPROVED

Sohil
5/8/2020 7:55:20 AM

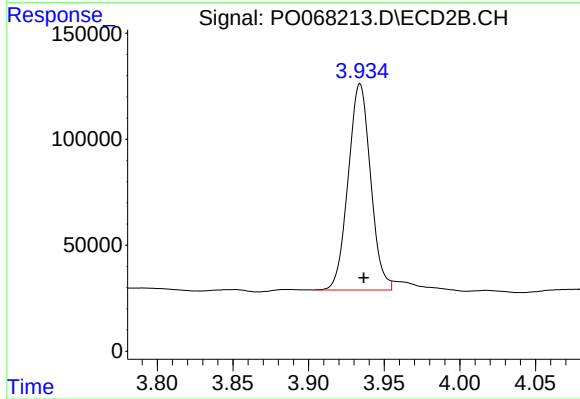


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.003 min
Response: 1004602
Conc: 31.44 ng/ml m

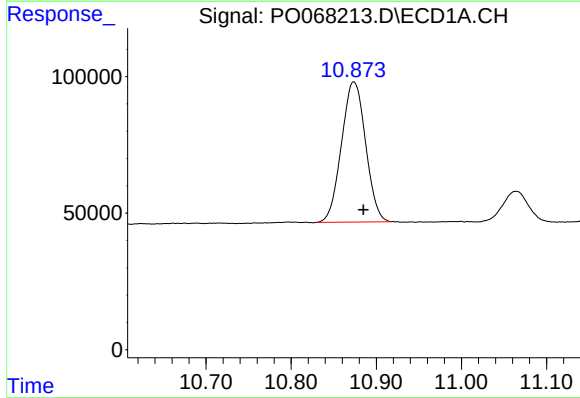

#2 Decachlorobiphenyl

R.T.: 10.873 min
Delta R.T.: -0.012 min
Response: 1011547
Conc: 26.80 ng/ml m

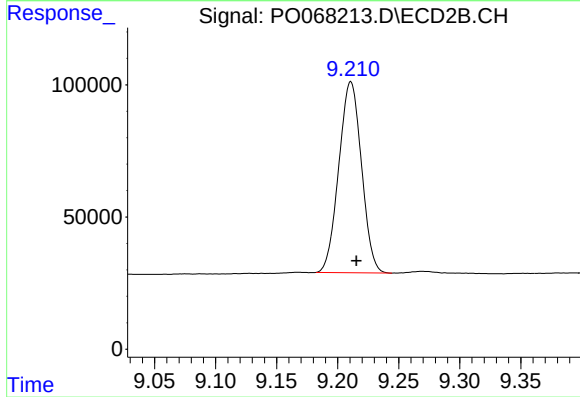

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.005 min
Response: 934348
Conc: 24.21 ng/ml