

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0050819\
 Data File : P0055966.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 May 2019 11:20
 Operator : SM/SJ
 Sample : K2639-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 NB-08-050319-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 11:40:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.272	3.587	726583	759473	24.280	26.890
2)	SA Decachlor...	9.865	8.533	633423	461853	16.929	17.078
Target Compounds							
20)	L4 AR-1242-5	0.000	5.452	0	13321	N.D.	11.097 #
25)	L5 AR-1248-5	0.000	5.452	0	13321	N.D.	8.894 #
26)	L6 AR-1254-1	0.000	5.452	0	13321	N.D.	4.977 #
27)	L6 AR-1254-2	6.498	5.653	29449	23100	8.873	9.457
28)	L6 AR-1254-3	6.871	5.995	56076	20070	15.424	5.058 #
30)	L6 AR-1254-5	0.000	6.639	0	16514	N.D.	4.564 #
31)	L7 AR-1260-1	0.000	6.131	0	10017	N.D.	4.547 #
36)	L8 AR-1262-1	0.000	6.639	0	16514	N.D.	4.027 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050819\
Data File : PO055966.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2019 11:20
Operator : SM/SJ
Sample : K2639-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NB-08-050319-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 11:40:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

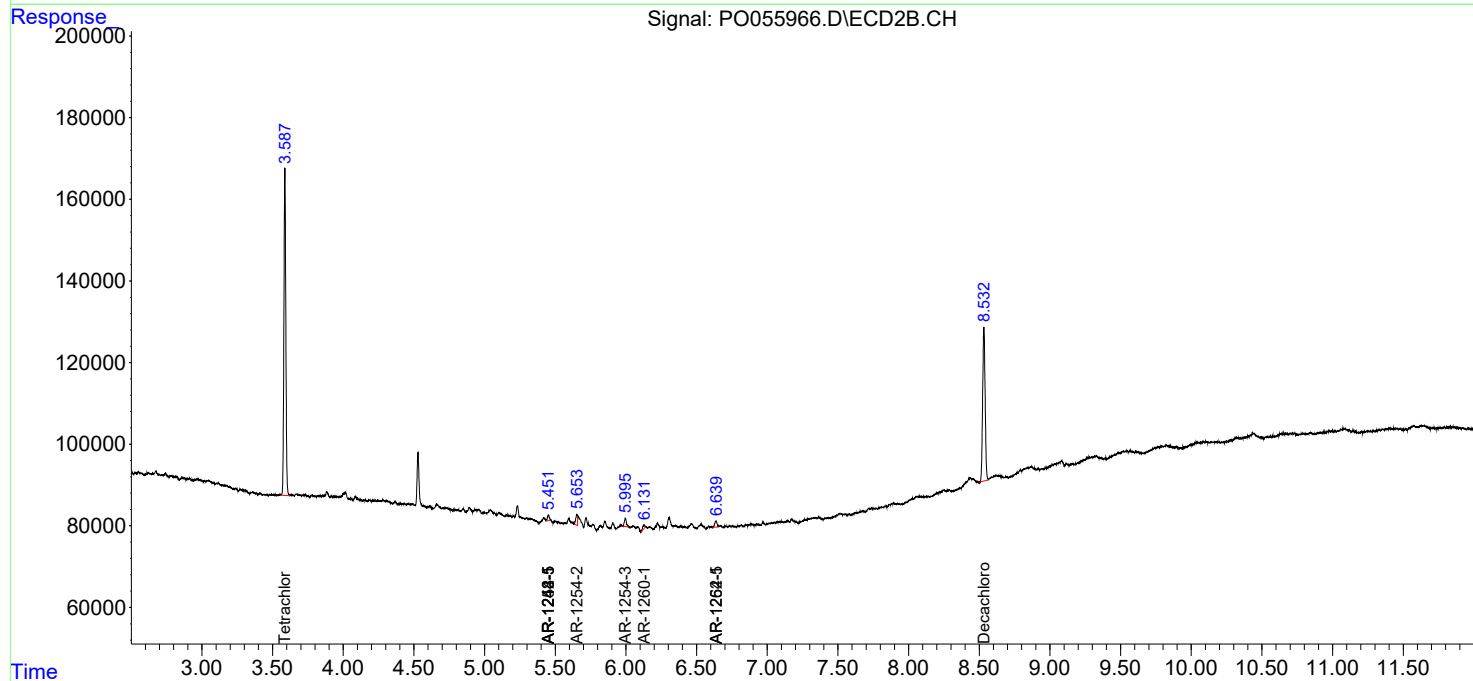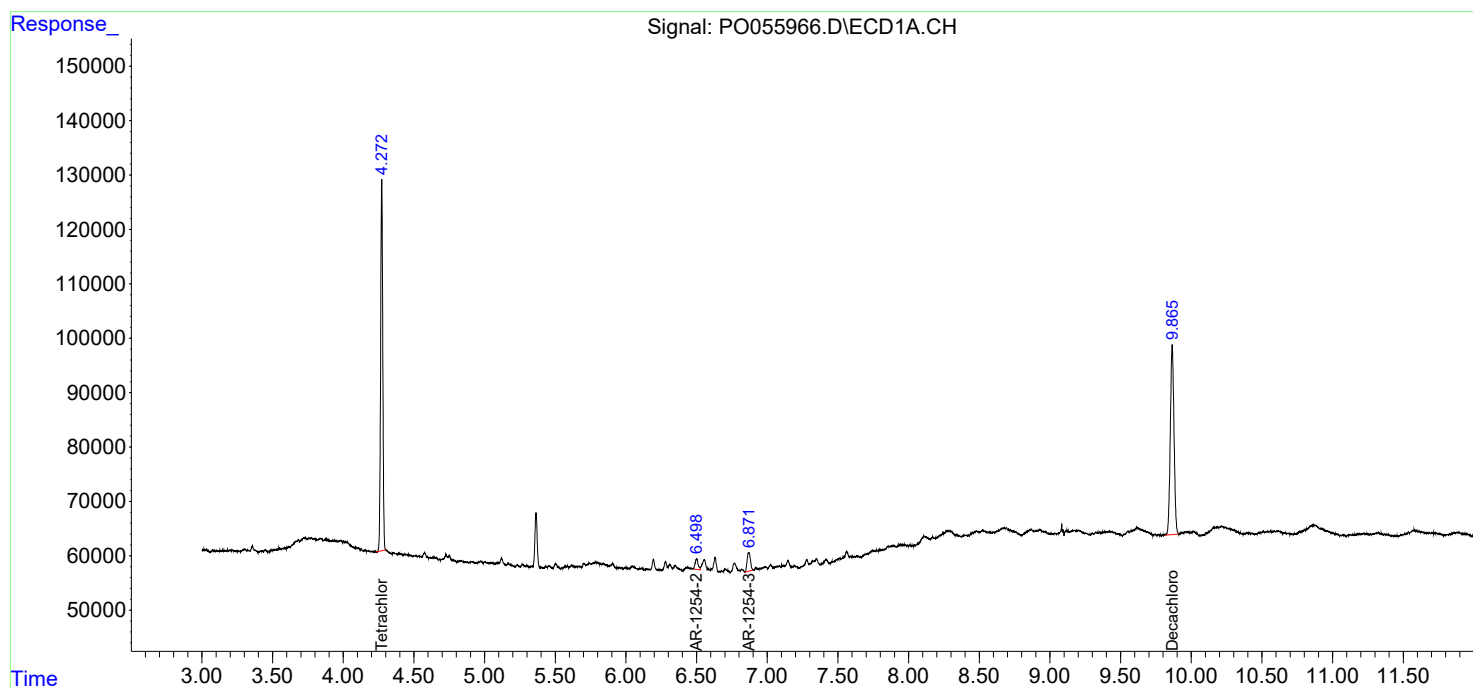


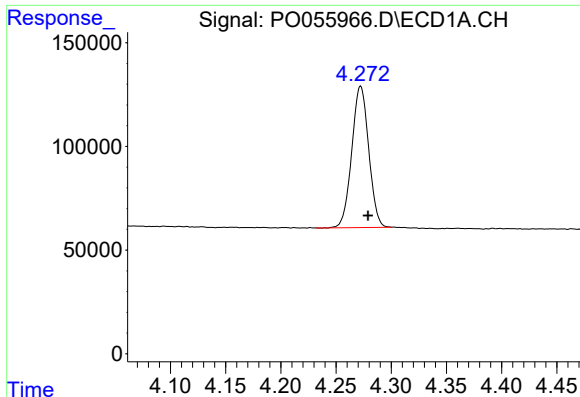

#1 Tetrachloro-m-xylene


R.T.: 4.272 min
Delta R.T.: -0.007 min
Response: 726583
Conc: 24.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-08-050319-B

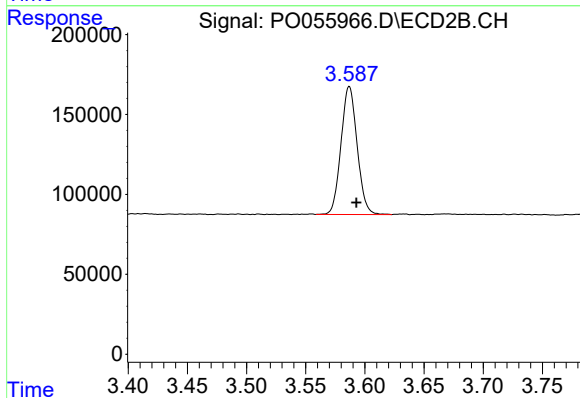


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: -0.006 min
Response: 759473
Conc: 26.89 ng/ml

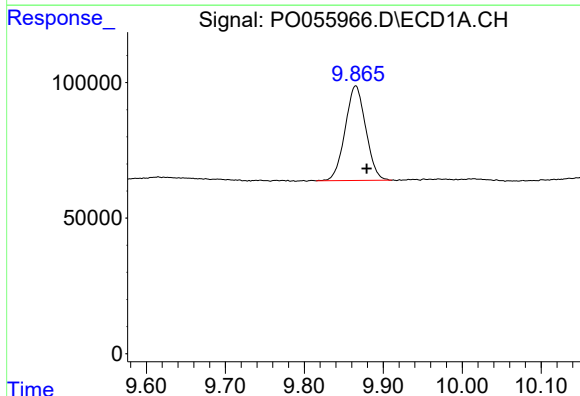


#2 Decachlorobiphenyl

R.T.: 9.865 min
Delta R.T.: -0.014 min
Response: 633423
Conc: 16.93 ng/ml

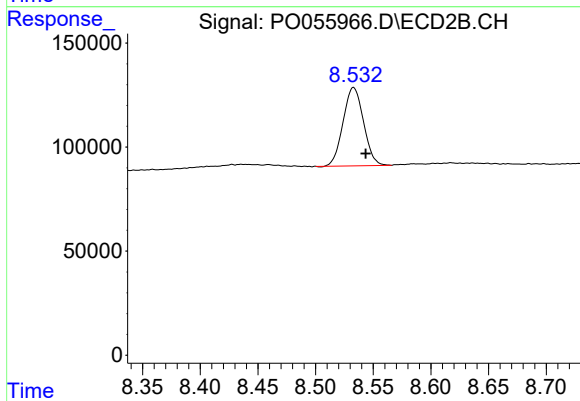

#2 Decachlorobiphenyl


R.T.: 8.533 min
Delta R.T.: -0.011 min
Response: 461853
Conc: 17.08 ng/ml

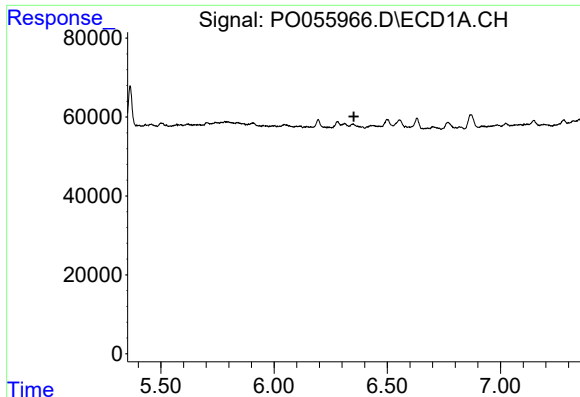

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
NB-08-050319-B

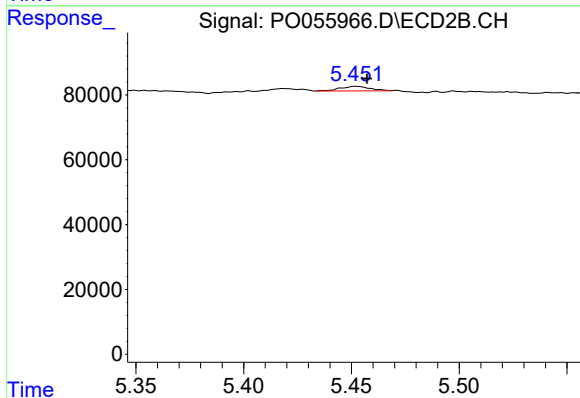


#20 AR-1242-5

R.T.: 5.452 min
Delta R.T.: -0.006 min
Response: 13321
Conc: 11.10 ng/ml

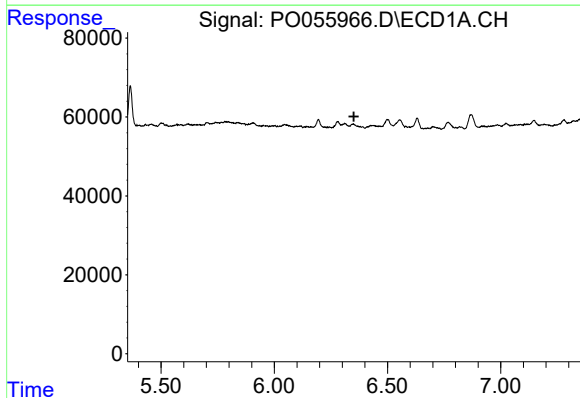


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

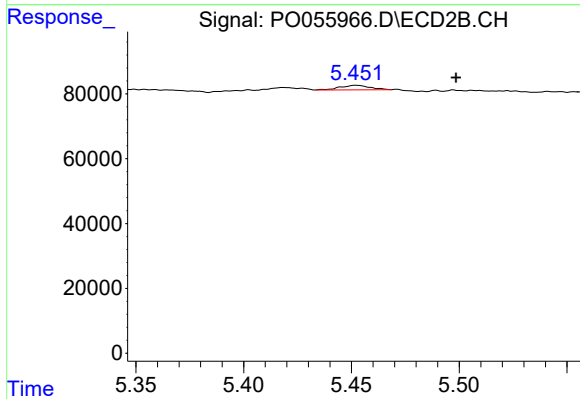

#25 AR-1248-5


R.T.: 5.452 min
Delta R.T.: -0.047 min
Response: 13321
Conc: 8.89 ng/ml

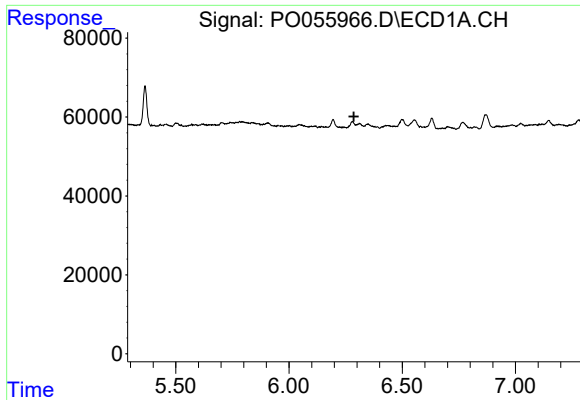

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
NB-08-050319-B

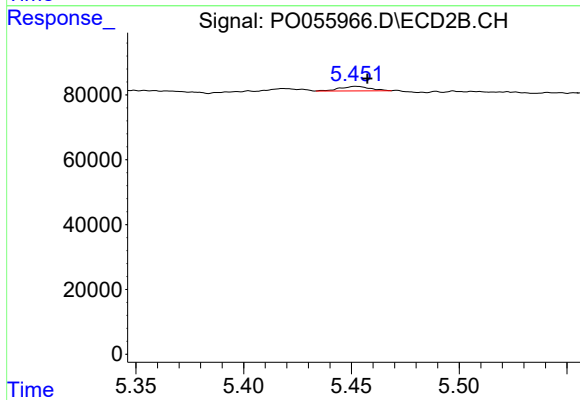


#26 AR-1254-1

R.T.: 5.452 min
Delta R.T.: -0.006 min
Response: 13321
Conc: 4.98 ng/ml

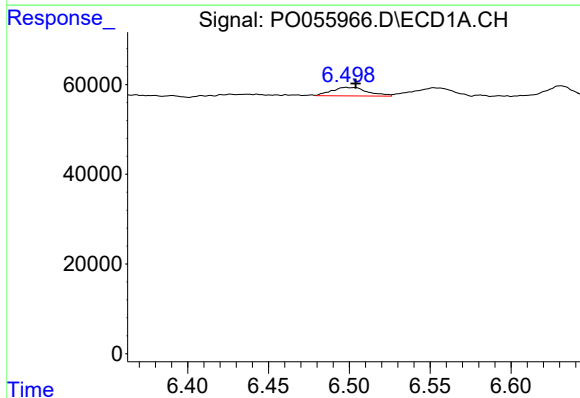


#27 AR-1254-2

R.T.: 6.498 min
Delta R.T.: -0.006 min
Response: 29449
Conc: 8.87 ng/ml

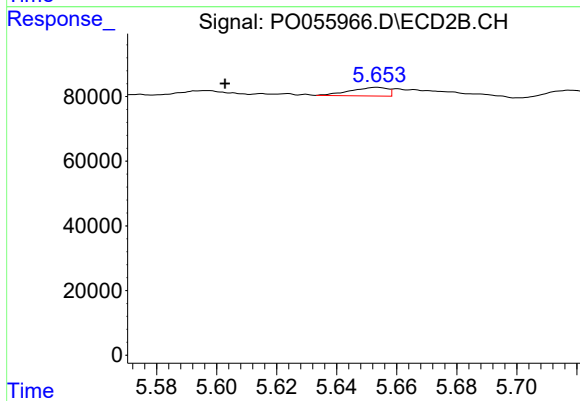

#27 AR-1254-2


R.T.: 5.653 min
Delta R.T.: 0.051 min
Response: 23100
Conc: 9.46 ng/ml

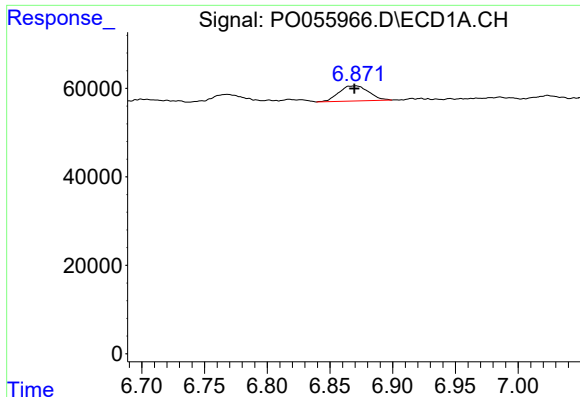

#28 AR-1254-3


R.T.: 6.871 min
Delta R.T.: 0.001 min
Response: 56076
Conc: 15.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-08-050319-B

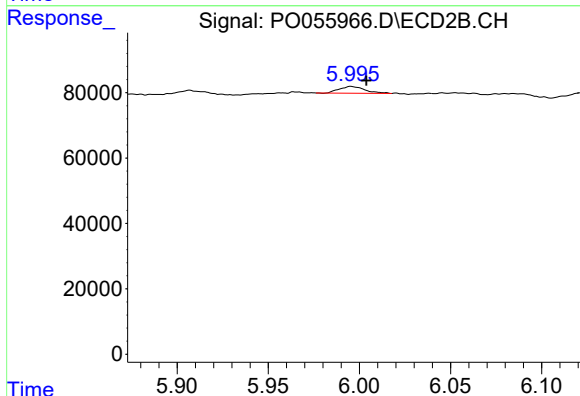


#28 AR-1254-3

R.T.: 5.995 min
Delta R.T.: -0.008 min
Response: 20070
Conc: 5.06 ng/ml

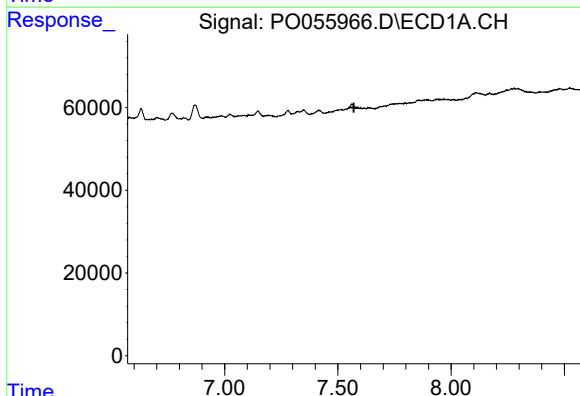


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.571 min
Response: 0
Conc: N.D.

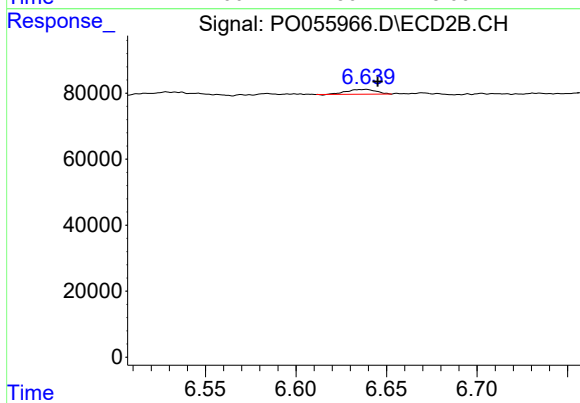

#30 AR-1254-5


R.T.: 6.639 min
Delta R.T.: -0.006 min
Response: 16514
Conc: 4.56 ng/ml

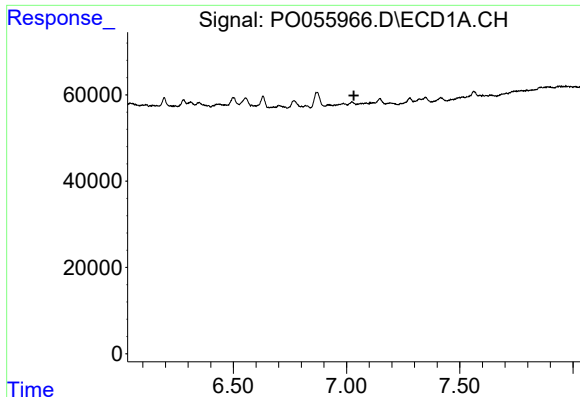

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
NB-08-050319-B

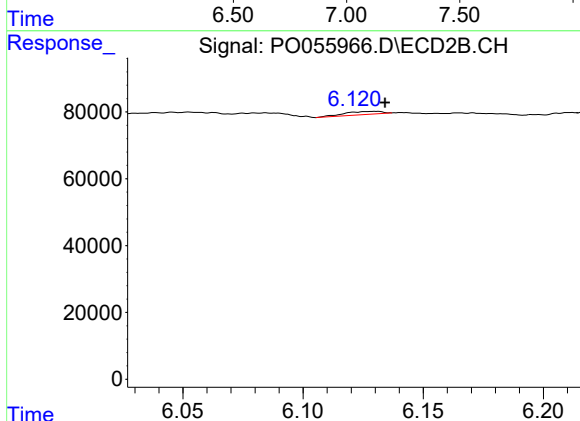


#31 AR-1260-1

R.T.: 6.131 min
Delta R.T.: -0.003 min
Response: 10017
Conc: 4.55 ng/ml

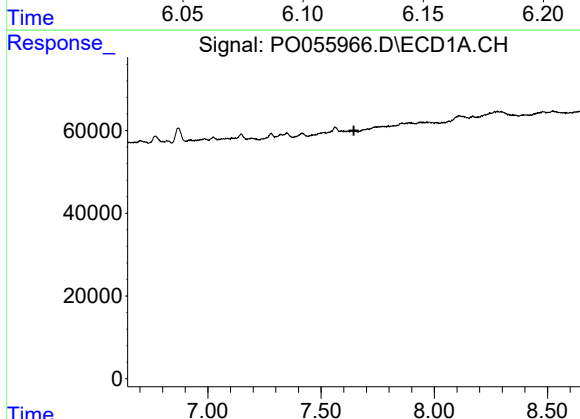

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

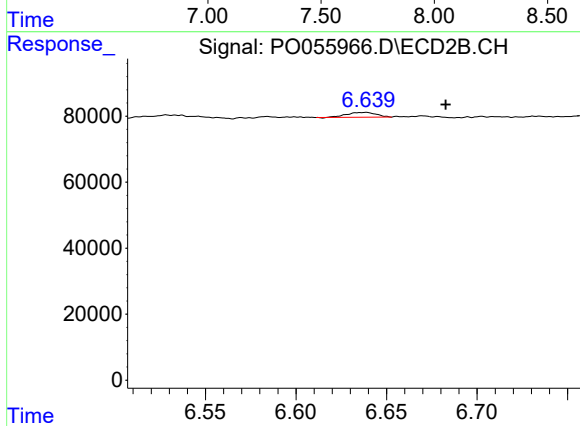

#36 AR-1262-1

R.T.: 6.639 min
Delta R.T.: -0.044 min
Response: 16514
Conc: 4.03 ng/ml