

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050819\
 Data File : P0055993.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 May 2019 20:35
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 04:14:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.272	3.588	598366	599488	19.995	21.226
2) SA Decachlor...	9.862	8.532	603344	479984	16.125	17.749
Target Compounds						
7) L1 AR-1016-5	0.000	5.097	0	4019	N.D.	3.651 #
15) L3 AR-1232-5	0.000	5.097	0	4019	N.D.	8.294 #
20) L4 AR-1242-5	0.000	5.476	0	18163	N.D.	15.130 #
24) L5 AR-1248-4	6.282	5.097	35913	4019	20.595	2.862 #
25) L5 AR-1248-5	6.282	5.476	35913	18163	21.500	12.127 #
26) L6 AR-1254-1	6.282	5.476	35913	18163	17.103	6.786 #
28) L6 AR-1254-3	6.873	0.000	44726	0	12.302	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050819\
Data File : PO055993.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2019 20:35
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 04:14:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

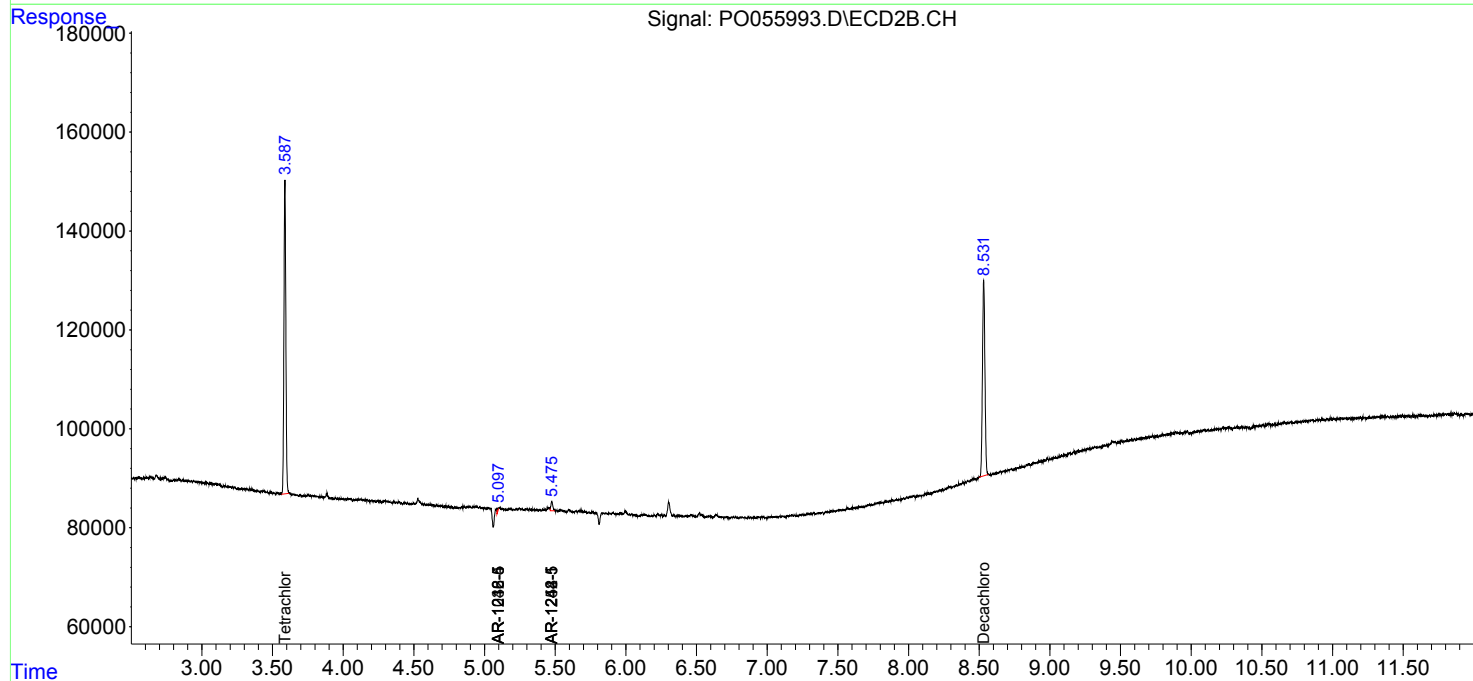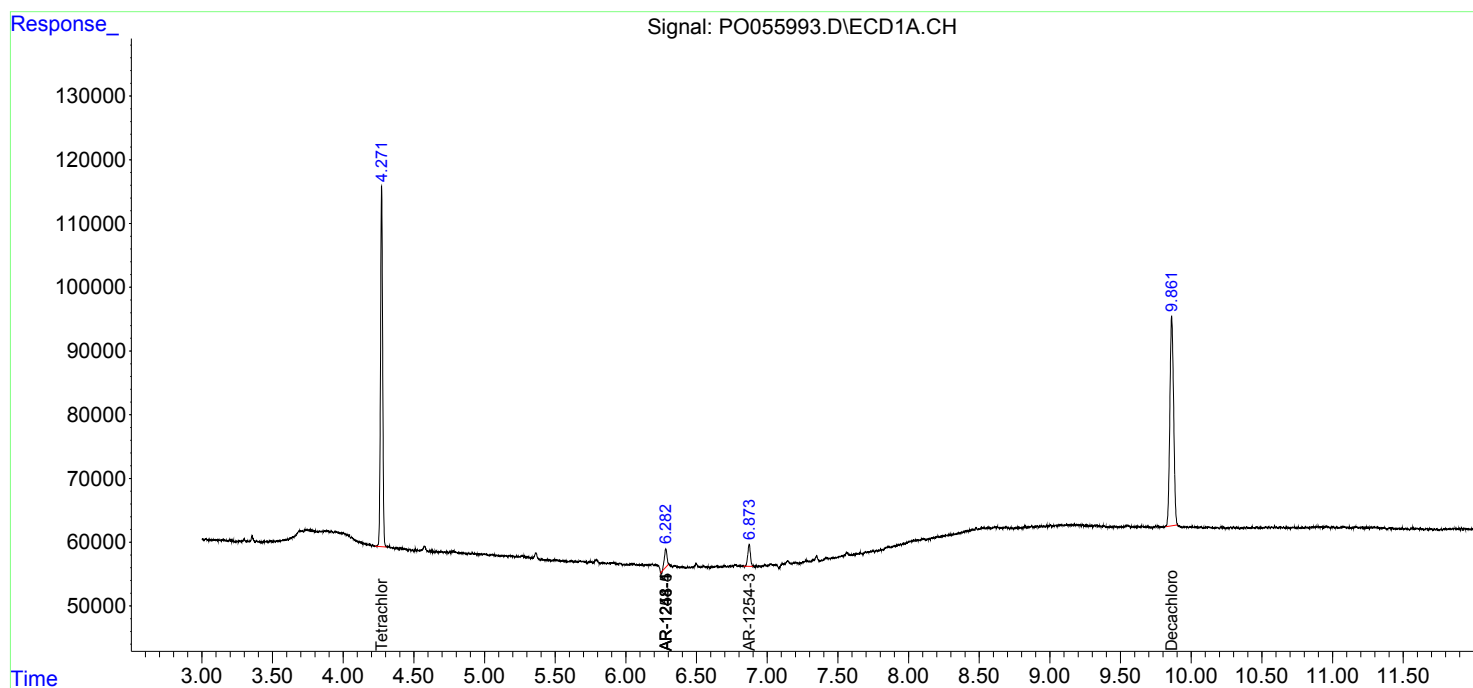


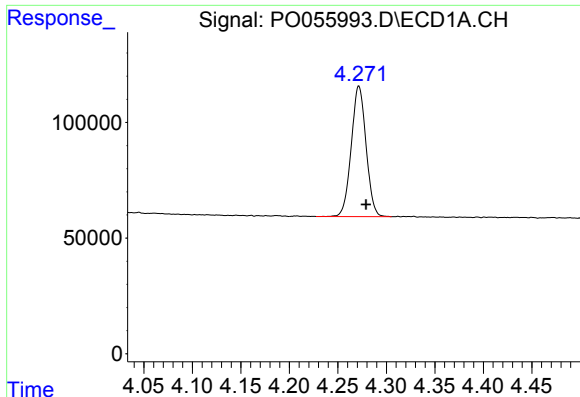

#1 Tetrachloro-m-xylene


R.T.: 4.272 min
Delta R.T.: -0.007 min
Response: 598366
Conc: 20.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

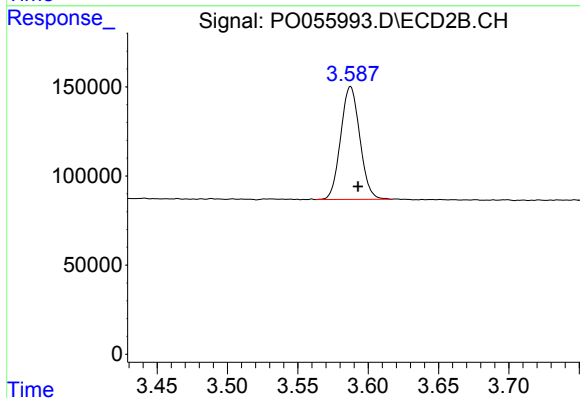


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.005 min
Response: 599488
Conc: 21.23 ng/ml

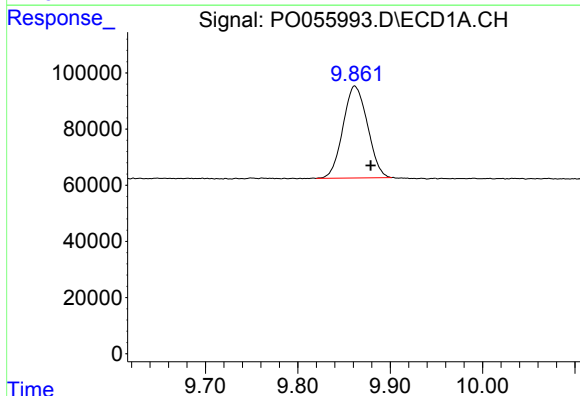


#2 Decachlorobiphenyl

R.T.: 9.862 min
Delta R.T.: -0.017 min
Response: 603344
Conc: 16.12 ng/ml

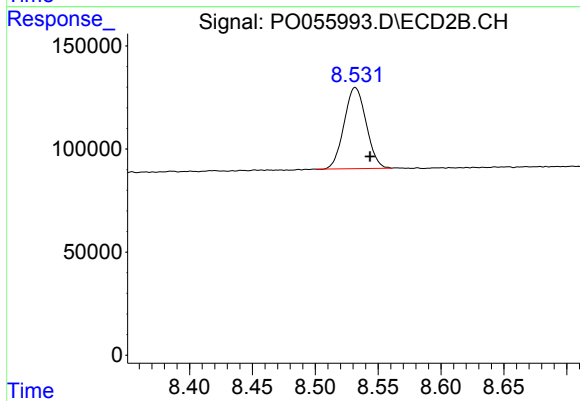

#2 Decachlorobiphenyl


R.T.: 8.532 min
Delta R.T.: -0.012 min
Response: 479984
Conc: 17.75 ng/ml

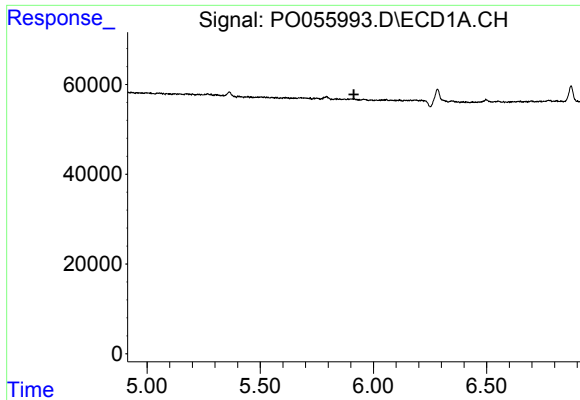

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

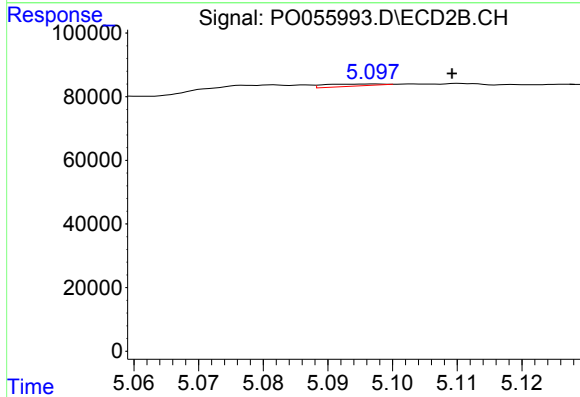


#7 AR-1016-5

R.T.: 5.097 min
Delta R.T.: -0.012 min
Response: 4019
Conc: 3.65 ng/ml

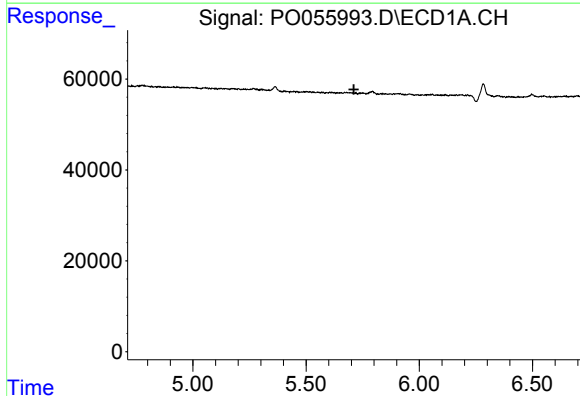


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.711 min
Response: 0
Conc: N.D.

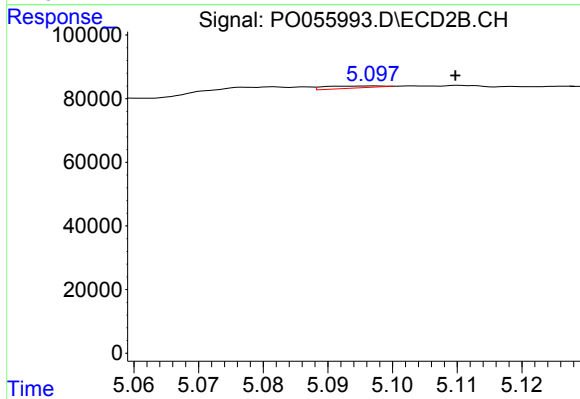

#15 AR-1232-5


R.T.: 5.097 min
Delta R.T.: -0.012 min
Response: 4019
Conc: 8.29 ng/ml

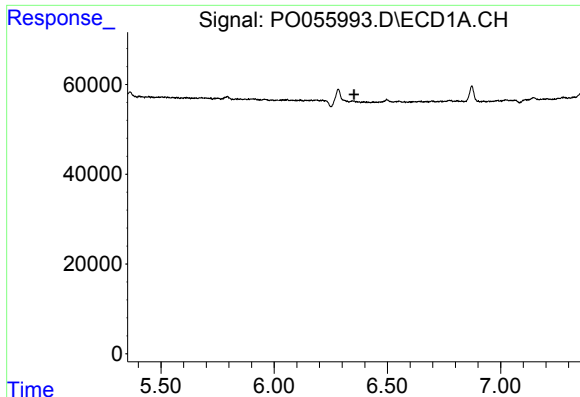

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

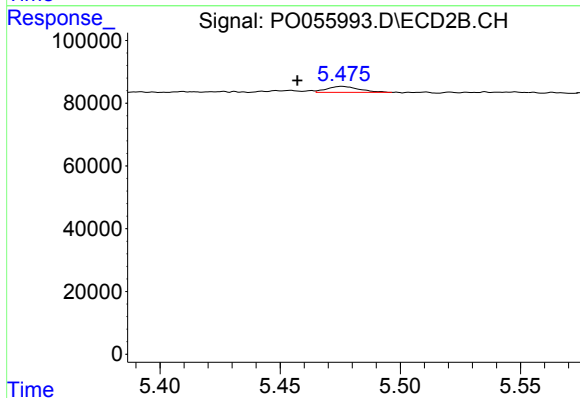


#20 AR-1242-5

R.T.: 5.476 min
Delta R.T.: 0.019 min
Response: 18163
Conc: 15.13 ng/ml

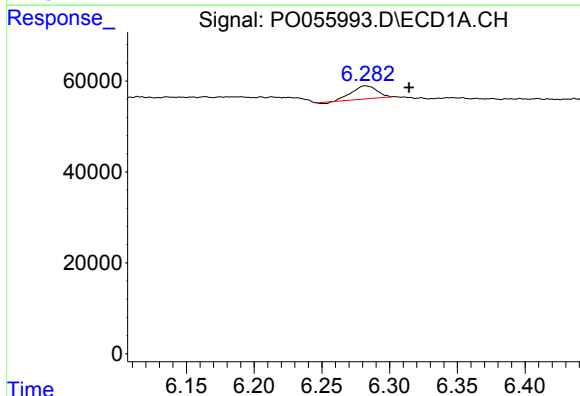


#24 AR-1248-4

R.T.: 6.282 min
Delta R.T.: -0.032 min
Response: 35913
Conc: 20.60 ng/ml

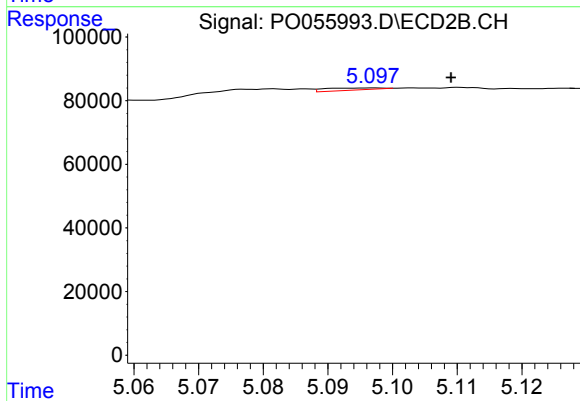

#24 AR-1248-4


R.T.: 5.097 min
Delta R.T.: -0.012 min
Response: 4019
Conc: 2.86 ng/ml

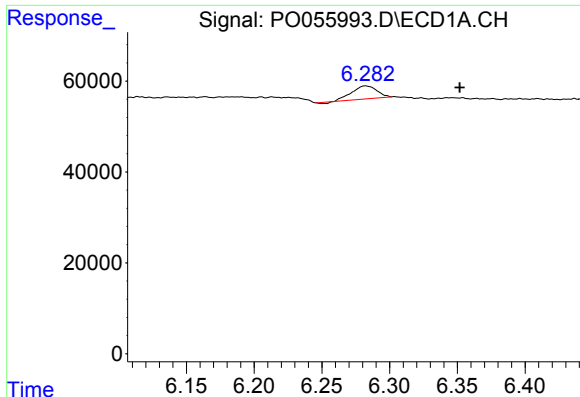

#25 AR-1248-5


R.T.: 6.282 min
Delta R.T.: -0.070 min
Response: 35913
Conc: 21.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

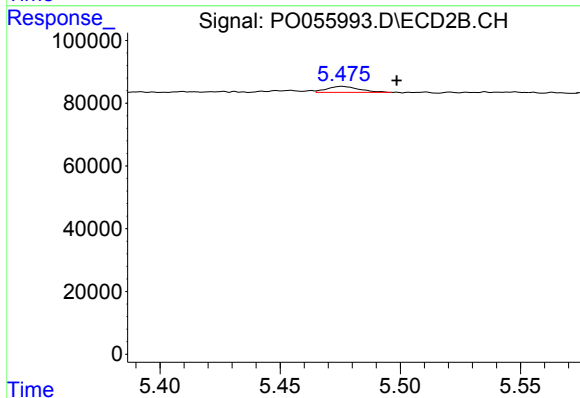


#25 AR-1248-5

R.T.: 5.476 min
Delta R.T.: -0.023 min
Response: 18163
Conc: 12.13 ng/ml

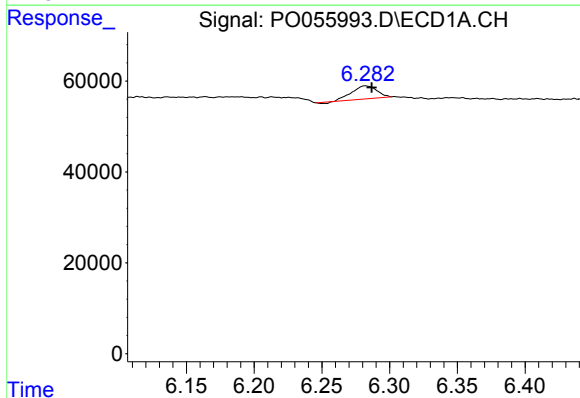


#26 AR-1254-1

R.T.: 6.282 min
Delta R.T.: -0.005 min
Response: 35913
Conc: 17.10 ng/ml

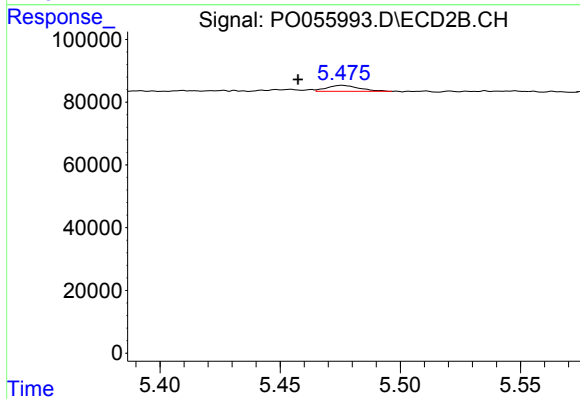

#26 AR-1254-1


R.T.: 5.476 min
Delta R.T.: 0.018 min
Response: 18163
Conc: 6.79 ng/ml

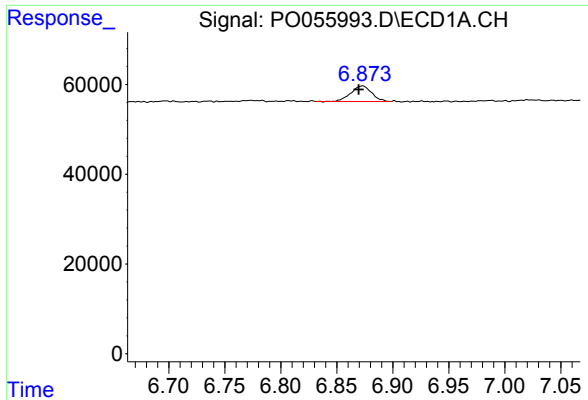

#28 AR-1254-3

R.T.: 6.873 min
Delta R.T.: 0.004 min
Response: 44726
Conc: 12.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

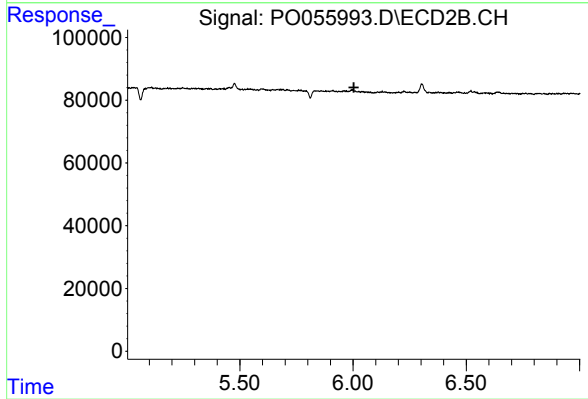

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.