

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050819\
Data File : P0055964.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2019 10:46
Operator : SM/SJ
Sample : K2689-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
329

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 11:25:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.286	3.590	630843	548746	21.080m	19.429
2) SA Decachlor...	9.881	8.537	745170	560753	19.915	20.736

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050819\
Data File : P0055964.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2019 10:46
Operator : SM/SJ
Sample : K2689-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
329

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 11:25:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

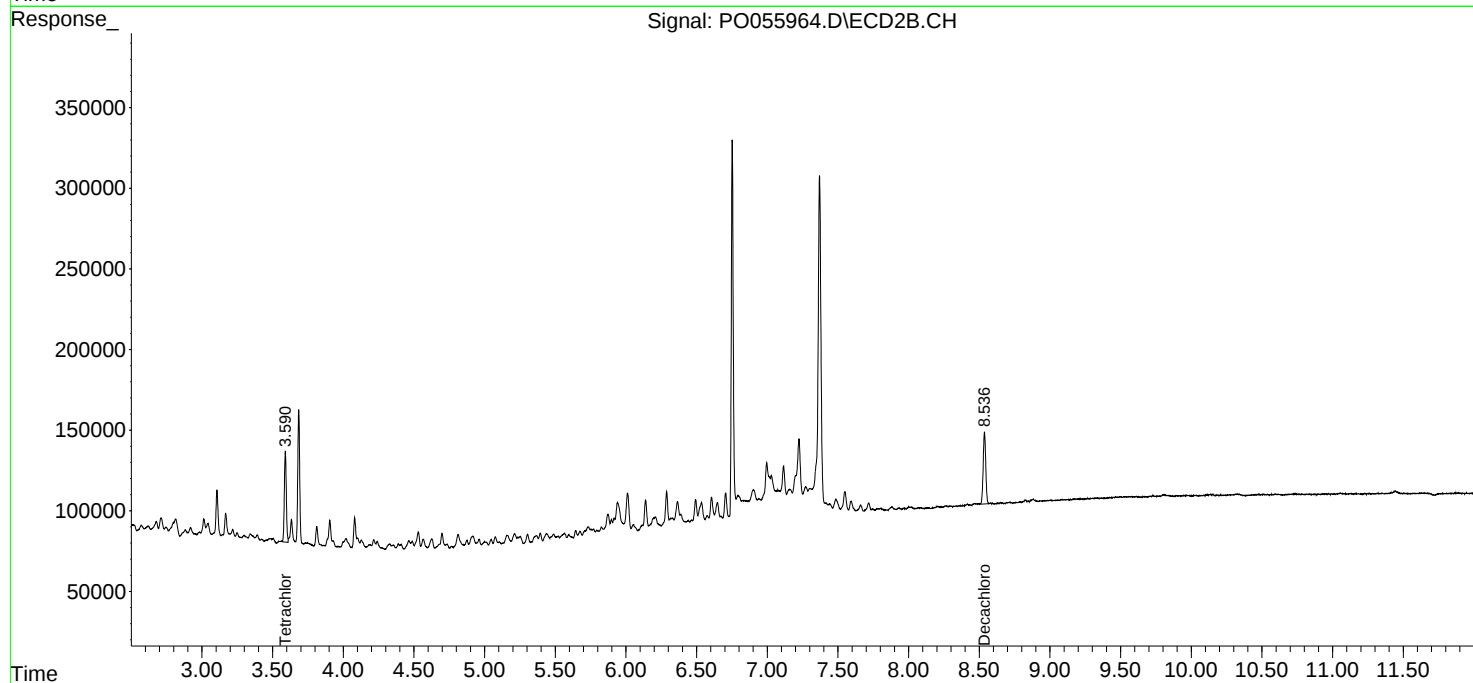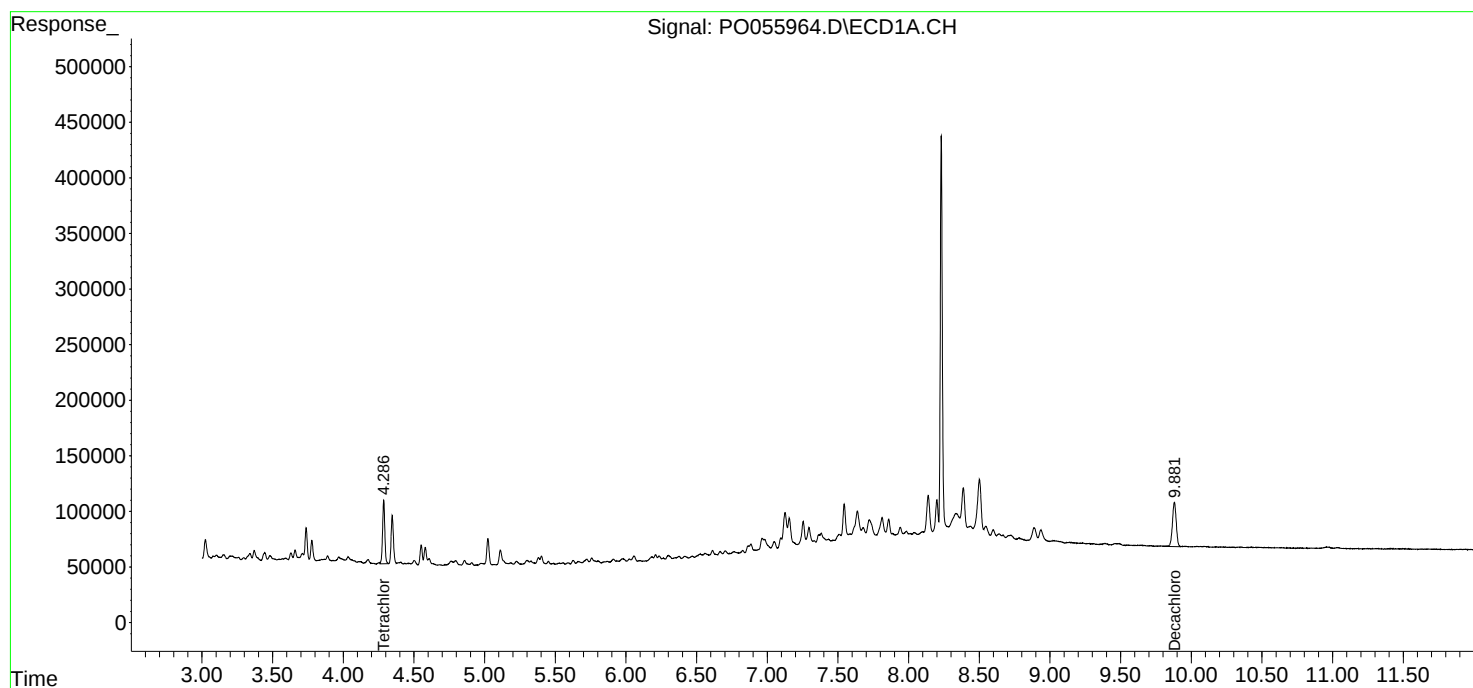


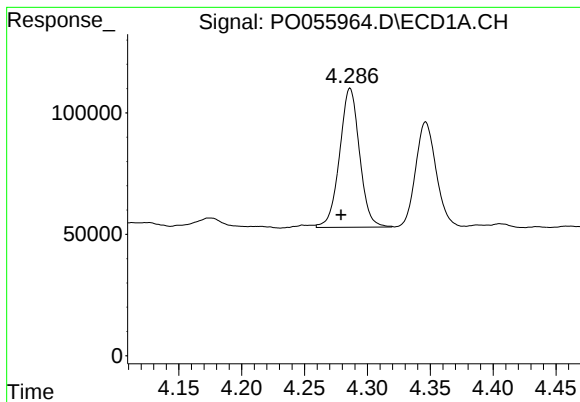

#1 Tetrachloro-m-xylene


R.T.: 4.286 min
Delta R.T.: 0.007 min
Response: 630843
Conc: 21.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
329

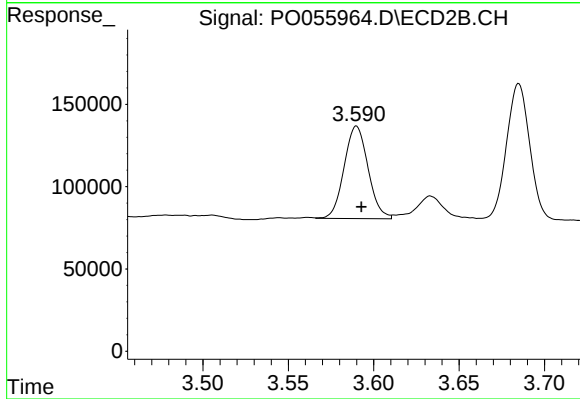


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.003 min
Response: 548746
Conc: 19.43 ng/ml

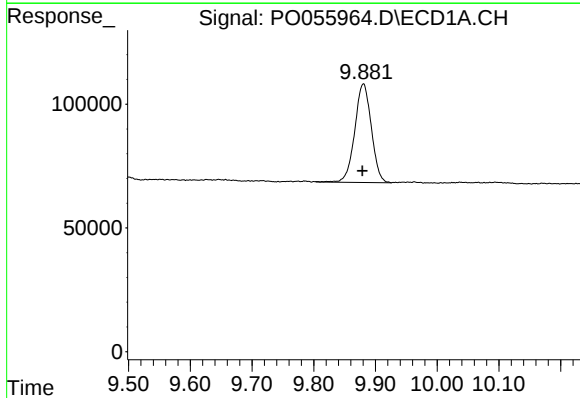

#2 Decachlorobiphenyl

R.T.: 9.881 min
Delta R.T.: 0.002 min
Response: 745170
Conc: 19.92 ng/ml

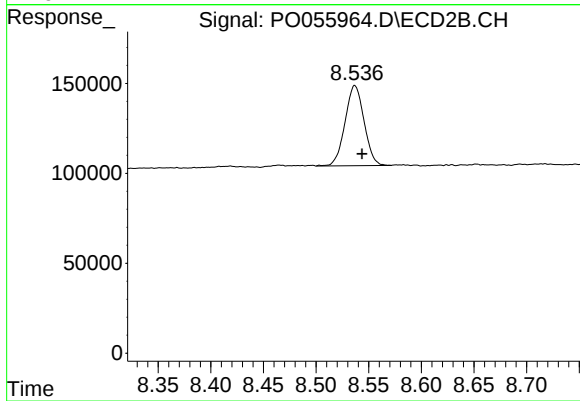

#2 Decachlorobiphenyl

R.T.: 8.537 min
Delta R.T.: -0.007 min
Response: 560753
Conc: 20.74 ng/ml