

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050819\
Data File : P0055983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2019 16:48
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 04:10:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.589	738306	776571	24.671	27.496
2) SA Decachlor...	9.874	8.538	524106	381665	14.007	14.113

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050819\
Data File : PO055983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2019 16:48
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 04:10:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

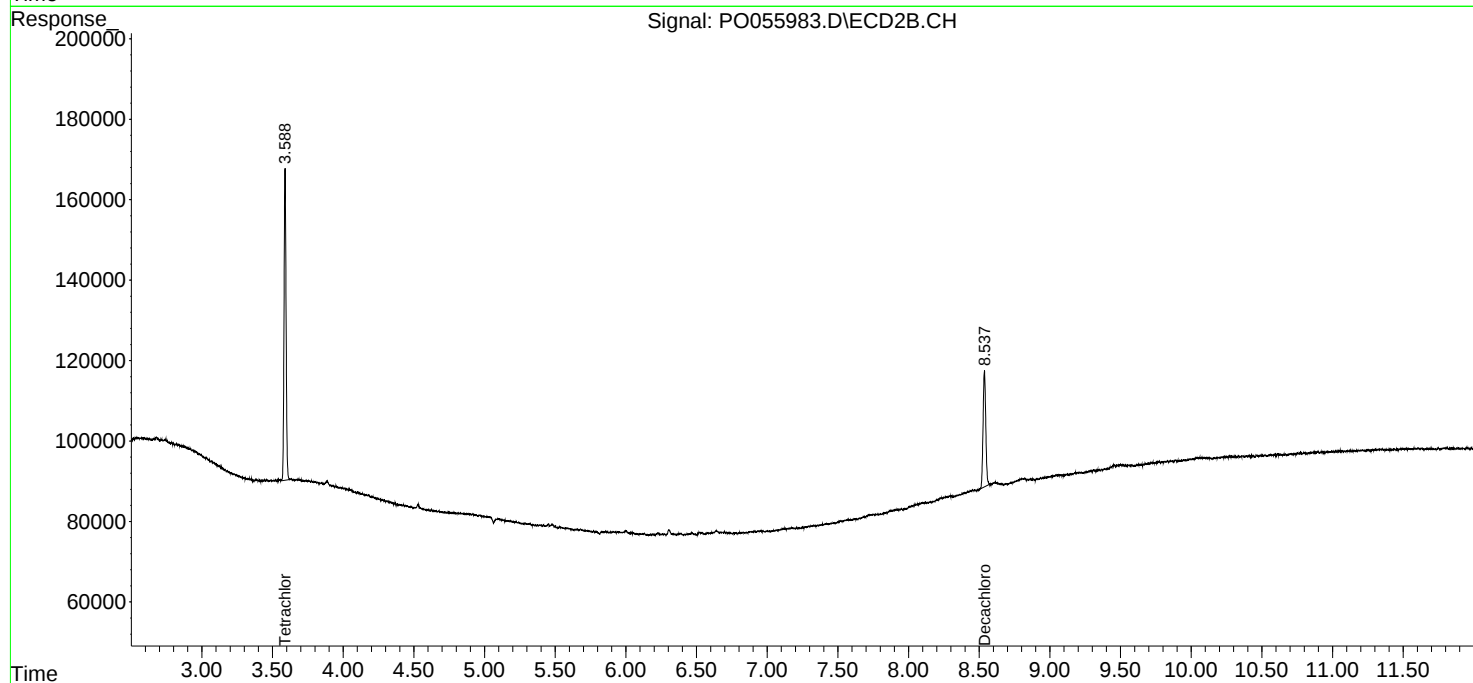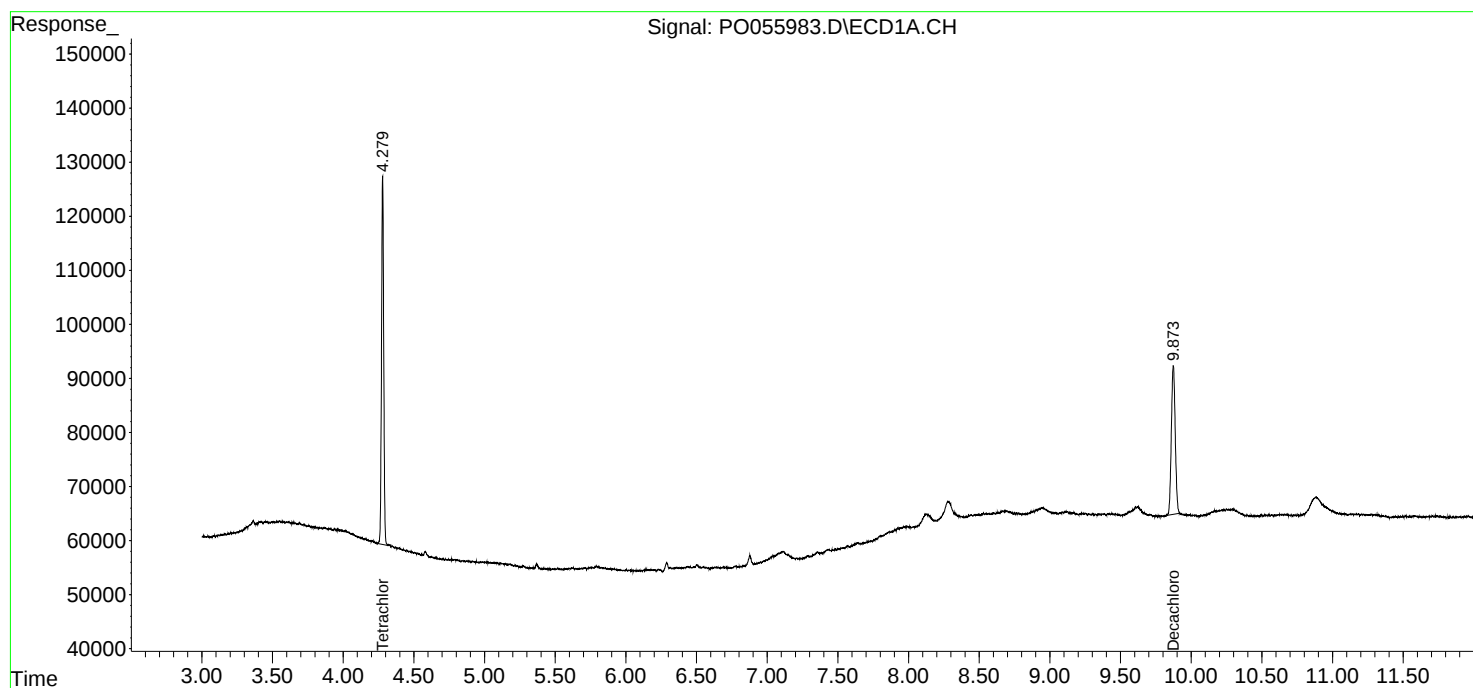


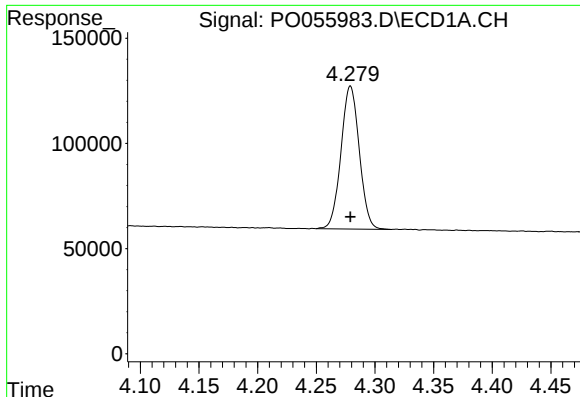

#1 Tetrachloro-m-xylene


R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 738306
Conc: 24.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

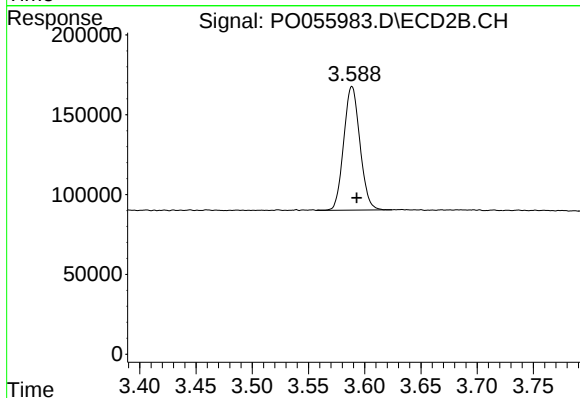


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 776571
Conc: 27.50 ng/ml

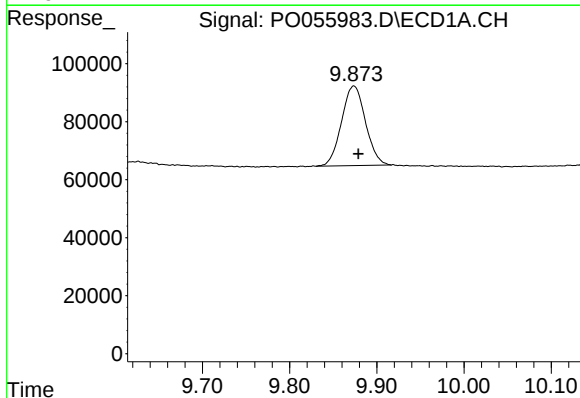

#2 Decachlorobiphenyl

R.T.: 9.874 min
Delta R.T.: -0.005 min
Response: 524106
Conc: 14.01 ng/ml

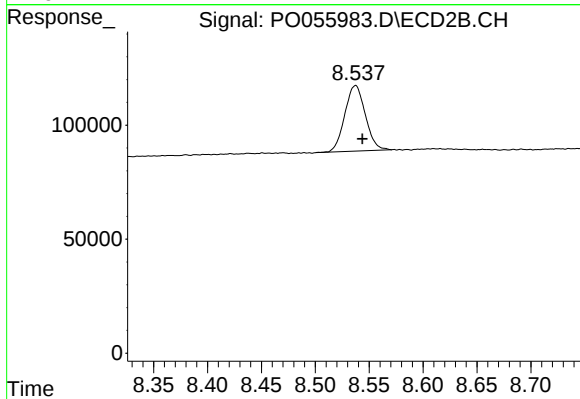

#2 Decachlorobiphenyl

R.T.: 8.538 min
Delta R.T.: -0.006 min
Response: 381665
Conc: 14.11 ng/ml