

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050819\
 Data File : P0055991.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 May 2019 20:01
 Operator : SM/SJ
 Sample : K2675-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OUTFALL001-WK-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 04:13:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.273	3.588	1021153	999438	34.123	35.387
2) SA Decachlor...	9.863	8.533	906957	713136	24.239	26.370m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050819\
Data File : P0055991.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 May 2019 20:01
Operator : SM/SJ
Sample : K2675-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OUTFALL001-WK-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 04:13:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

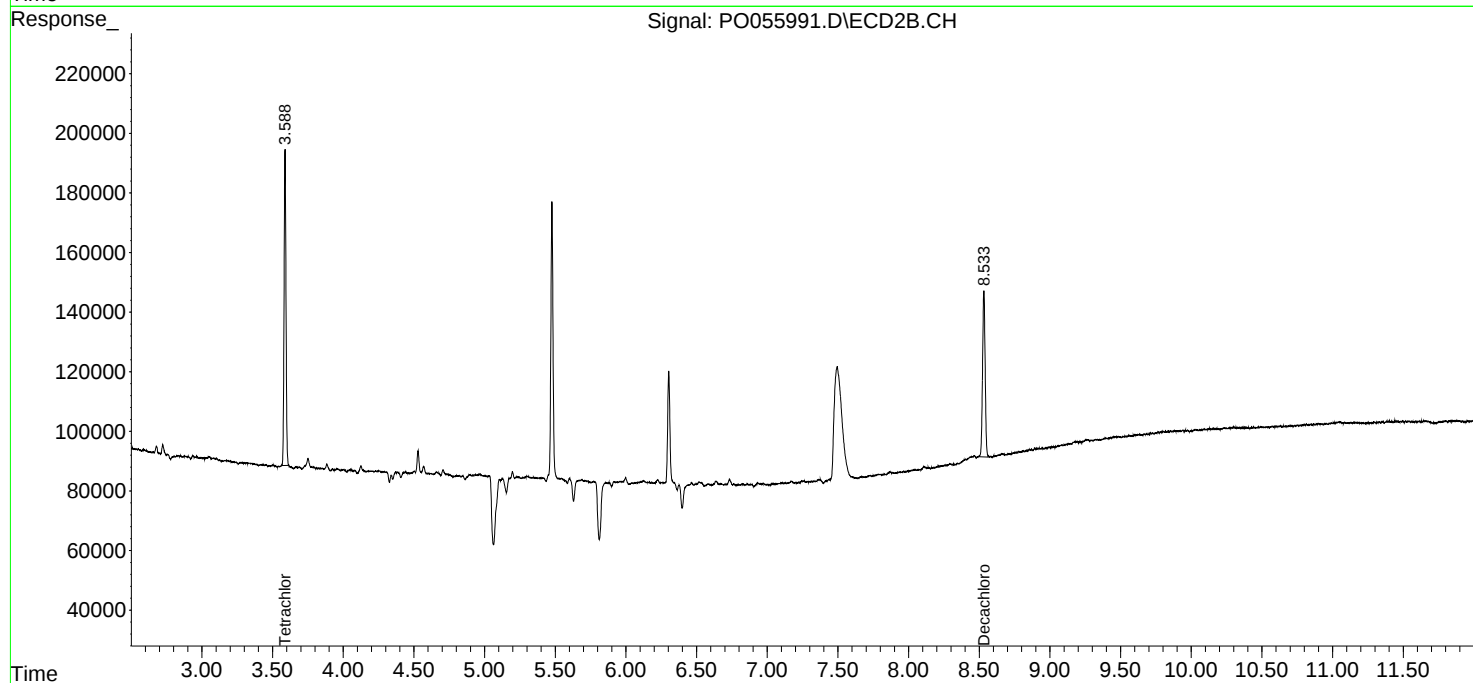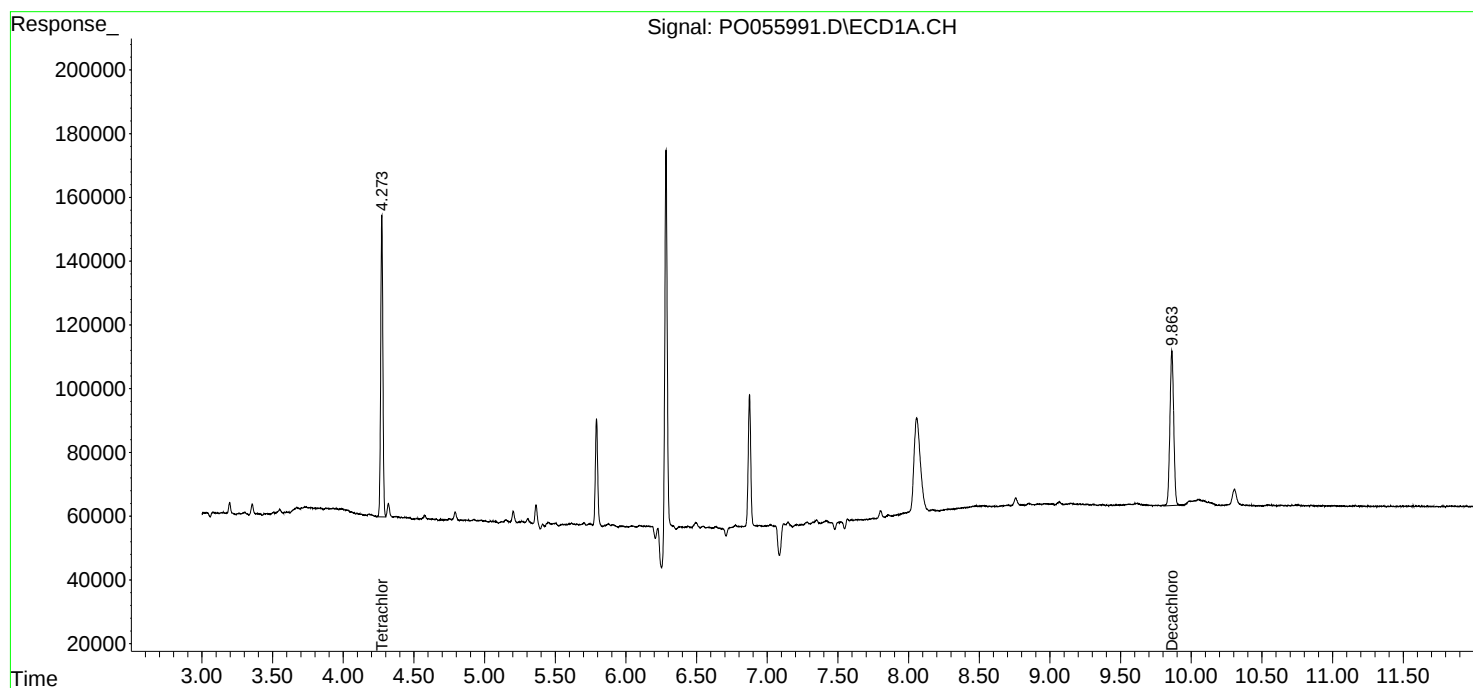


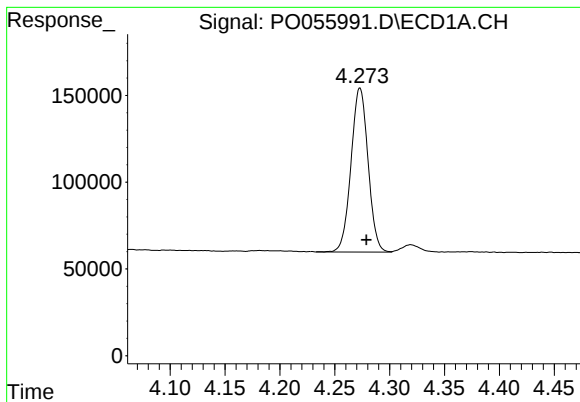

#1 Tetrachloro-m-xylene


R.T.: 4.273 min
Delta R.T.: -0.006 min
Response: 1021153
Conc: 34.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
OUTFALL001-WK-1

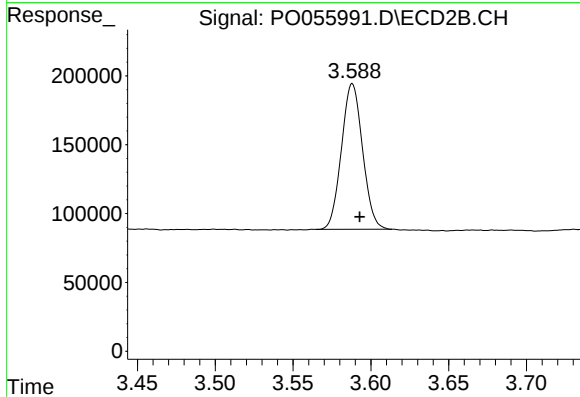


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.005 min
Response: 999438
Conc: 35.39 ng/ml

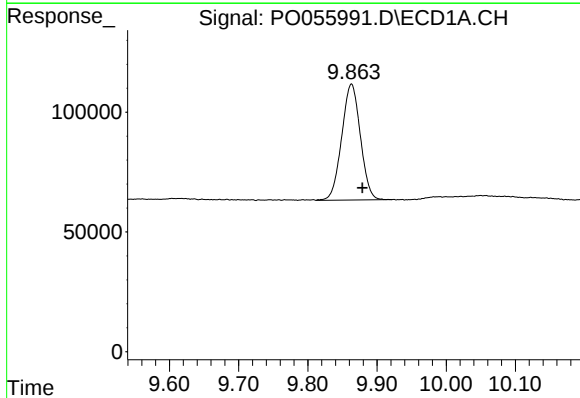

#2 Decachlorobiphenyl

R.T.: 9.863 min
Delta R.T.: -0.016 min
Response: 906957
Conc: 24.24 ng/ml

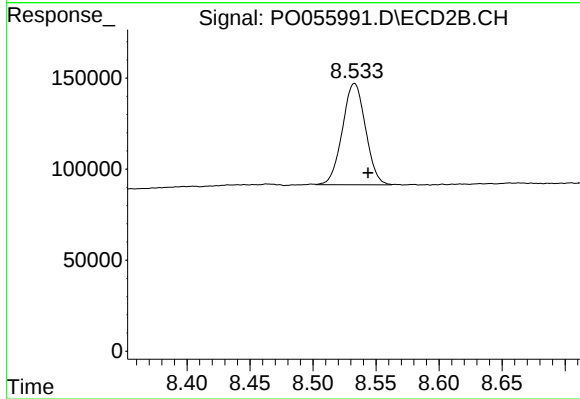

#2 Decachlorobiphenyl

R.T.: 8.533 min
Delta R.T.: -0.011 min
Response: 713136
Conc: 26.37 ng/ml m