

Data Path : P:\HPCHEM1\ECD 0\Data\P0050918\
 Data File : P0044545.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 May 2018 2:07
 Operator : SM/UA
 Sample : J2780-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BRICK-AND-MORTAR

Manual Integrations
 APPROVED

ugo
 5/11/2018 11:39:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 05:41:23 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 10 02:14:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.035	3.301	4406861	5885184	21.906m	21.733m
2) SA Decachlor...	9.355	8.043	2873219	3051718	19.788	17.467

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO050918\
Data File : PO044545.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2018 2:07
Operator : SM/UA
Sample : J2780-01
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BRICK-AND-MORTAR


Manual Integrations
APPROVED

ugo
5/11/2018 11:39:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 05:41:23 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

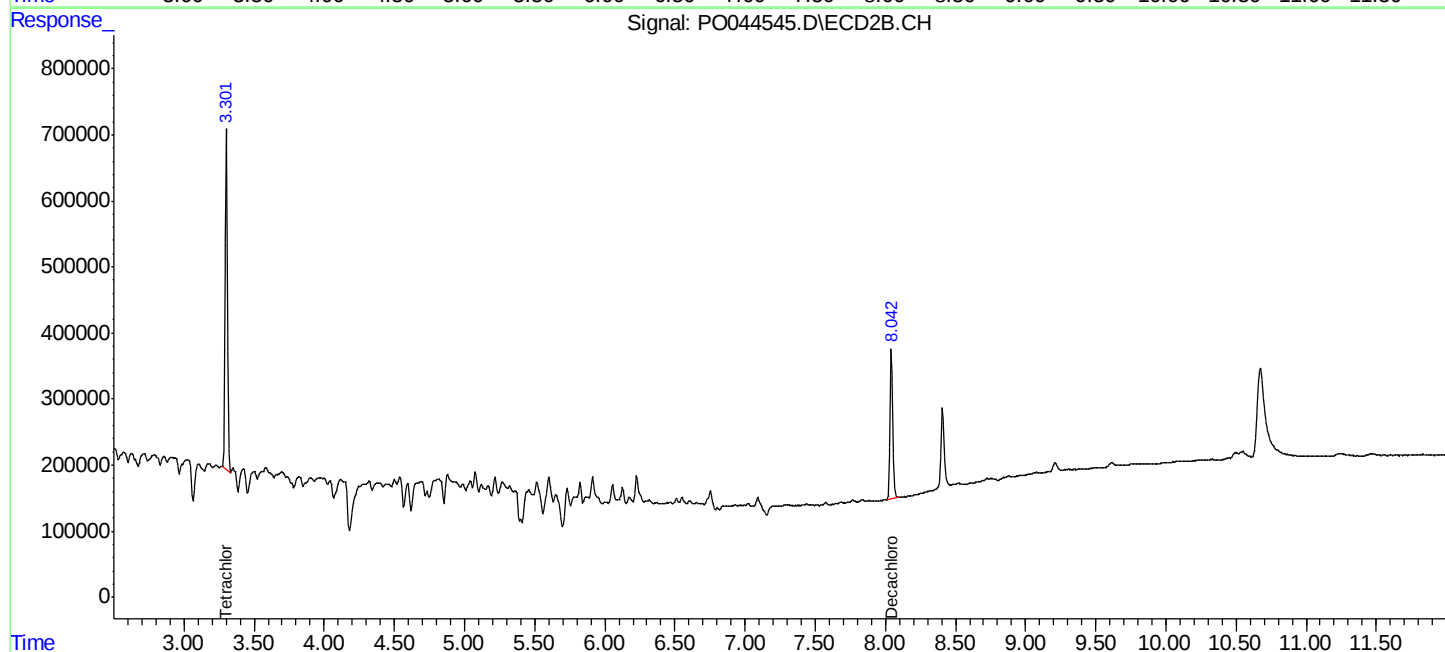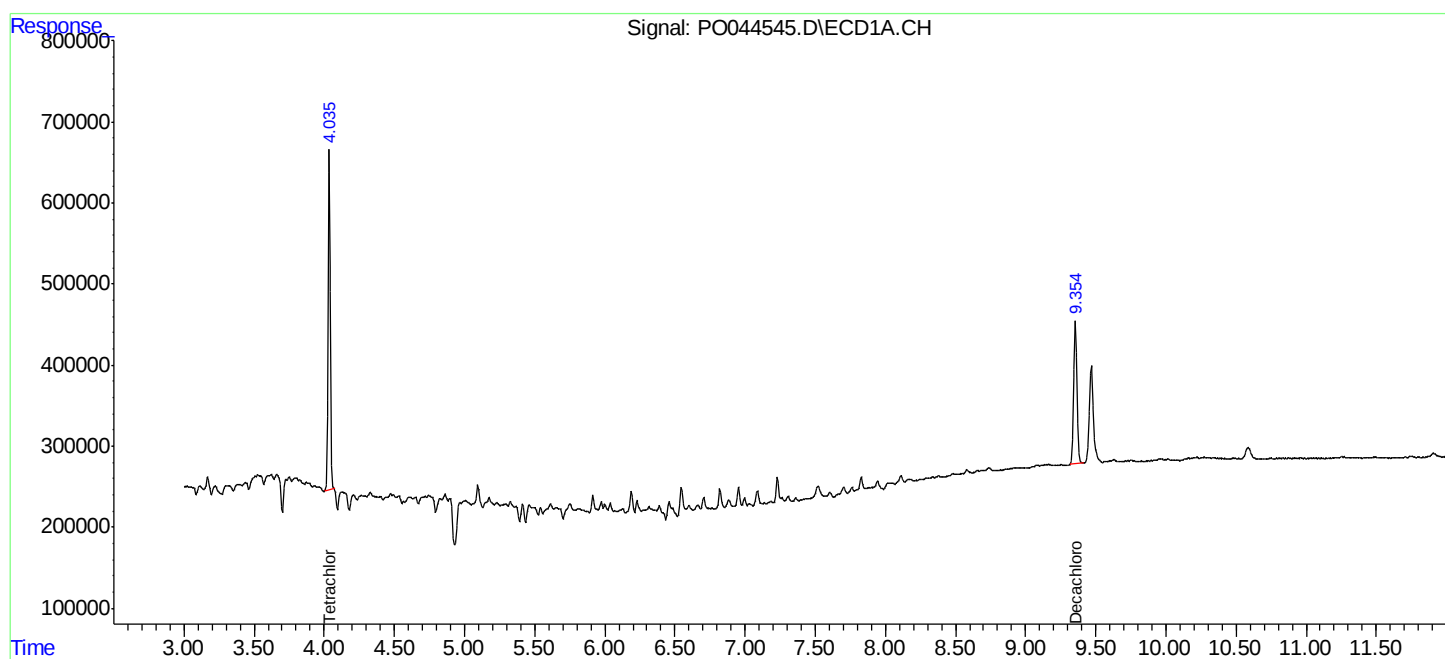

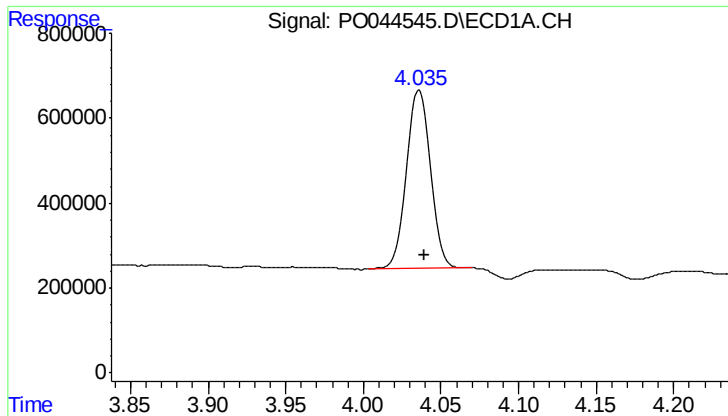


#1 Tetrachloro-m-xylene

R.T.: 4.035 min
 Delta R.T.: -0.004 min
 Response: 4406861
 Conc: 21.91 ng/ml

Instrument :
 ECD_O
 ClientSampleId :
 BRICK-AND-MORTAR


Manual Integrations
 APPROVED

ugo
 5/11/2018 11:39:21 AM

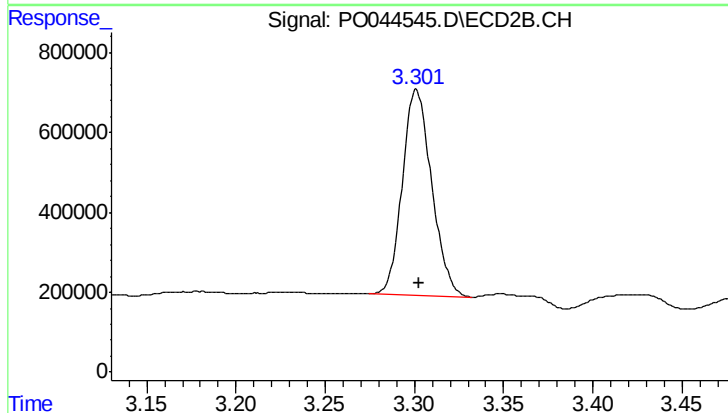


#1 Tetrachloro-m-xylene

R.T.: 3.301 min
 Delta R.T.: -0.002 min
 Response: 5885184
 Conc: 21.73 ng/ml m

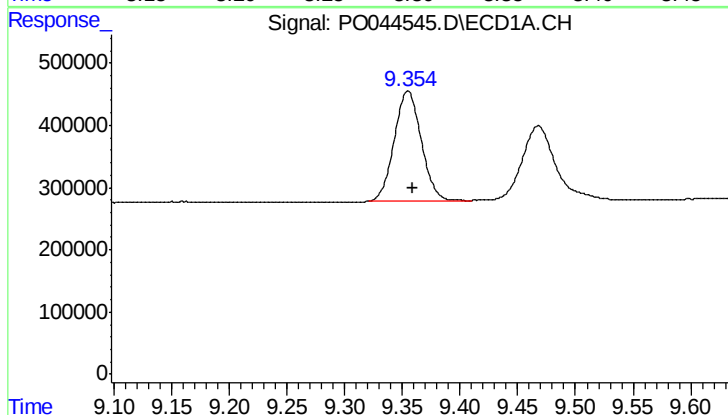

#2 Decachlorobiphenyl

R.T.: 9.355 min
 Delta R.T.: -0.005 min
 Response: 2873219
 Conc: 19.79 ng/ml

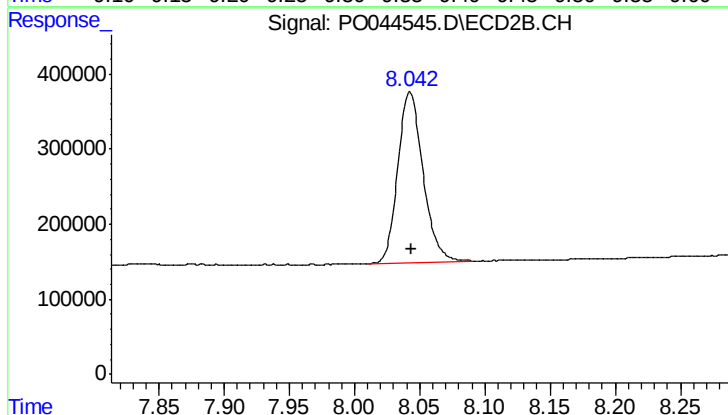

#2 Decachlorobiphenyl

R.T.: 8.043 min
 Delta R.T.: -0.002 min
 Response: 3051718
 Conc: 17.47 ng/ml