

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050919\
 Data File : P0056027.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 May 2019 22:16
 Operator : SM/SJ
 Sample : K2749-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRS-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 05:13:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.269	3.585	743258	725413	24.837	25.684
2) SA Decachlor...	9.858	8.528	638537	454878	17.065	16.821
Target Compounds						
28) L6 AR-1254-3	6.864	0.000	25047	0	6.890	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050919\
Data File : P0056027.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 May 2019 22:16
Operator : SM/SJ
Sample : K2749-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TRS-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 05:13:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

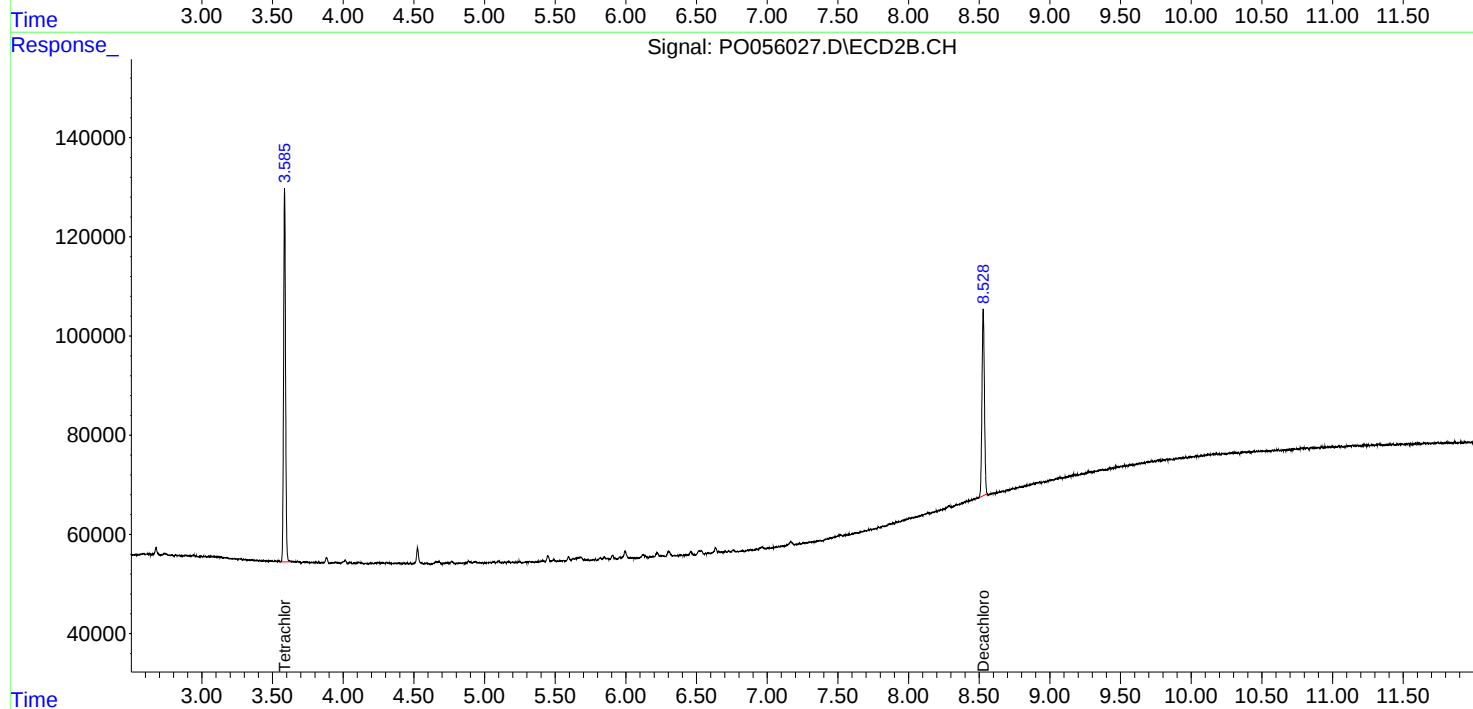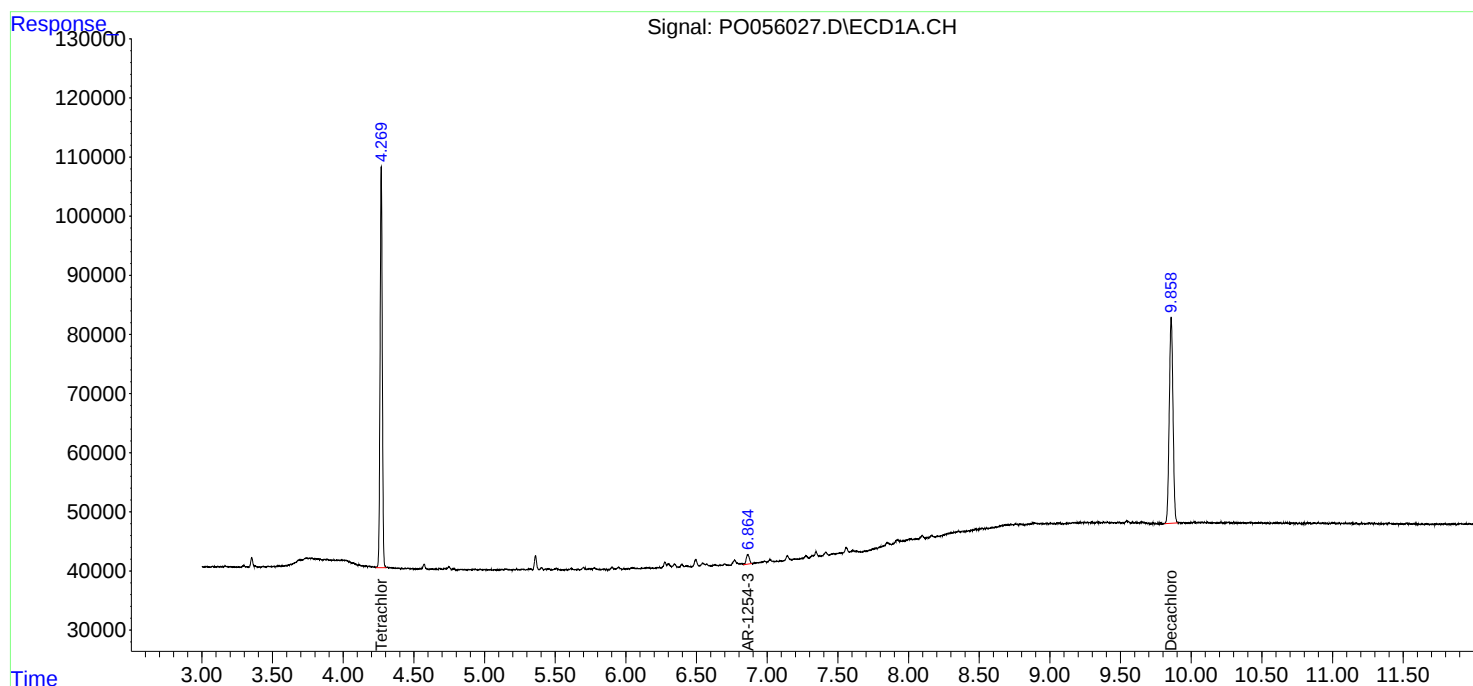


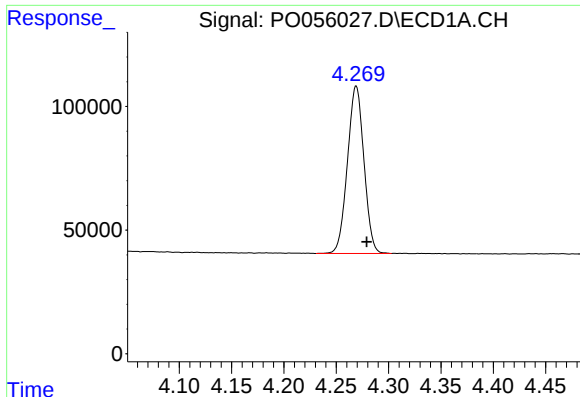

#1 Tetrachloro-m-xylene


R.T.: 4.269 min
Delta R.T.: -0.010 min
Response: 743258
Conc: 24.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRS-2

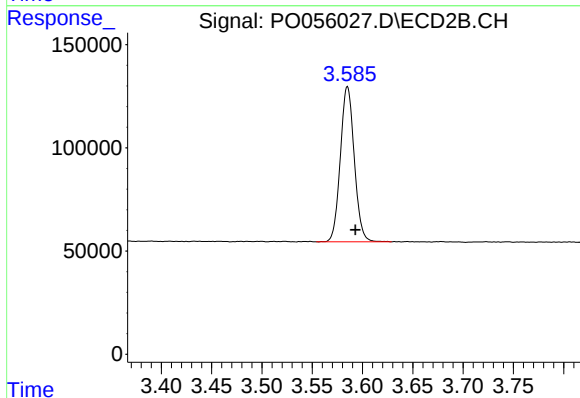


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: -0.008 min
Response: 725413
Conc: 25.68 ng/ml

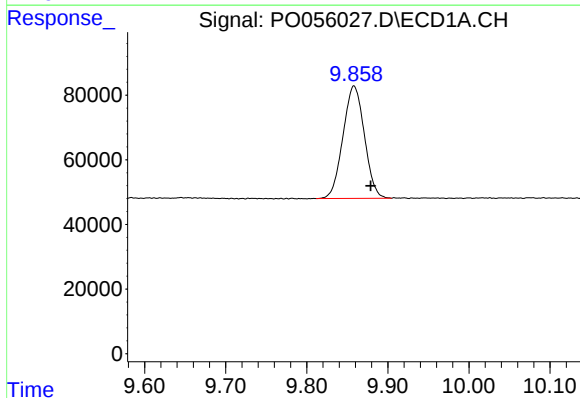


#2 Decachlorobiphenyl

R.T.: 9.858 min
Delta R.T.: -0.021 min
Response: 638537
Conc: 17.07 ng/ml

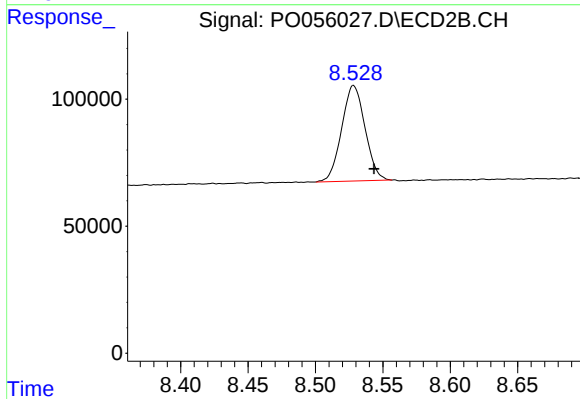

#2 Decachlorobiphenyl


R.T.: 8.528 min
Delta R.T.: -0.015 min
Response: 454878
Conc: 16.82 ng/ml

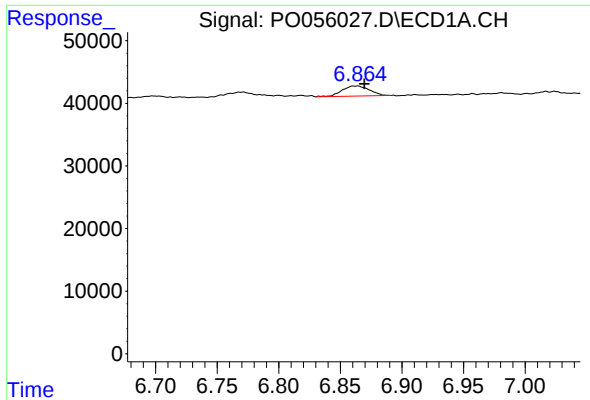

#28 AR-1254-3

R.T.: 6.864 min
Delta R.T.: -0.005 min
Response: 25047
Conc: 6.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRS-2

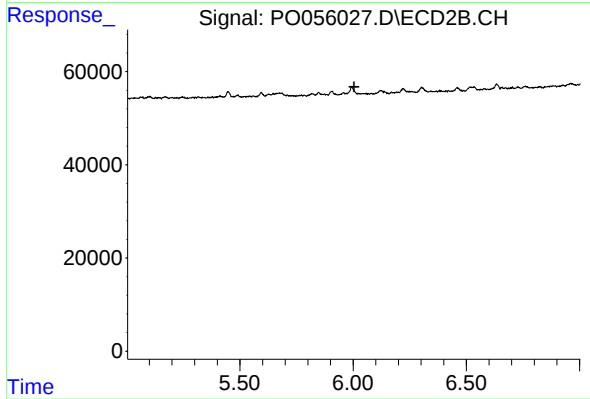

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.