

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050919\
 Data File : P0056020.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 May 2019 20:18
 Operator : SM/SJ
 Sample : K2751-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Ankita
 5/13/2019 4:14:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 05:09:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.270	3.585	867785	1077000	28.998	38.133 #
2)	SA Decachlor...	9.859	8.529	572958	409647	15.313m	15.148

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050919\
Data File : PO056020.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 May 2019 20:18
Operator : SM/SJ
Sample : K2751-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
5/13/2019 4:14:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 05:09:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

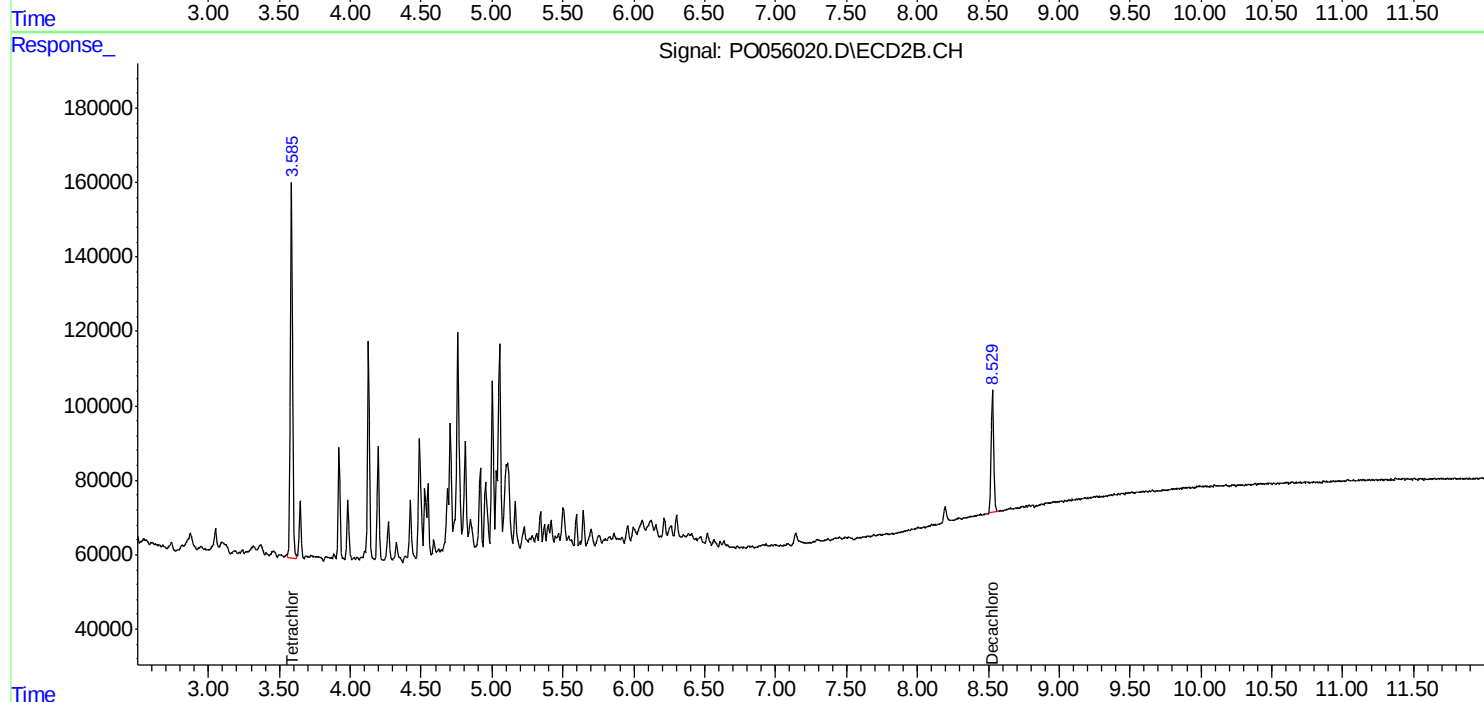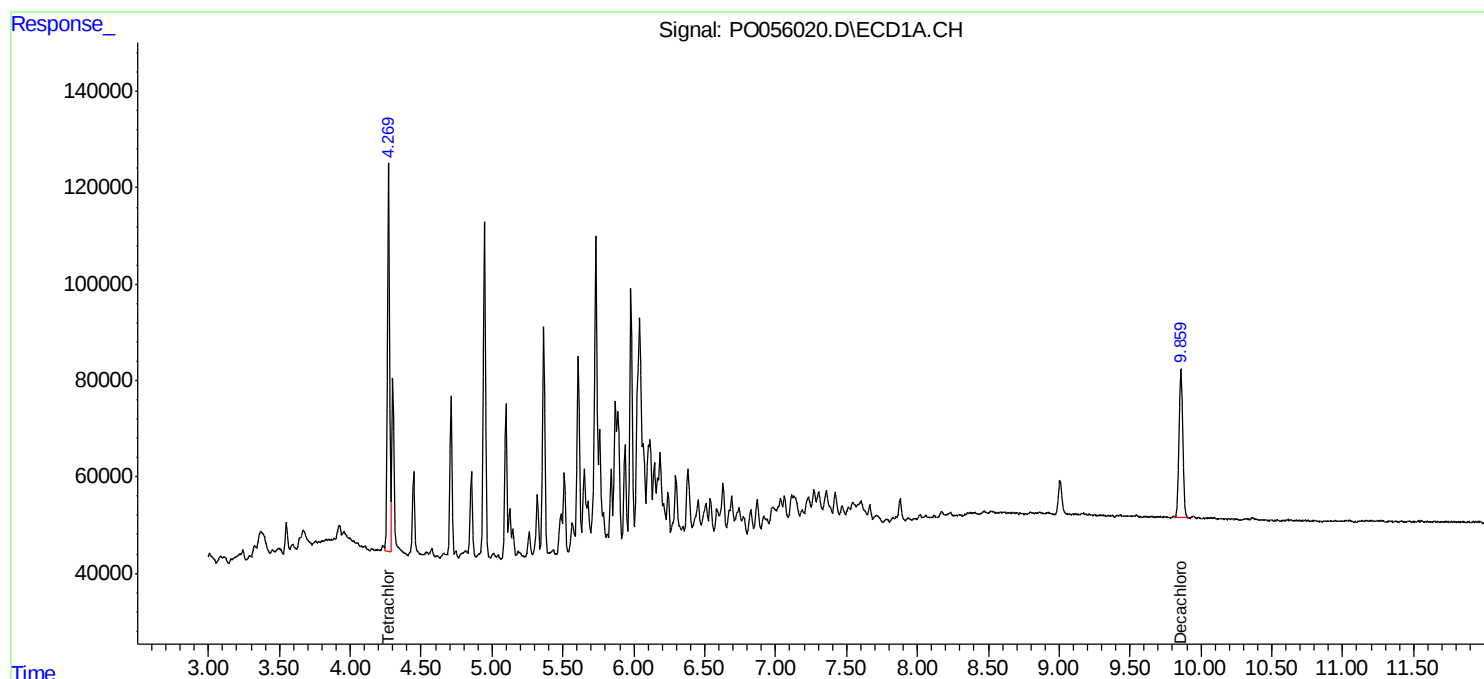

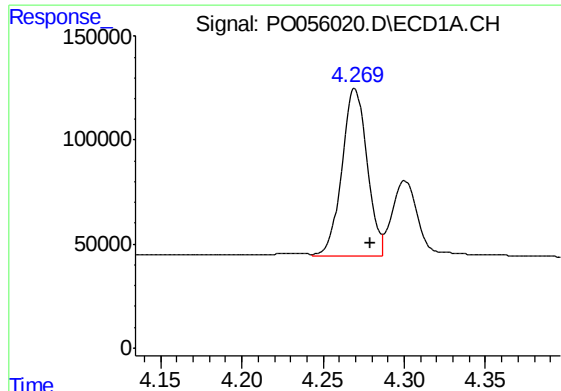


#1 Tetrachloro-m-xylene

R.T.: 4.270 min
Delta R.T.: -0.009 min
Response: 867785
Conc: 29.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
5/13/2019 4:14:34 PM

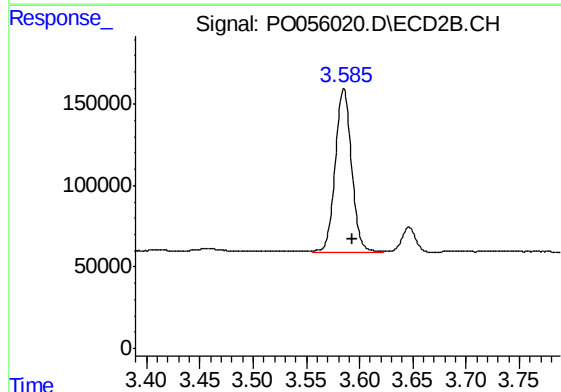


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: -0.008 min
Response: 1077000
Conc: 38.13 ng/ml

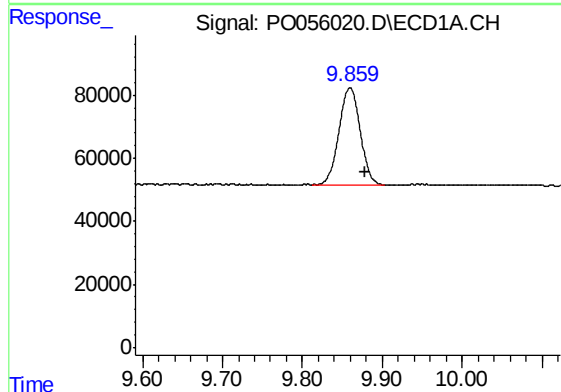

#2 Decachlorobiphenyl

R.T.: 9.859 min
Delta R.T.: -0.020 min
Response: 572958
Conc: 15.31 ng/ml m

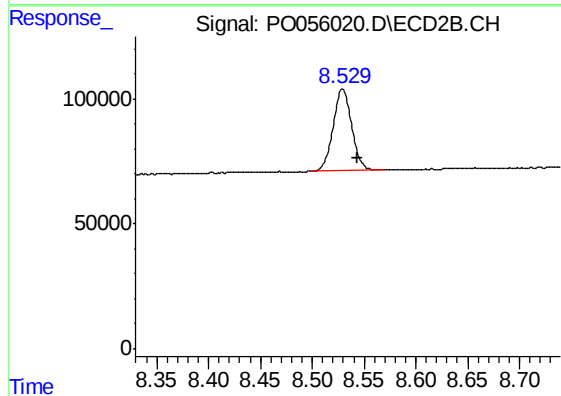

#2 Decachlorobiphenyl

R.T.: 8.529 min
Delta R.T.: -0.014 min
Response: 409647
Conc: 15.15 ng/ml