

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050919\
 Data File : P0056022.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 May 2019 20:52
 Operator : SM/SJ
 Sample : K2751-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 05:10:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.271	3.587	902191	585513	30.148	20.731 #
2)	SA Decachlor...	9.859	8.530	263277	183745	7.036	6.795

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050919\
Data File : PO056022.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 May 2019 20:52
Operator : SM/SJ
Sample : K2751-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 05:10:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

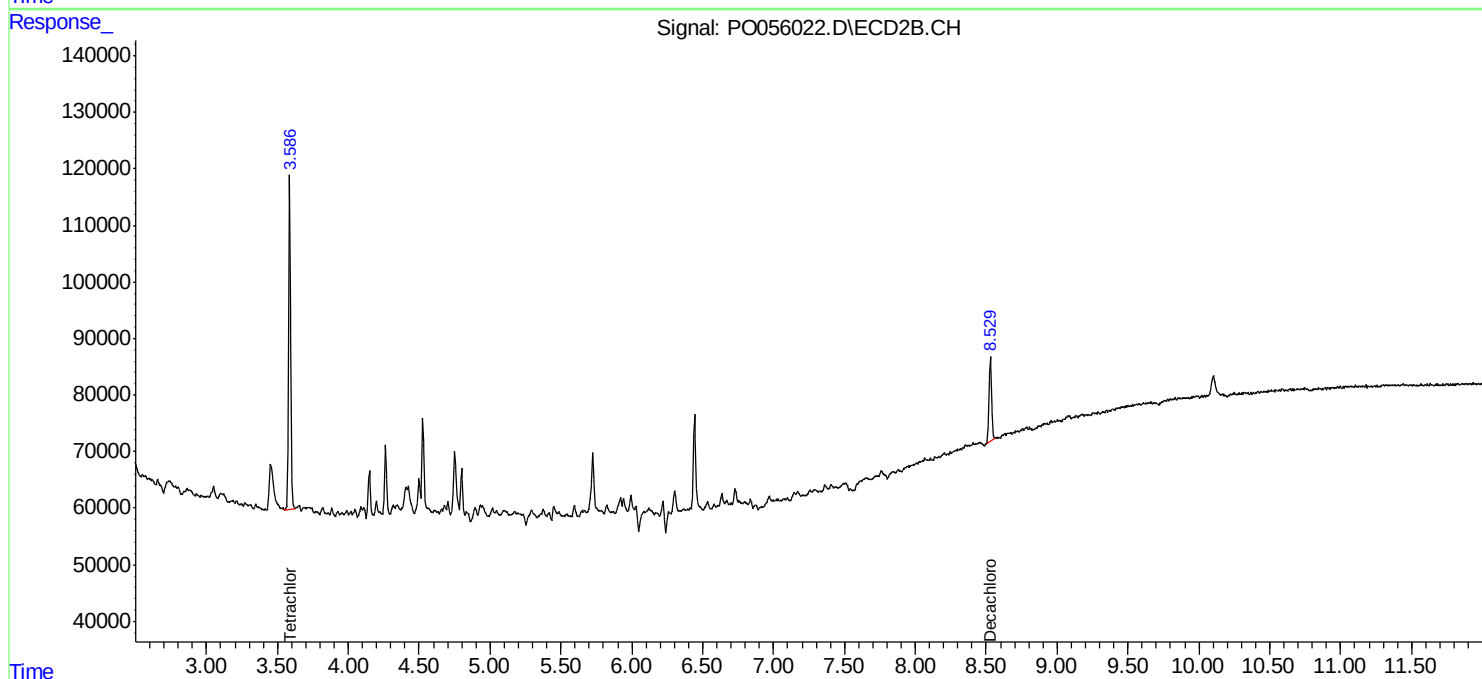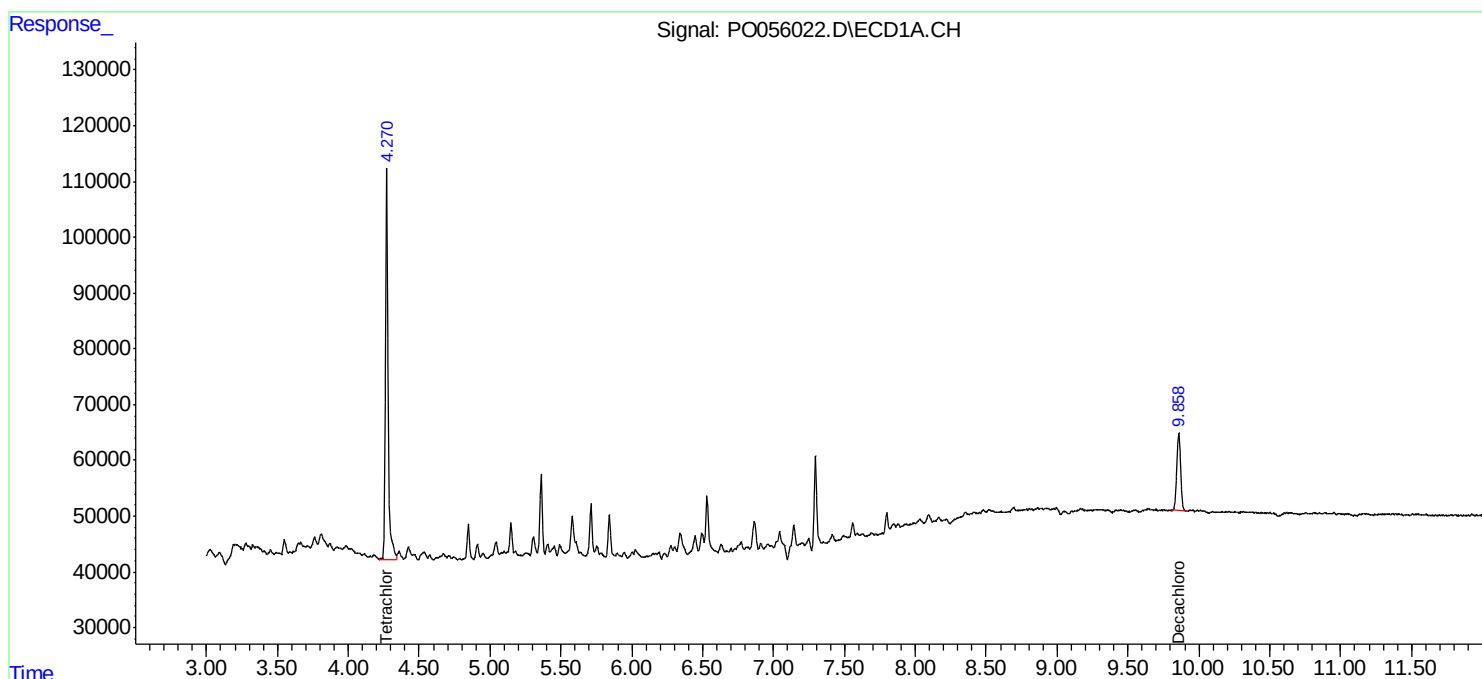


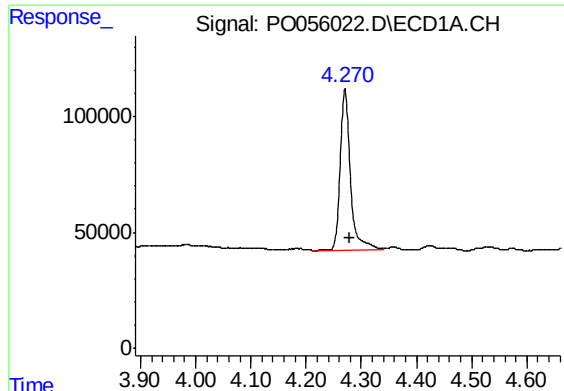

#1 Tetrachloro-m-xylene


R.T.: 4.271 min
Delta R.T.: -0.008 min
Response: 902191
Conc: 30.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2

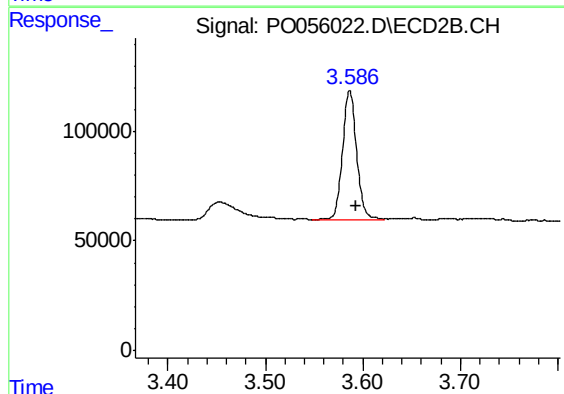


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: -0.006 min
Response: 585513
Conc: 20.73 ng/ml

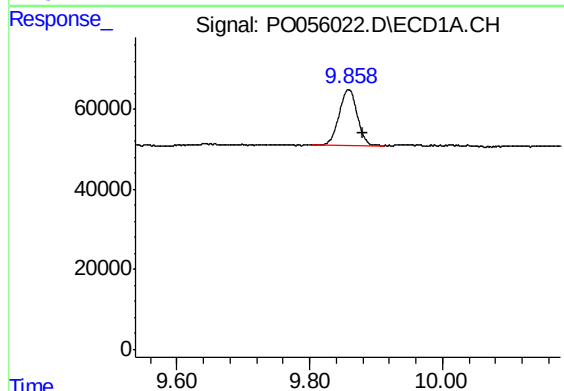

#2 Decachlorobiphenyl

R.T.: 9.859 min
Delta R.T.: -0.020 min
Response: 263277
Conc: 7.04 ng/ml

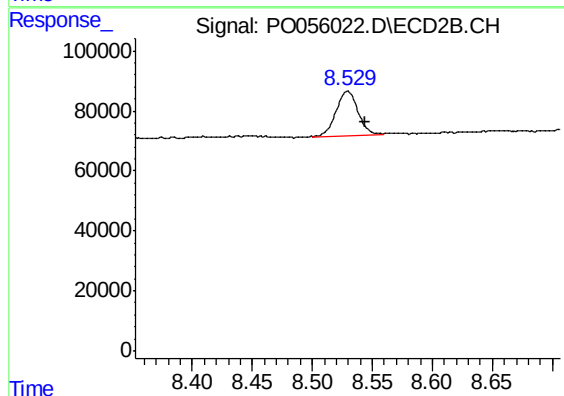

#2 Decachlorobiphenyl

R.T.: 8.530 min
Delta R.T.: -0.014 min
Response: 183745
Conc: 6.79 ng/ml