

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0050919\
 Data File : P0056028.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 May 2019 22:33
 Operator : SM/SJ
 Sample : K2749-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FR-COMP

Manual Integrations
 APPROVED

Ankita
 5/13/2019 4:14:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 05:13:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.269	3.585	661469	644555	22.104	22.821
2)	SA Decachlor...	9.857	8.529	577224	410329	15.427	15.173
Target Compounds							
31)	L7 AR-1260-1	7.018	6.122	45600	52404	21.116	23.786
32)	L7 AR-1260-2	7.276	6.308	67254	73845	25.680	24.183m
33)	L7 AR-1260-3	7.632	6.461	40312	60760	20.156	24.382m
34)	L7 AR-1260-4	7.856	6.929	55098	43929	23.825	21.289
35)	L7 AR-1260-5	8.165	7.169	96539	105305	22.756	20.968

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO050919\
Data File : PO056028.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 May 2019 22:33
Operator : SM/SJ
Sample : K2749-05
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FR-COMP


Manual Integrations
APPROVED

Ankita
5/13/2019 4:14:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 05:13:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

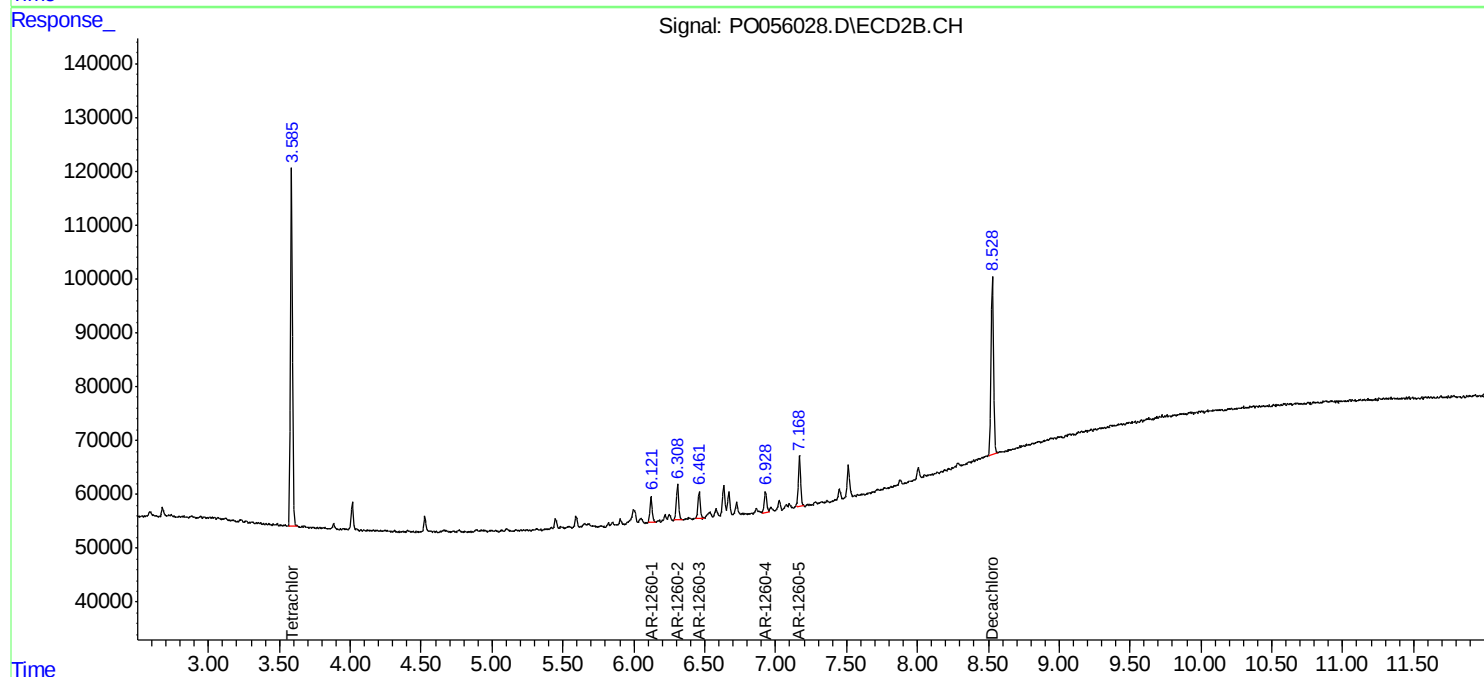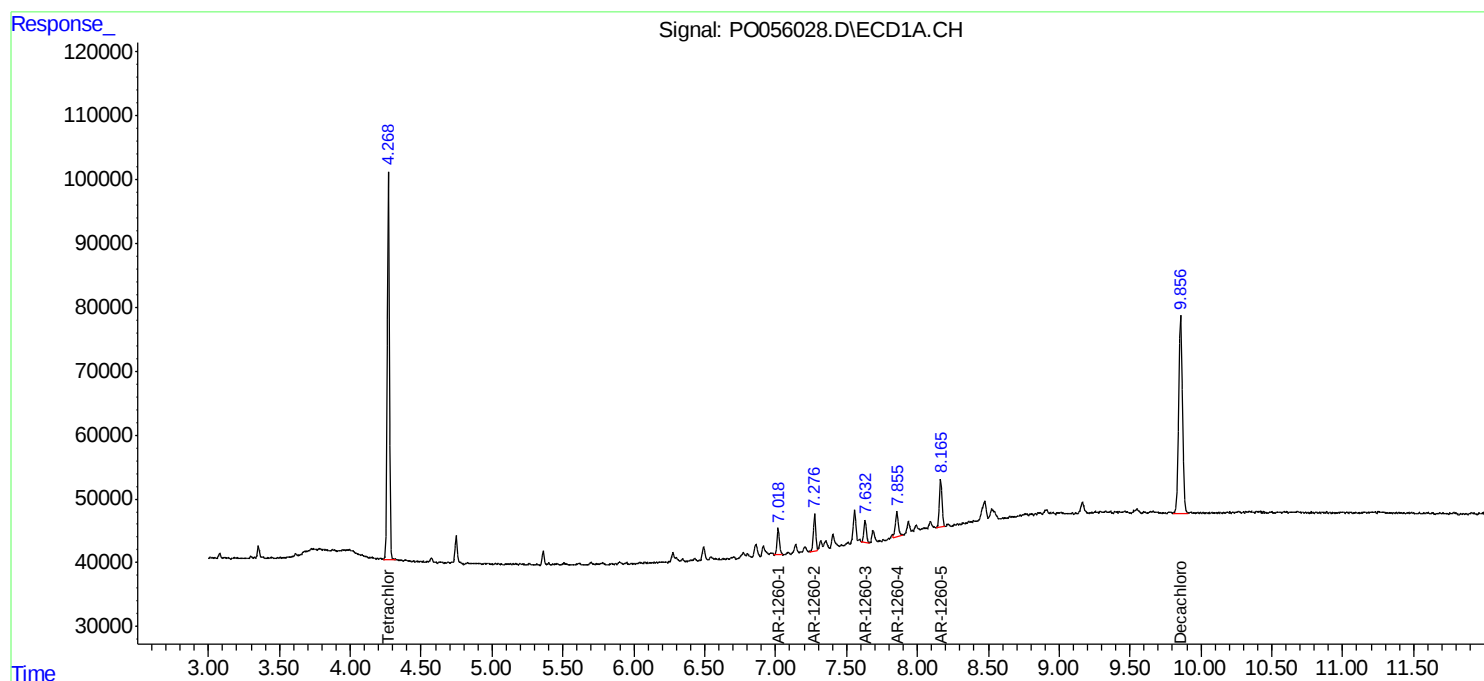

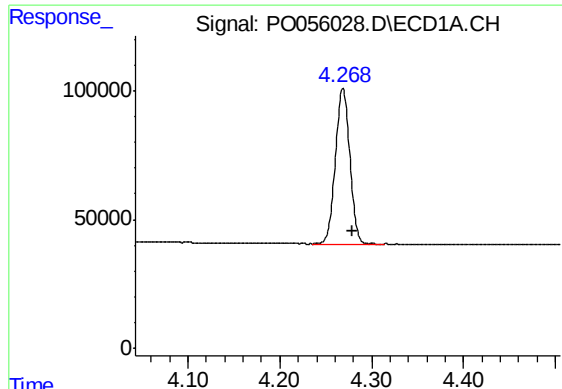


#1 Tetrachloro-m-xylene

R.T.: 4.269 min
Delta R.T.: -0.010 min
Response: 661469
Conc: 22.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FR-COMP


Manual Integrations
APPROVED

Ankita
5/13/2019 4:14:39 PM

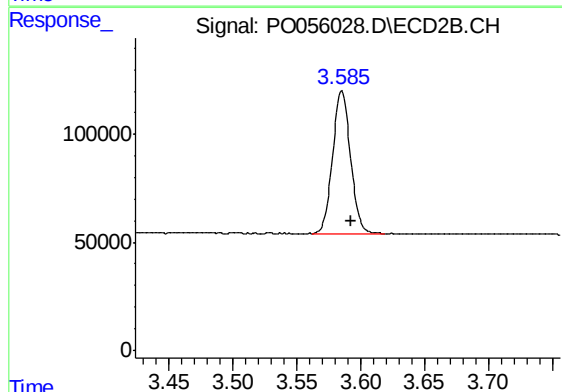


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: -0.008 min
Response: 644555
Conc: 22.82 ng/ml

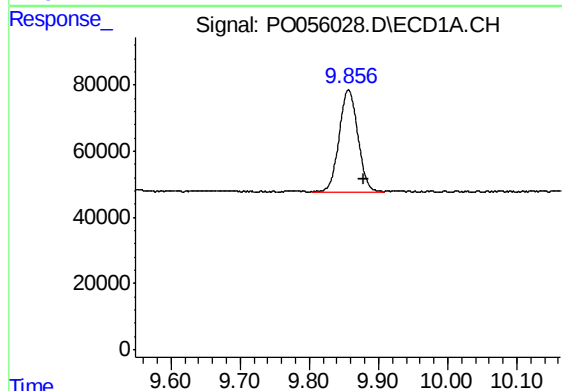


#2 Decachlorobiphenyl

R.T.: 9.857 min
Delta R.T.: -0.022 min
Response: 577224
Conc: 15.43 ng/ml

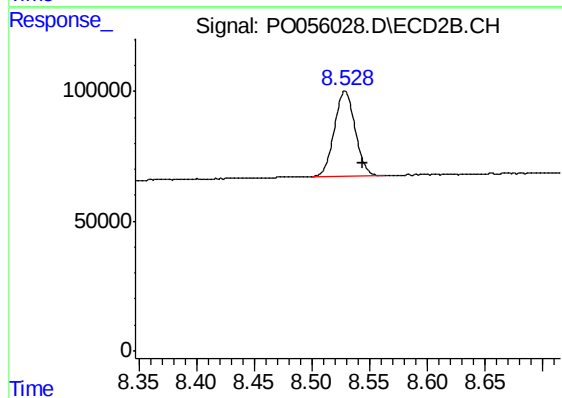

#2 Decachlorobiphenyl

R.T.: 8.529 min
Delta R.T.: -0.015 min
Response: 410329
Conc: 15.17 ng/ml

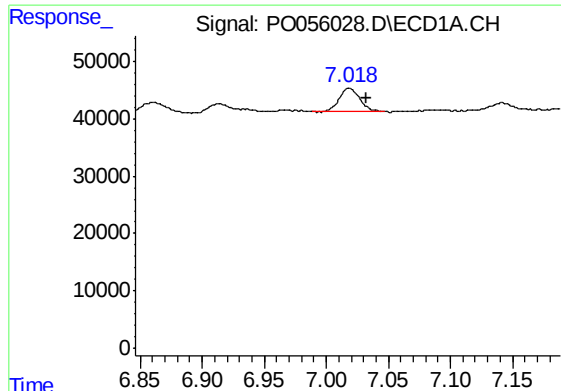


#31 AR-1260-1

R.T.: 7.018 min
Delta R.T.: -0.014 min
Response: 45600
Conc: 21.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
FR-COMP


Manual Integrations
APPROVED

Ankita
5/13/2019 4:14:39 PM

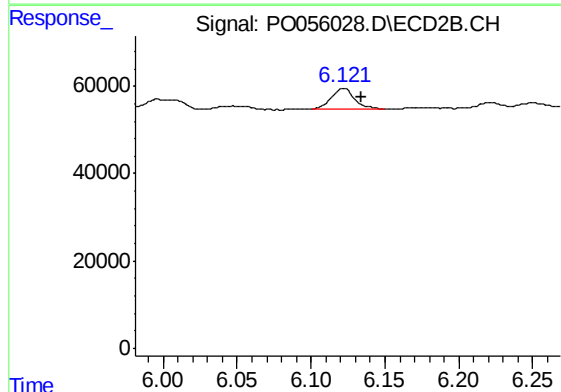


#31 AR-1260-1

R.T.: 6.122 min
Delta R.T.: -0.012 min
Response: 52404
Conc: 23.79 ng/ml

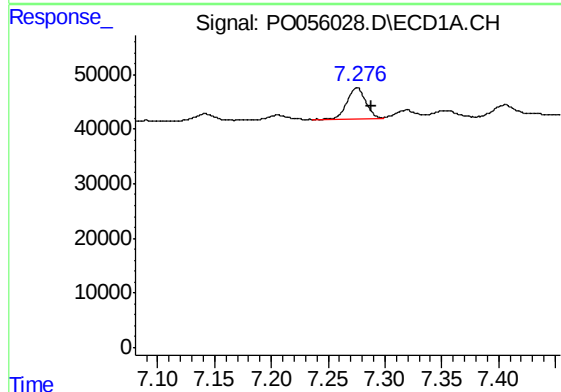


#32 AR-1260-2

R.T.: 7.276 min
Delta R.T.: -0.012 min
Response: 67254
Conc: 25.68 ng/ml

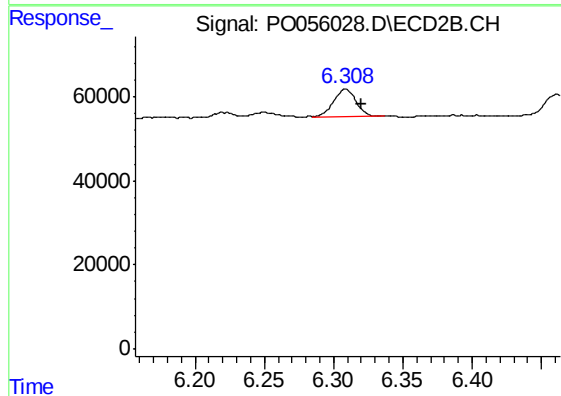

#32 AR-1260-2

R.T.: 6.308 min
Delta R.T.: -0.012 min
Response: 73845
Conc: 24.18 ng/ml m

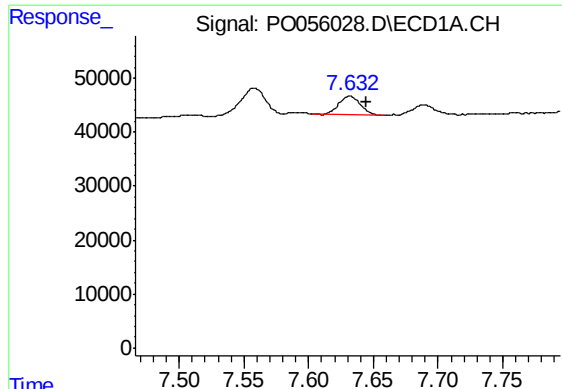


#33 AR-1260-3

R.T.: 7.632 min
Delta R.T.: -0.013 min
Response: 40312
Conc: 20.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FR-COMP


Manual Integrations
APPROVED

Ankita
5/13/2019 4:14:39 PM

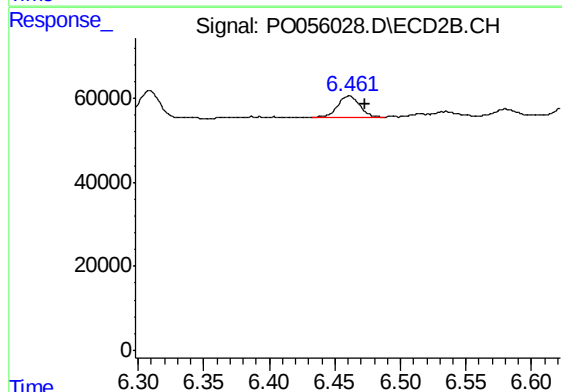


#33 AR-1260-3

R.T.: 6.461 min
Delta R.T.: -0.012 min
Response: 60760
Conc: 24.38 ng/ml m

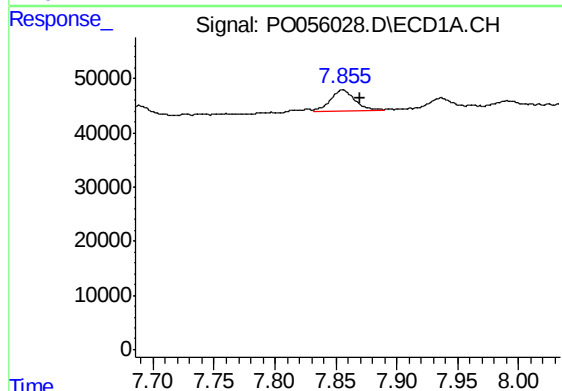


#34 AR-1260-4

R.T.: 7.856 min
Delta R.T.: -0.015 min
Response: 55098
Conc: 23.82 ng/ml

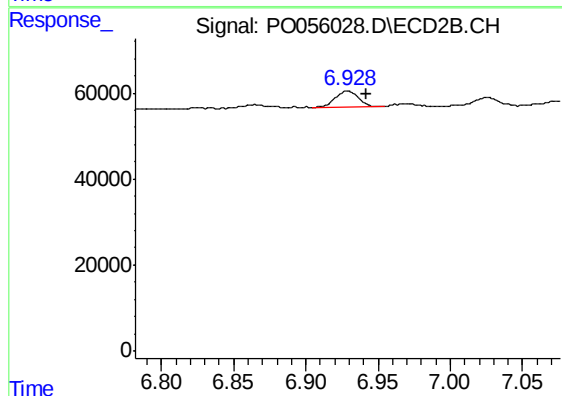

#34 AR-1260-4

R.T.: 6.929 min
Delta R.T.: -0.013 min
Response: 43929
Conc: 21.29 ng/ml

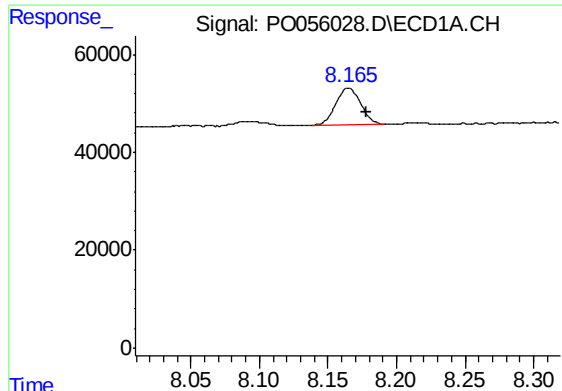


#35 AR-1260-5

R.T.: 8.165 min
Delta R.T.: -0.014 min
Response: 96539
Conc: 22.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
FR-COMP

Manual Integrations
APPROVED

Ankita
5/13/2019 4:14:39 PM

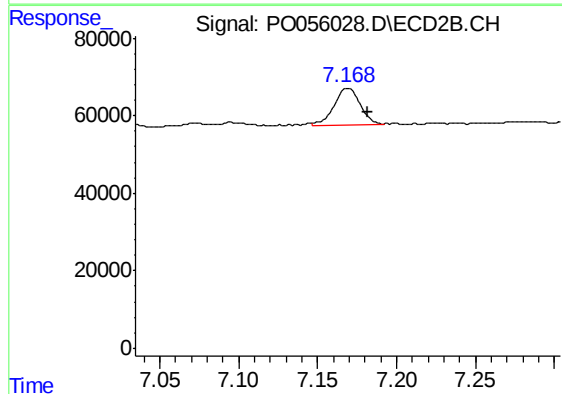

#35 AR-1260-5

R.T.: 7.169 min
Delta R.T.: -0.013 min
Response: 105305
Conc: 20.97 ng/ml