

Data Path : P:\HPCHEM1\ECD_0\Data\P0051018\
Data File : P0044571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2018 16:19
Operator : SM/UA
Sample : J2790-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-SF-01-004-A

Manual Integrations
APPROVED

ugo
5/11/2018 11:54:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 17:41:25 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.045	3.300	6179852	7484203	30.720	27.638m
2) SA Decachlor...	9.374	8.048	3472771	3757120	23.917	21.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0051018\
Data File : P0044571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2018 16:19
Operator : SM/UA
Sample : J2790-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-SF-01-004-A


Manual Integrations
APPROVED

ugo
5/11/2018 11:54:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 17:41:25 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

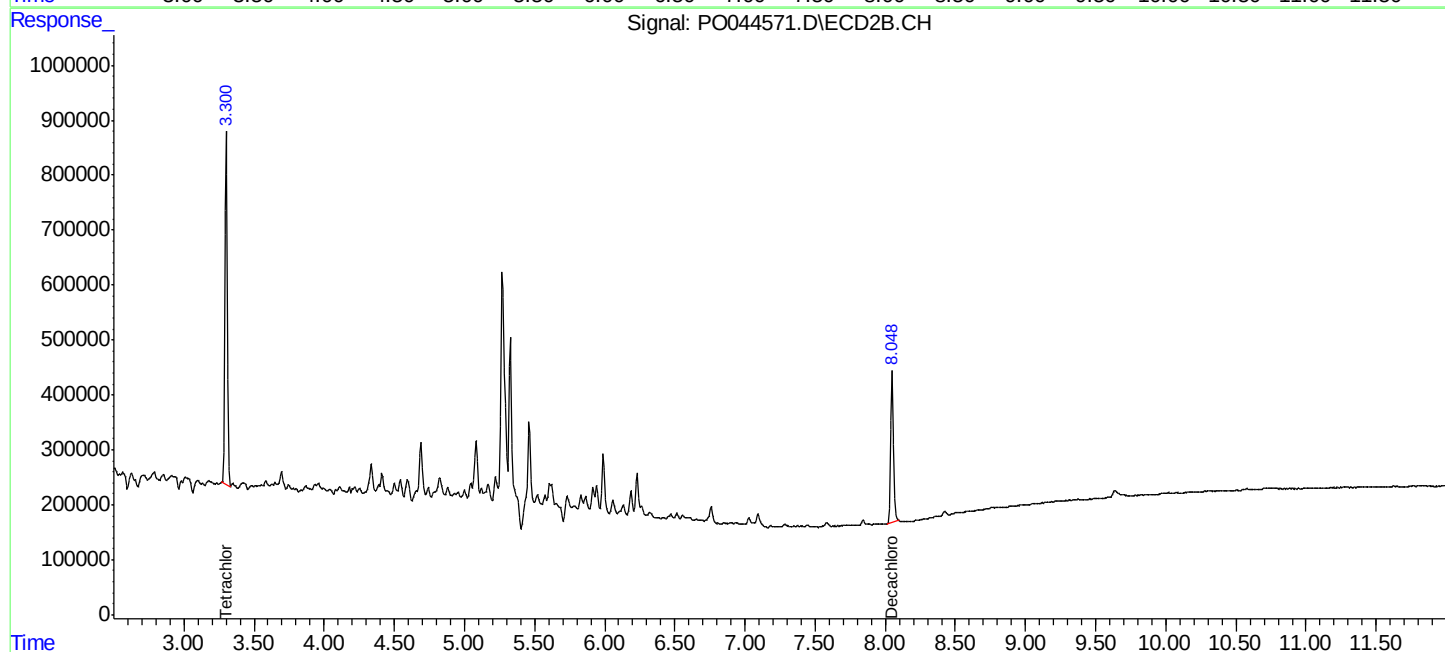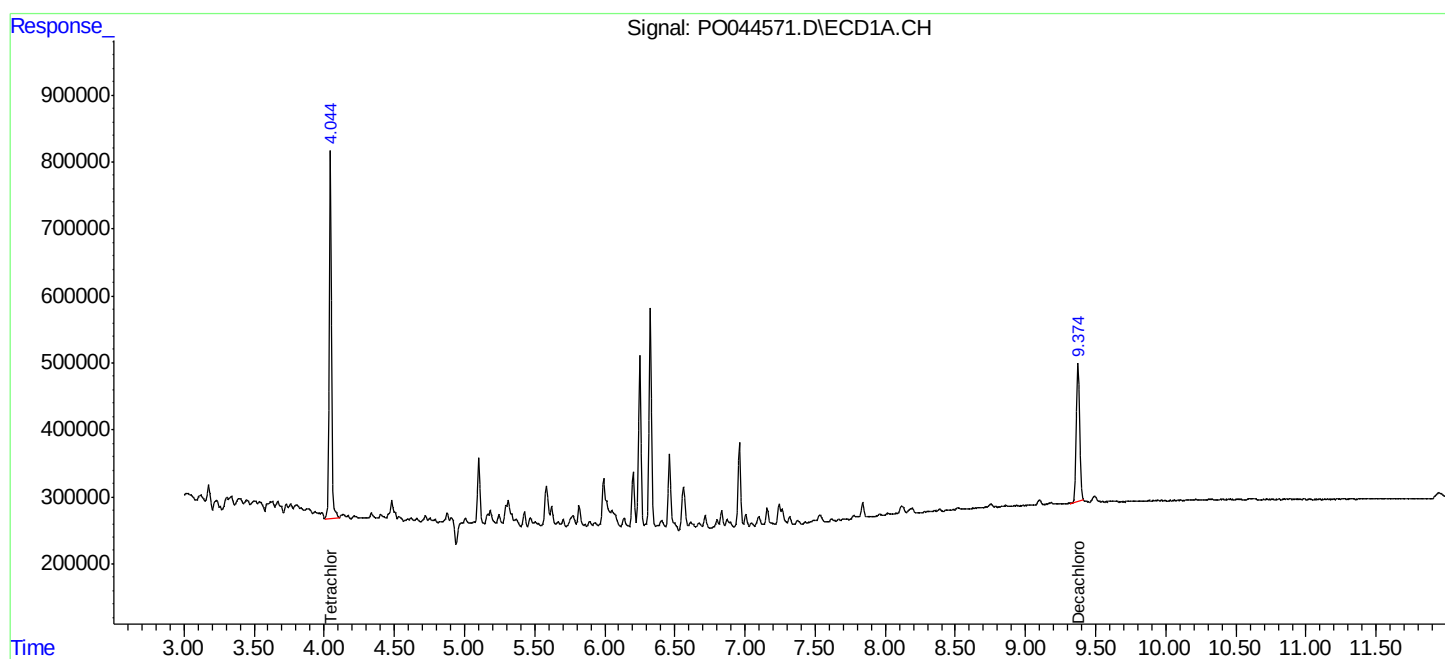

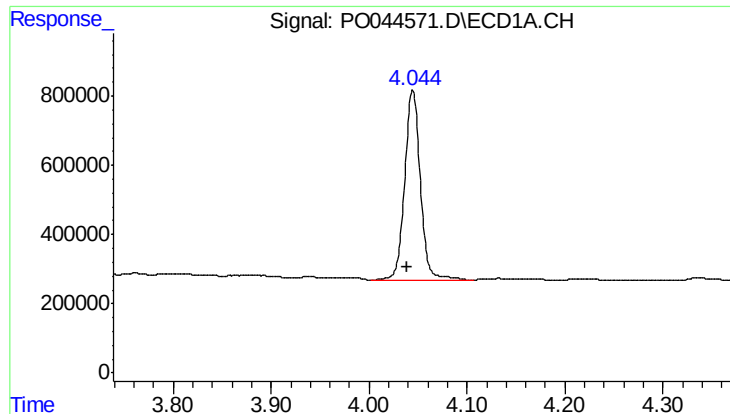


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.006 min
Response: 6179852
Conc: 30.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-01-004-A


Manual Integrations
APPROVED

ugo
5/11/2018 11:54:47 AM

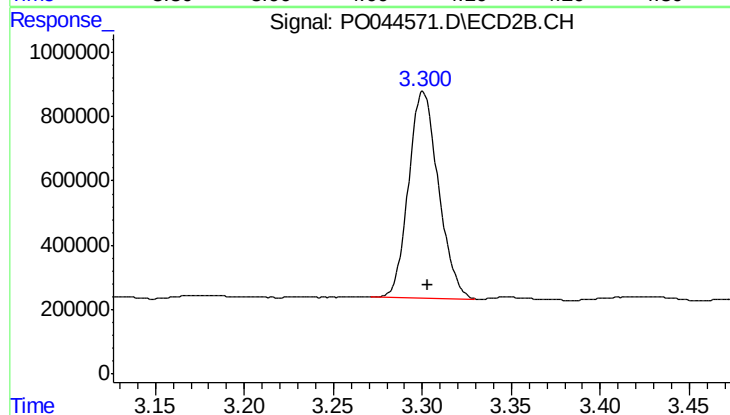


#1 Tetrachloro-m-xylene

R.T.: 3.300 min
Delta R.T.: -0.003 min
Response: 7484203
Conc: 27.64 ng/ml m

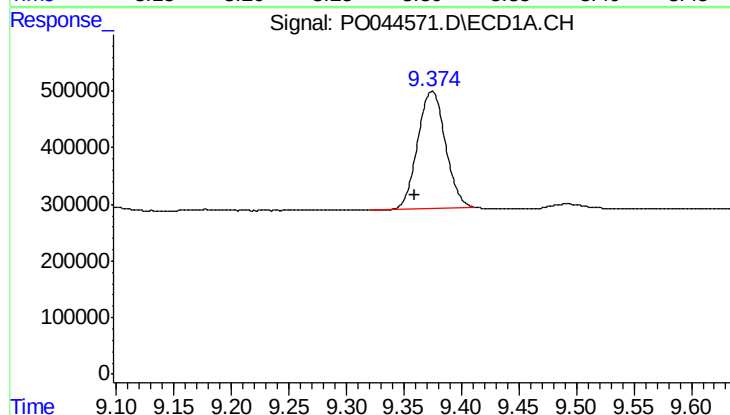

#2 Decachlorobiphenyl

R.T.: 9.374 min
Delta R.T.: 0.015 min
Response: 3472771
Conc: 23.92 ng/ml

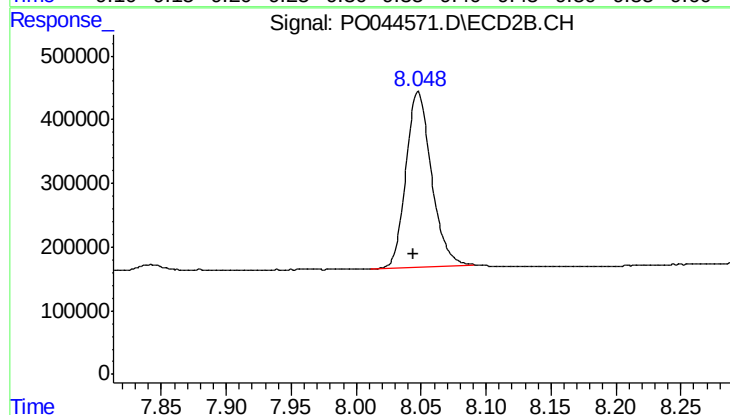

#2 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.004 min
Response: 3757120
Conc: 21.50 ng/ml