

Data Path : P:\HPCHEM1\ECD_0\Data\P0051018\
Data File : P0044581.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2018 18:53
Operator : SM/UA
Sample : J2783-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BS-CONCRETE-RO-277

Manual Integrations
APPROVED

ugo
5/11/2018 11:54:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 19:36:39 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.038	3.306	2484321	2560966	12.349m	9.457
2) SA Decachlor...	9.359	8.044	2322176	2290563	15.993	13.111

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0051018\
Data File : P0044581.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2018 18:53
Operator : SM/UA
Sample : J2783-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BS-CONCRETE-RO-277


Manual Integrations
APPROVED

ugo
5/11/2018 11:54:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 19:36:39 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

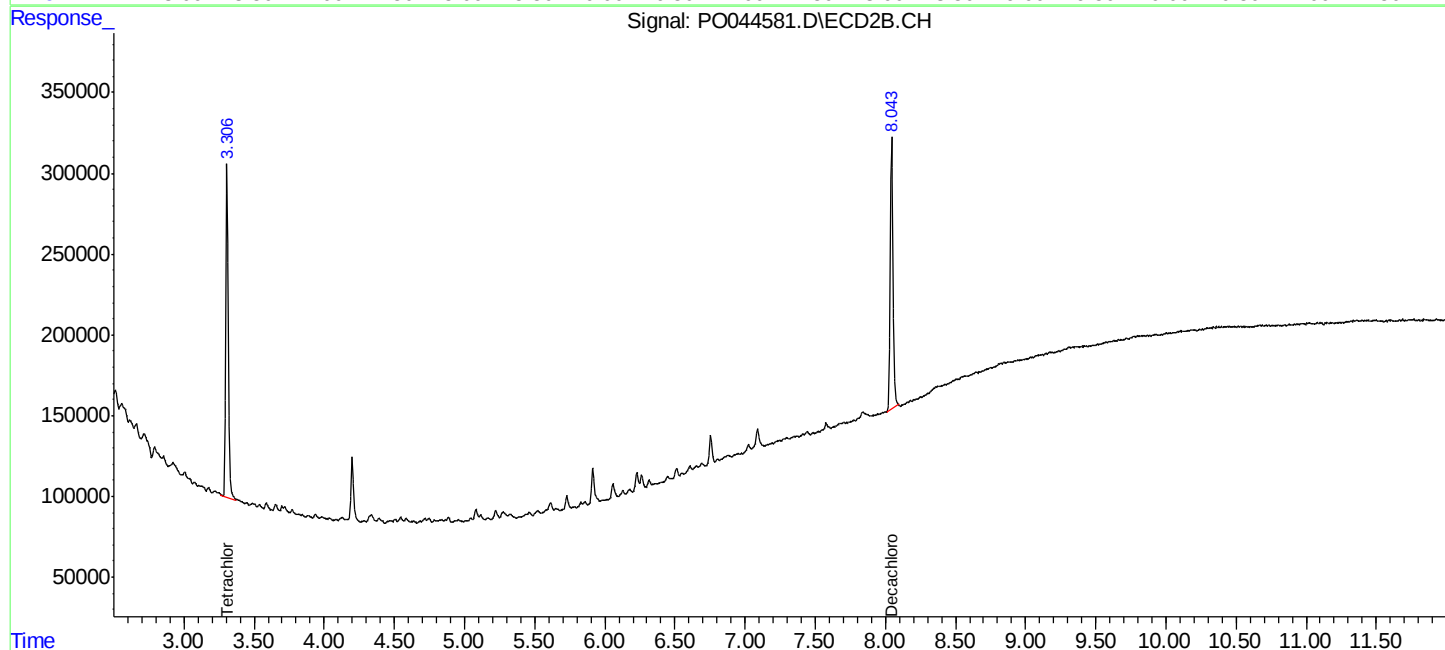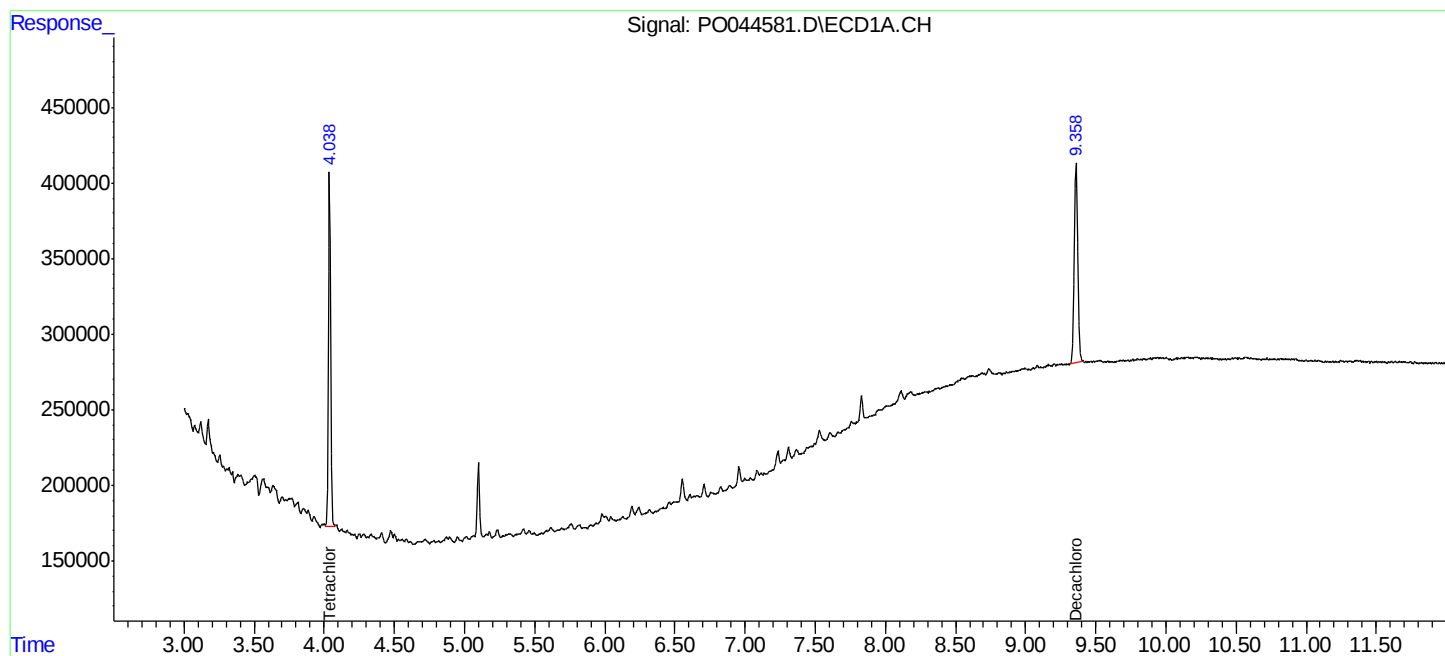

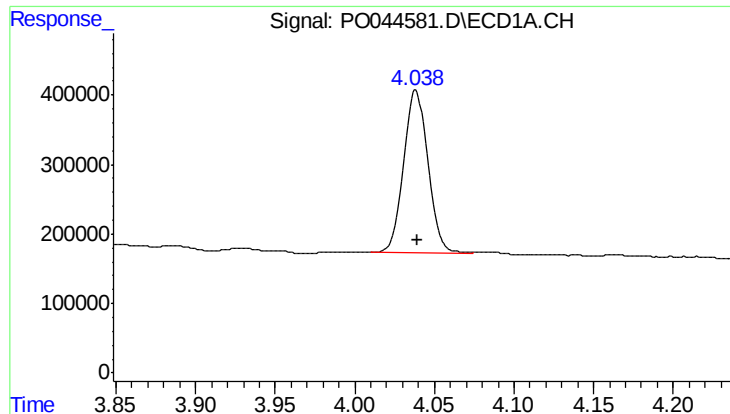


#1 Tetrachloro-m-xylene

R.T.: 4.038 min
Delta R.T.: -0.001 min
Response: 2484321
Conc: 12.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
BS-CONCRETE-RO-277


Manual Integrations
APPROVED

ugo
5/11/2018 11:54:24 AM

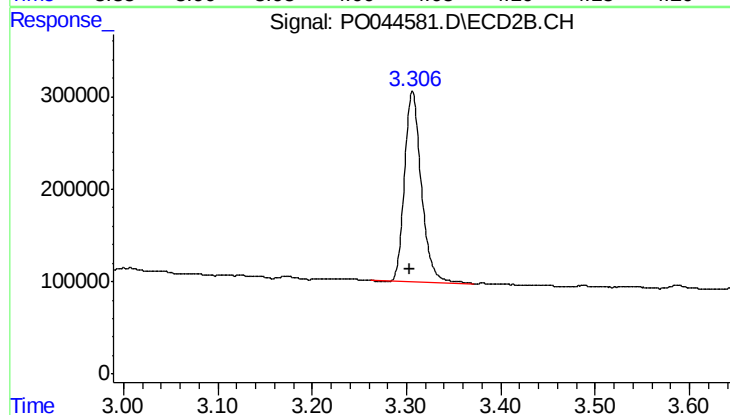


#1 Tetrachloro-m-xylene

R.T.: 3.306 min
Delta R.T.: 0.003 min
Response: 2560966
Conc: 9.46 ng/ml

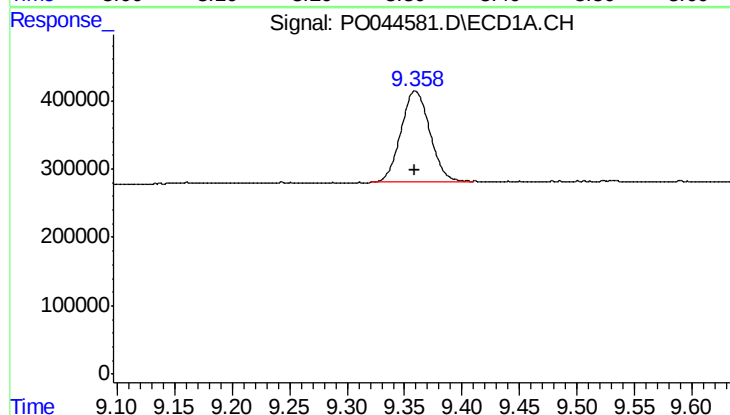

#2 Decachlorobiphenyl

R.T.: 9.359 min
Delta R.T.: 0.000 min
Response: 2322176
Conc: 15.99 ng/ml

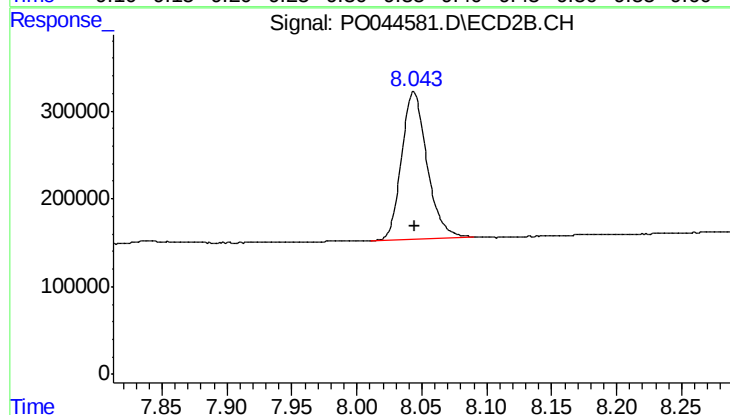

#2 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: 0.000 min
Response: 2290563
Conc: 13.11 ng/ml