

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051019\
Data File : P0056073.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2019 17:46
Operator : SM/SJ
Sample : K2751-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
30121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 02:37:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.268	3.585	840689	762326	28.093	26.991
2)	SA Decachlor...	9.860	8.529	741460	513298	19.816	18.981

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051019\
Data File : PO056073.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2019 17:46
Operator : SM/SJ
Sample : K2751-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
30121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 02:37:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

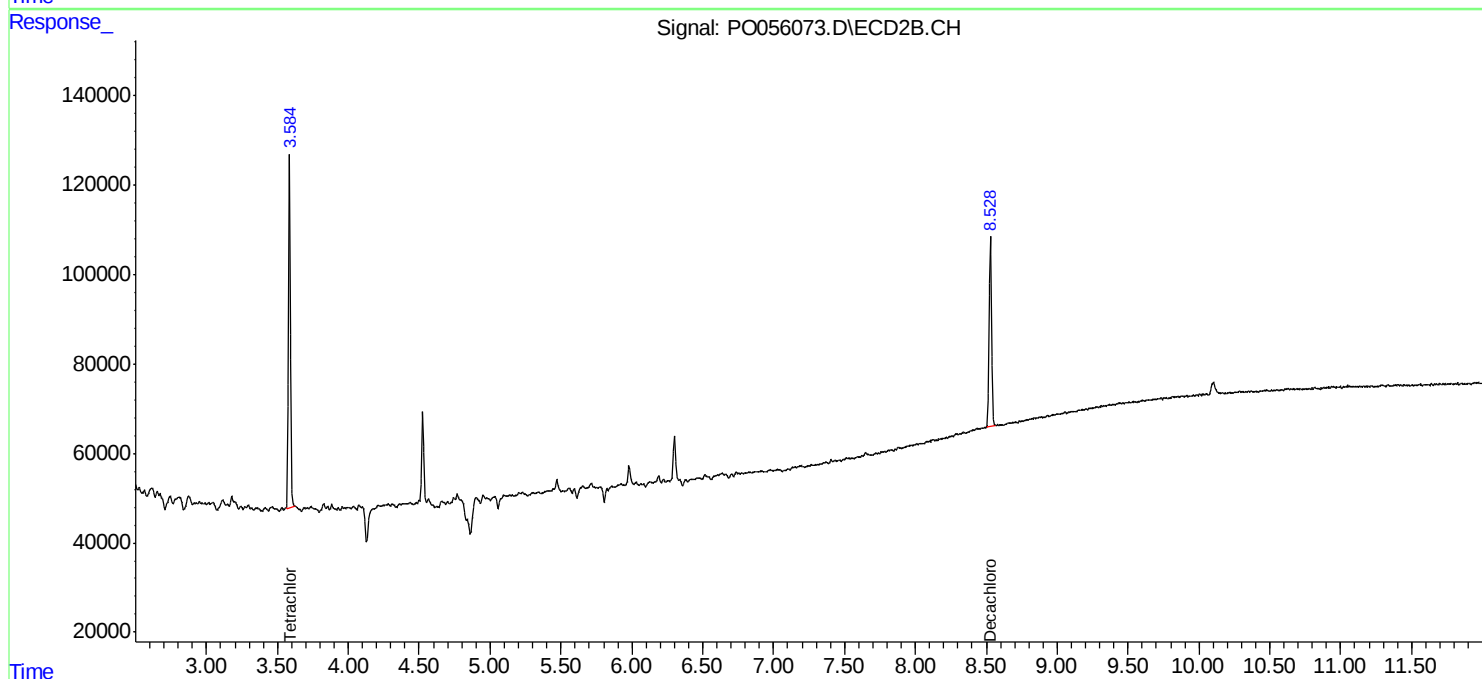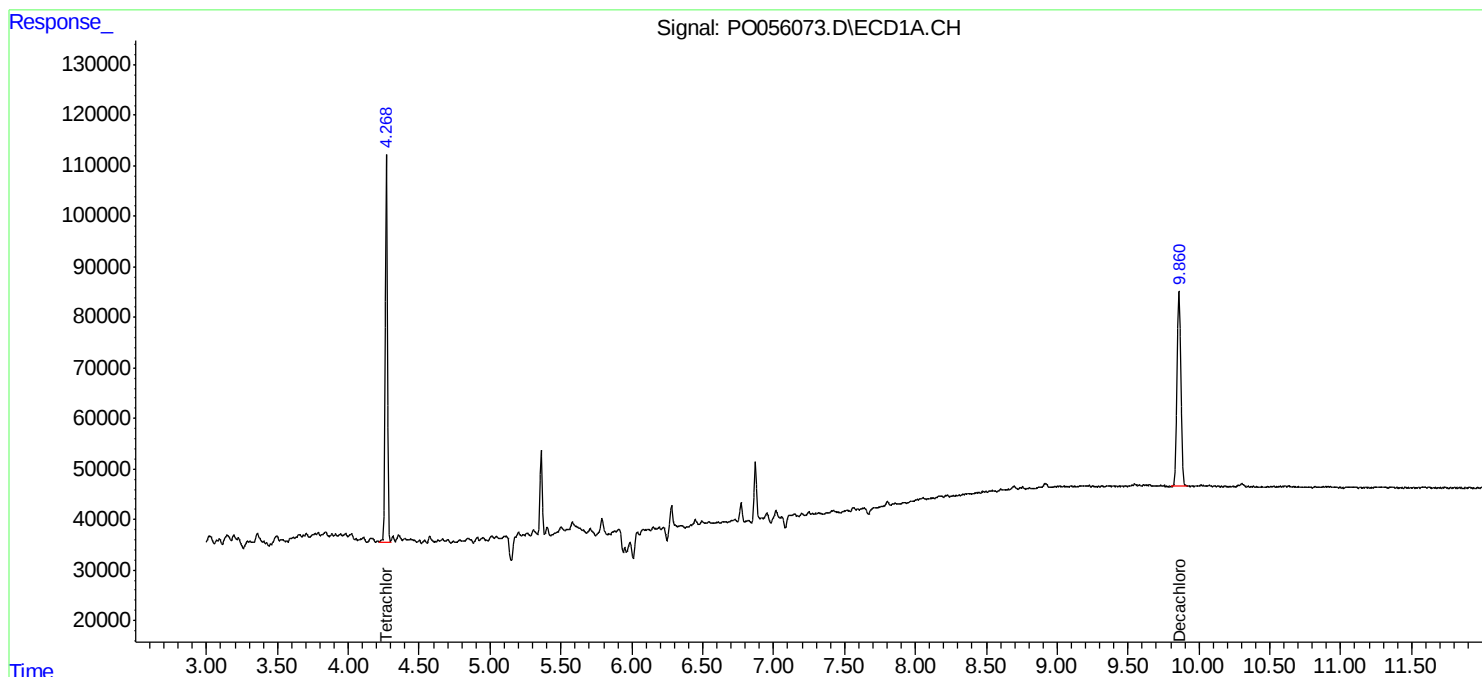


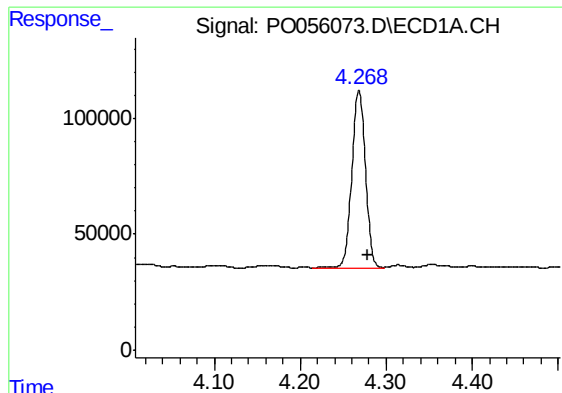

#1 Tetrachloro-m-xylene


R.T.: 4.268 min
Delta R.T.: -0.011 min
Response: 840689
Conc: 28.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
30121

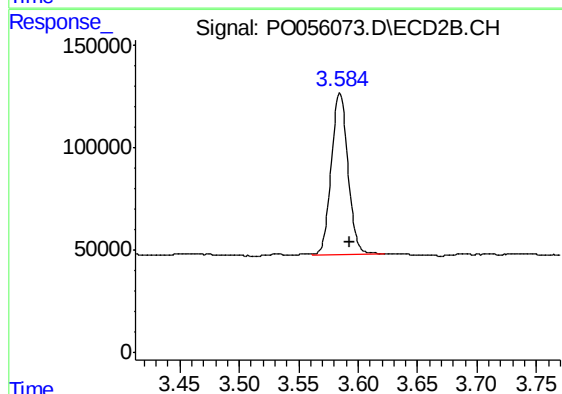


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: -0.008 min
Response: 762326
Conc: 26.99 ng/ml

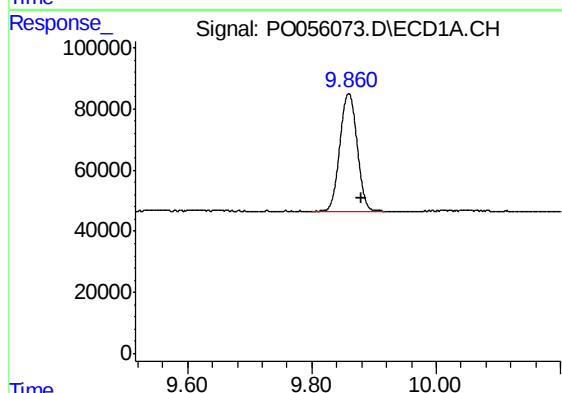

#2 Decachlorobiphenyl

R.T.: 9.860 min
Delta R.T.: -0.019 min
Response: 741460
Conc: 19.82 ng/ml

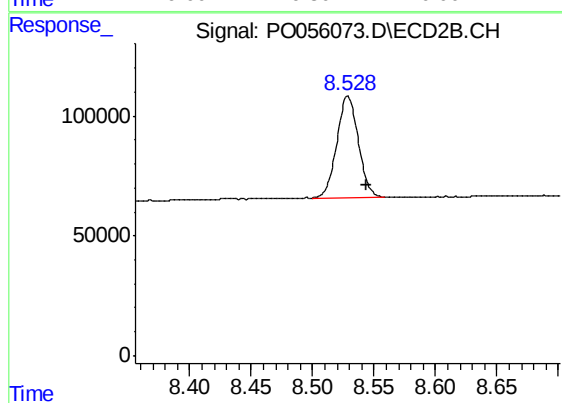

#2 Decachlorobiphenyl

R.T.: 8.529 min
Delta R.T.: -0.015 min
Response: 513298
Conc: 18.98 ng/ml