

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051019\
 Data File : P0056074.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 May 2019 18:03
 Operator : SM/SJ
 Sample : K2752-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 13:16:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.268	3.585	718045	694950	23.994	24.606
2) SA Decachlor...	9.860	8.530	571080	395621	15.263	14.629

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051019\
Data File : PO056074.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2019 18:03
Operator : SM/SJ
Sample : K2752-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 13:16:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

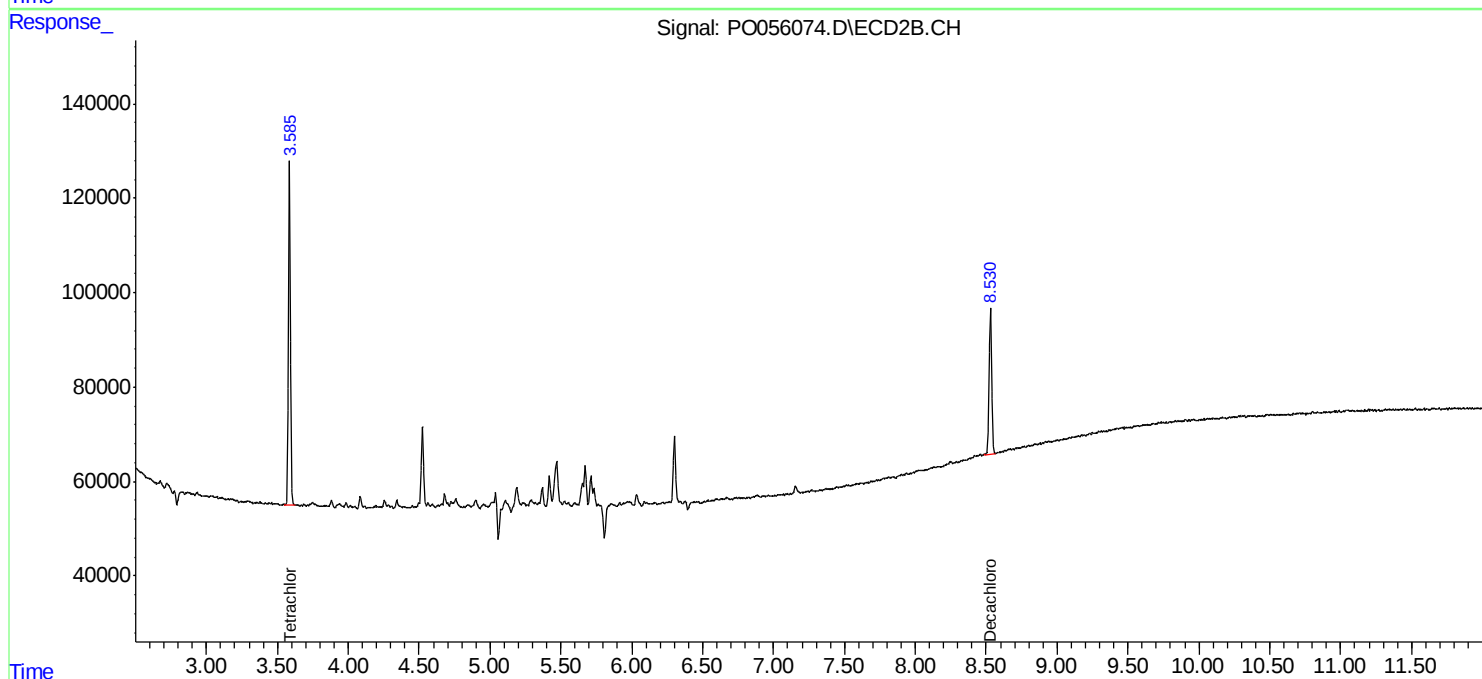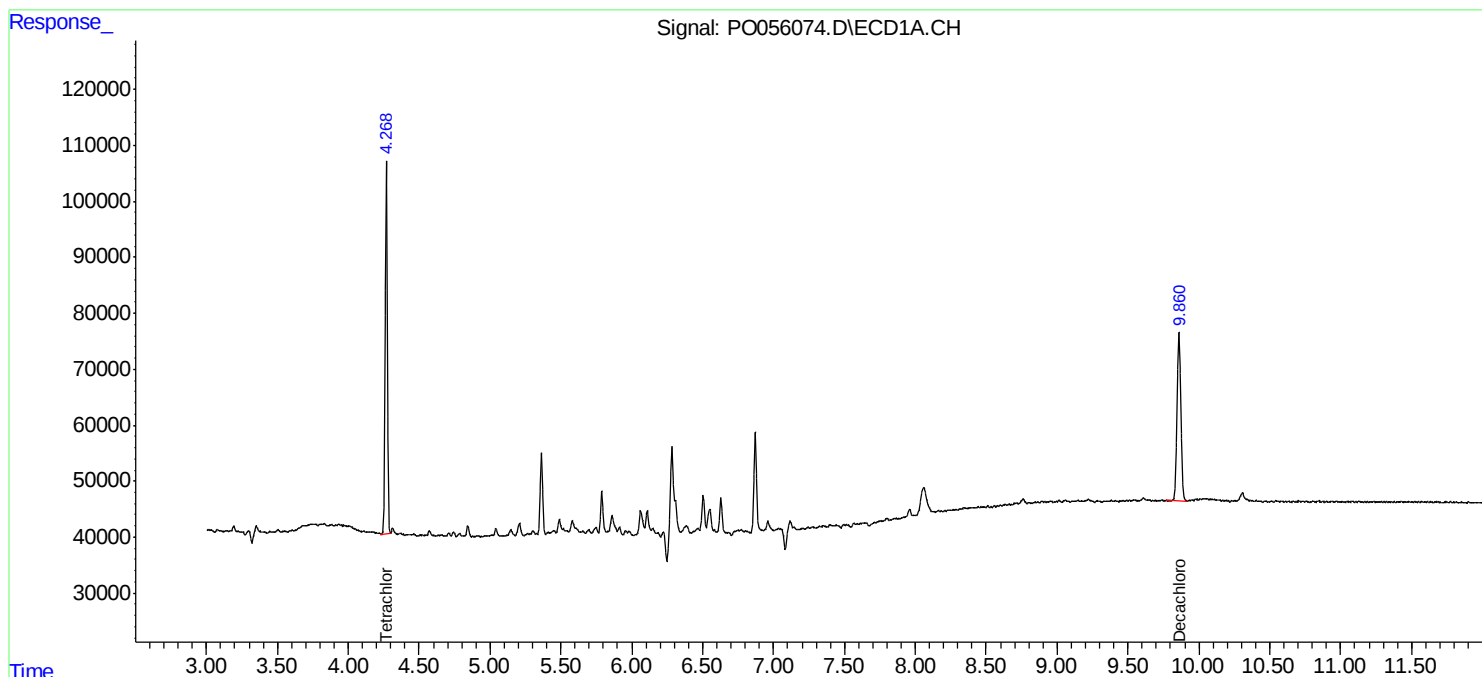


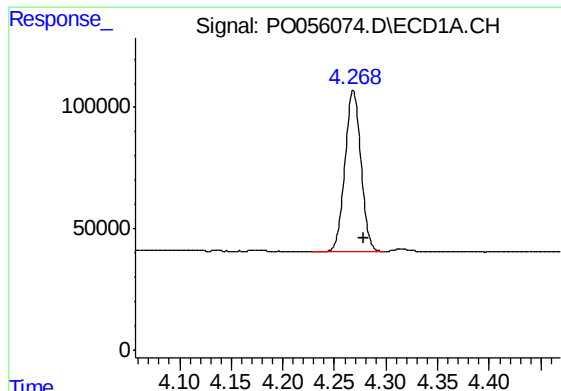

#1 Tetrachloro-m-xylene


R.T.: 4.268 min
Delta R.T.: -0.011 min
Response: 718045
Conc: 23.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-4

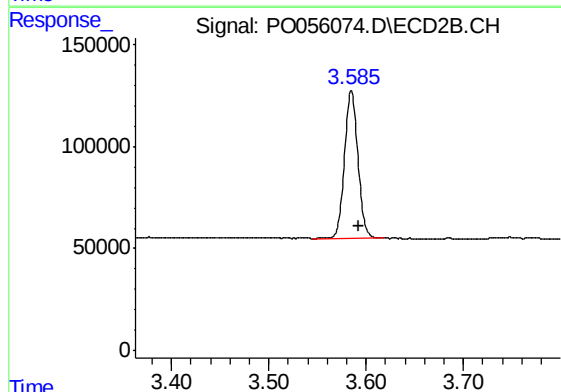


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: -0.008 min
Response: 694950
Conc: 24.61 ng/ml

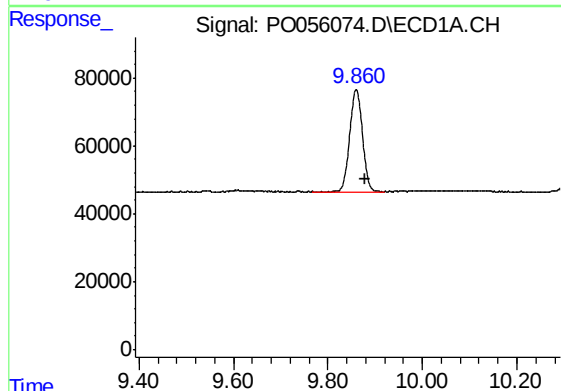

#2 Decachlorobiphenyl

R.T.: 9.860 min
Delta R.T.: -0.019 min
Response: 571080
Conc: 15.26 ng/ml

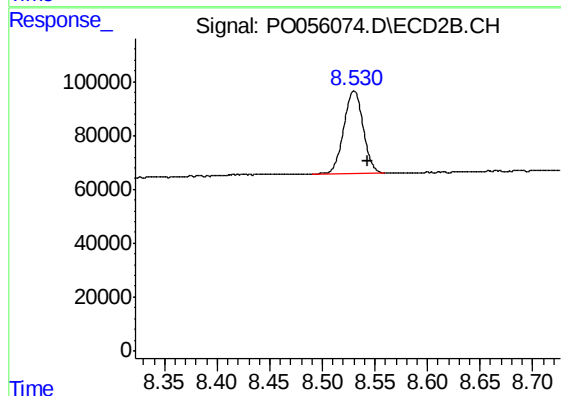

#2 Decachlorobiphenyl

R.T.: 8.530 min
Delta R.T.: -0.013 min
Response: 395621
Conc: 14.63 ng/ml