

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051019\
 Data File : P0056075.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 May 2019 18:20
 Operator : SM/SJ
 Sample : K2746-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-5.8.19

Manual Integrations
 APPROVED

Ankita
 5/13/2019 2:04:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 02:38:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.268	3.583	1021604	998846	34.138	35.366
2)	SA Decachlor...	9.859	8.529	1017178	726352	27.185	26.859
Target Compounds							
31)	L7 AR-1260-1	7.058	6.122	62098	153014	28.756	69.451 #
32)	L7 AR-1260-2	7.275	6.306	176195	239392	67.278	78.397m
33)	L7 AR-1260-3	7.632	6.460	93079	124789	46.540	50.075m
34)	L7 AR-1260-4	7.855	6.928	126676	73402	54.776	35.572 #
35)	L7 AR-1260-5	8.166	7.170	170182	245391	40.115	48.861

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051019\
Data File : PO056075.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2019 18:20
Operator : SM/SJ
Sample : K2746-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19


Manual Integrations
APPROVED

Ankita
5/13/2019 2:04:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 02:38:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

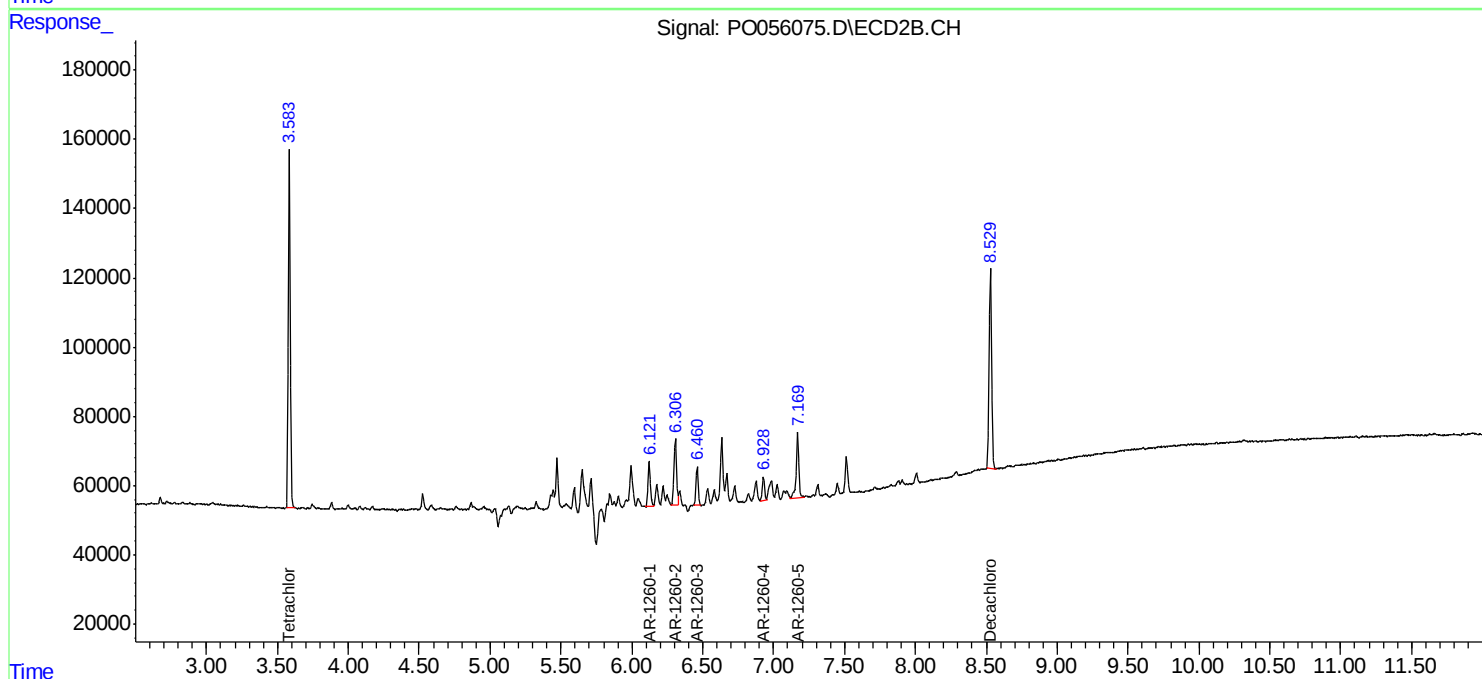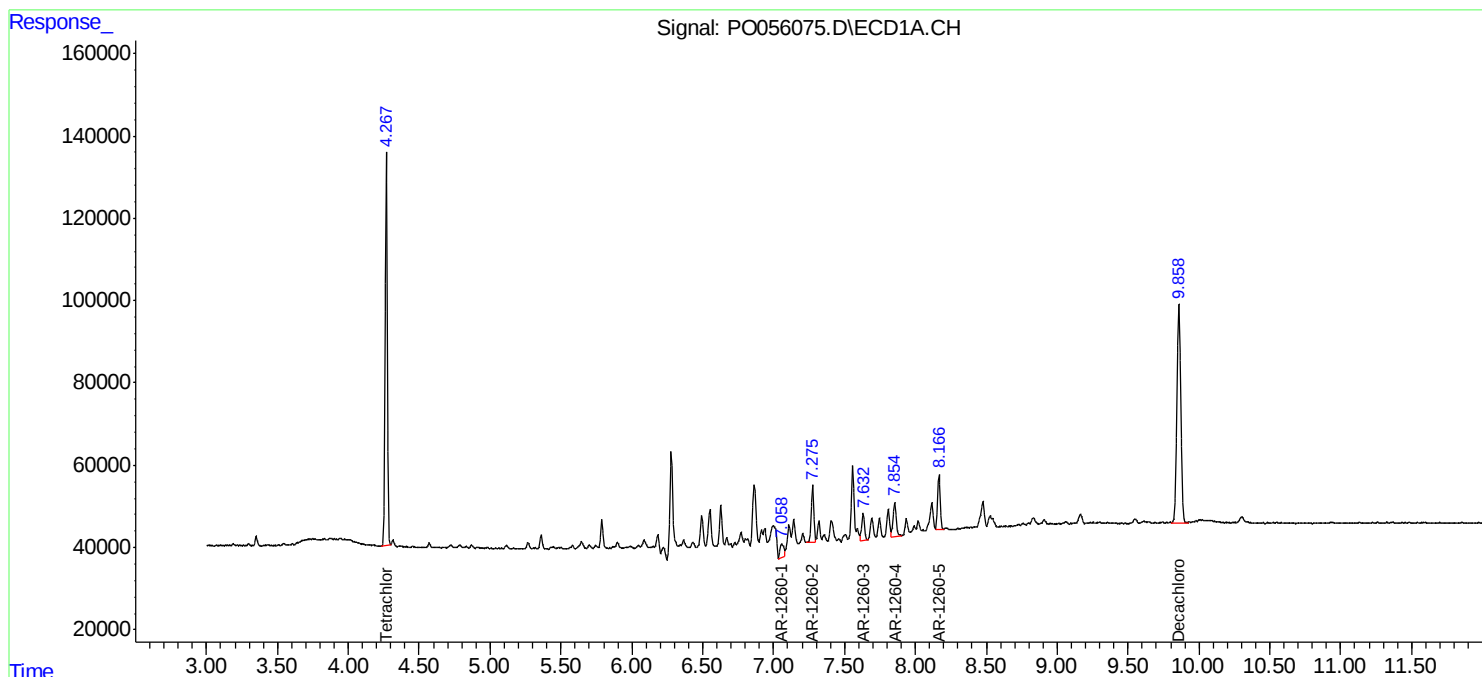

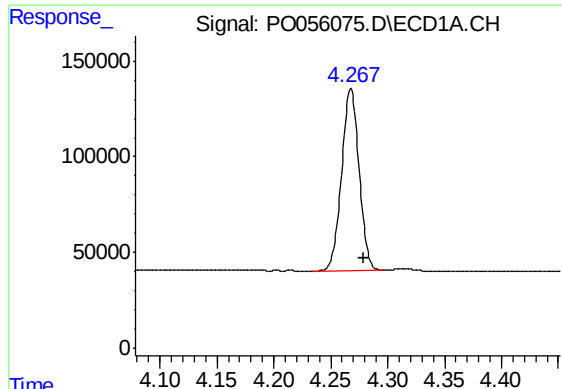


#1 Tetrachloro-m-xylene

R.T.: 4.268 min
Delta R.T.: -0.011 min
Response: 1021604
Conc: 34.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19


Manual Integrations
APPROVED

Ankita
5/13/2019 2:04:04 PM

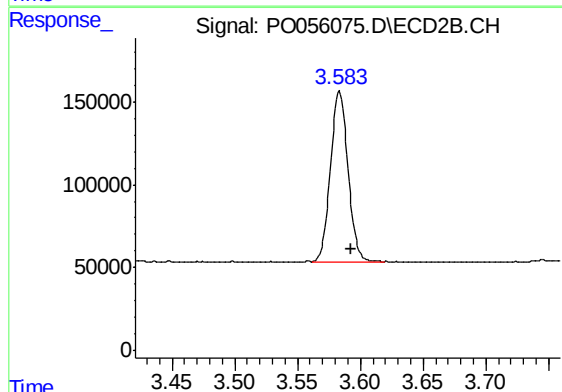


#1 Tetrachloro-m-xylene

R.T.: 3.583 min
Delta R.T.: -0.010 min
Response: 998846
Conc: 35.37 ng/ml

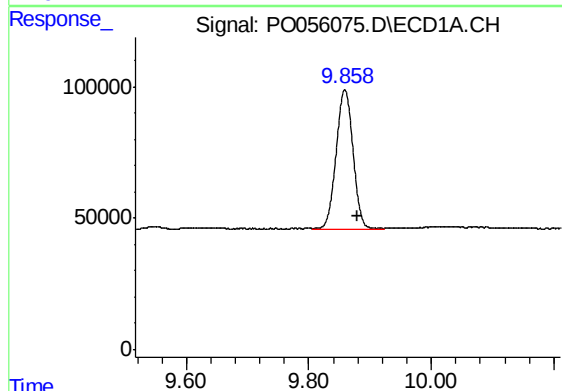


#2 Decachlorobiphenyl

R.T.: 9.859 min
Delta R.T.: -0.020 min
Response: 1017178
Conc: 27.19 ng/ml

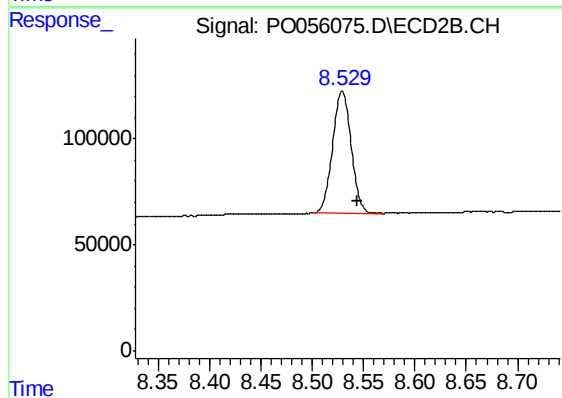

#2 Decachlorobiphenyl

R.T.: 8.529 min
Delta R.T.: -0.015 min
Response: 726352
Conc: 26.86 ng/ml

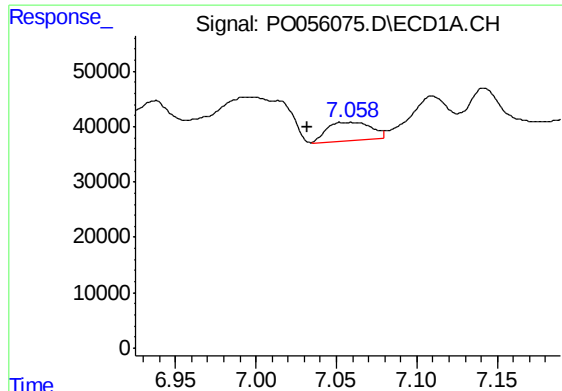


#31 AR-1260-1

R.T.: 7.058 min
Delta R.T.: 0.026 min
Response: 62098
Conc: 28.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19


Manual Integrations
APPROVED

Ankita
5/13/2019 2:04:04 PM

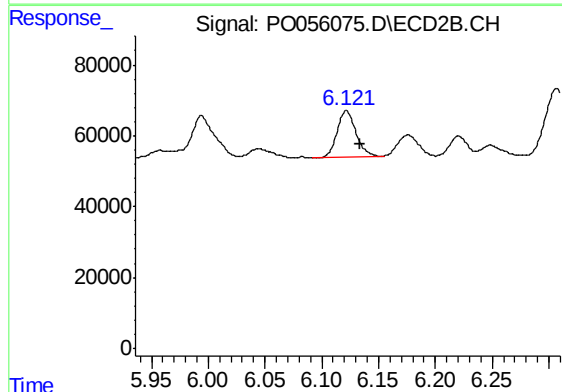


#31 AR-1260-1

R.T.: 6.122 min
Delta R.T.: -0.012 min
Response: 153014
Conc: 69.45 ng/ml

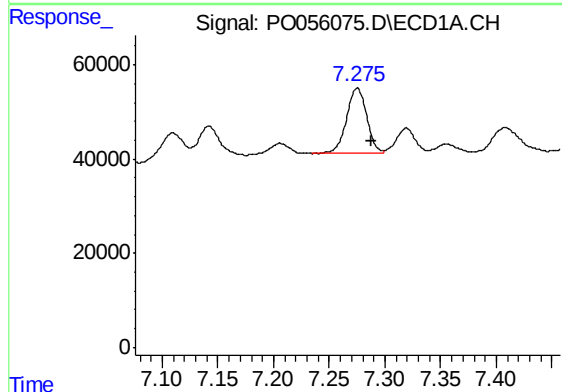


#32 AR-1260-2

R.T.: 7.275 min
Delta R.T.: -0.013 min
Response: 176195
Conc: 67.28 ng/ml

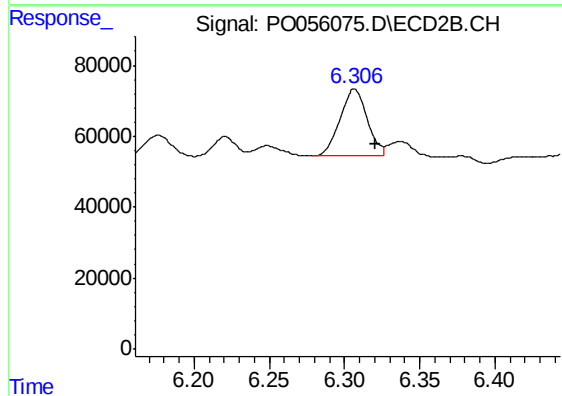

#32 AR-1260-2

R.T.: 6.306 min
Delta R.T.: -0.014 min
Response: 239392
Conc: 78.40 ng/ml m

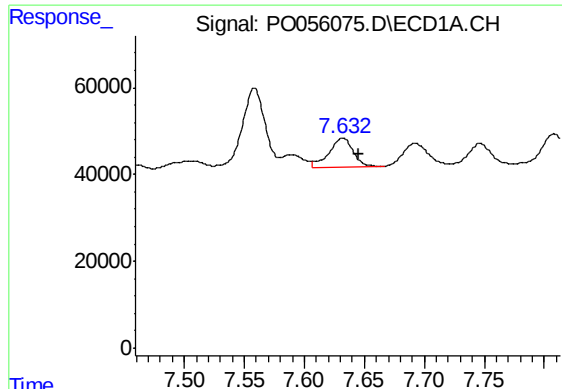


#33 AR-1260-3

R.T.: 7.632 min
Delta R.T.: -0.013 min
Response: 93079
Conc: 46.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19


Manual Integrations
APPROVED

Ankita
5/13/2019 2:04:04 PM

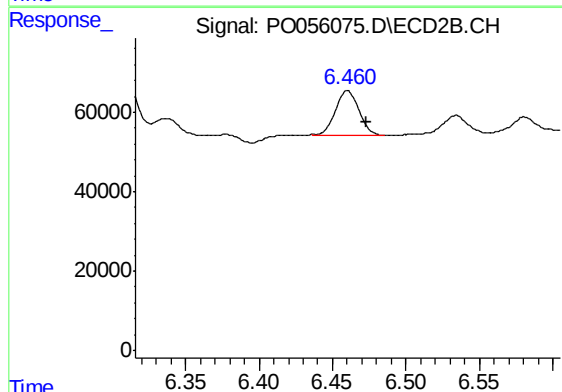


#33 AR-1260-3

R.T.: 6.460 min
Delta R.T.: -0.013 min
Response: 124789
Conc: 50.08 ng/ml m

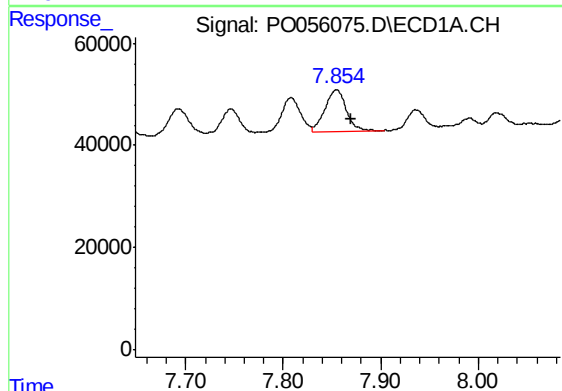


#34 AR-1260-4

R.T.: 7.855 min
Delta R.T.: -0.015 min
Response: 126676
Conc: 54.78 ng/ml

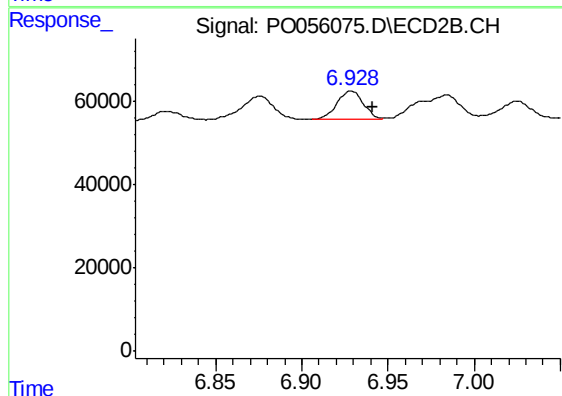

#34 AR-1260-4

R.T.: 6.928 min
Delta R.T.: -0.013 min
Response: 73402
Conc: 35.57 ng/ml

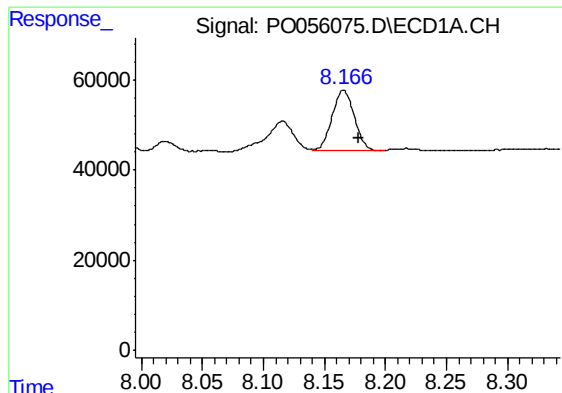


#35 AR-1260-5

R.T.: 8.166 min
Delta R.T.: -0.013 min
Response: 170182
Conc: 40.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19

Manual Integrations
APPROVED

Ankita
5/13/2019 2:04:04 PM

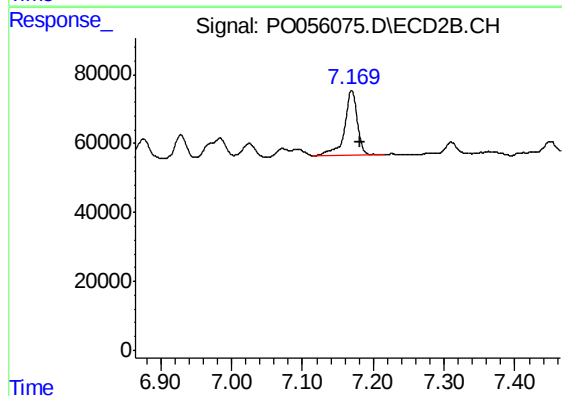

#35 AR-1260-5

R.T.: 7.170 min
Delta R.T.: -0.012 min
Response: 245391
Conc: 48.86 ng/ml