

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051019\
 Data File : P0056076.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 May 2019 18:37
 Operator : SM/SJ
 Sample : K2749-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRS-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 02:39:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.268	3.584	869790	840589	29.065	29.762
2)	SA Decachlor...	9.859	8.529	902174	642288	24.111	23.751

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051019\
Data File : PO056076.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 May 2019 18:37
Operator : SM/SJ
Sample : K2749-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TRS-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 02:39:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

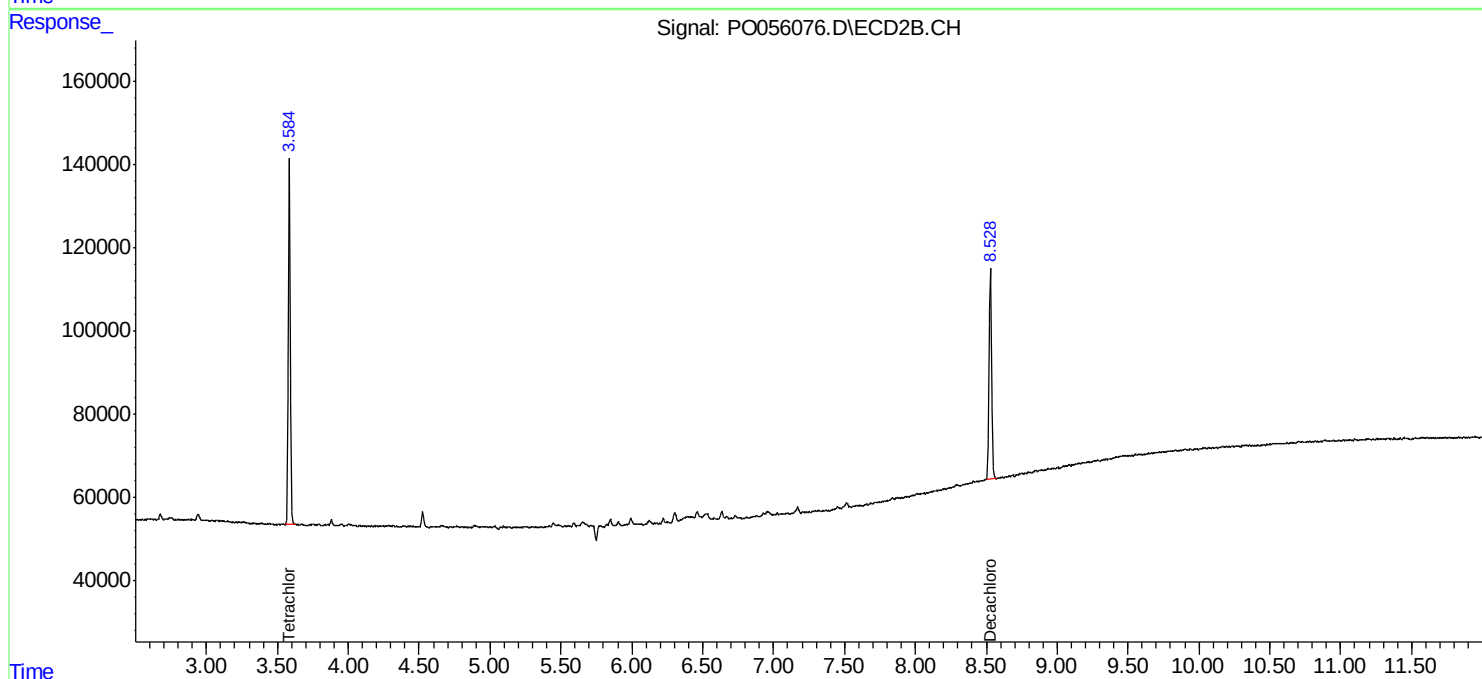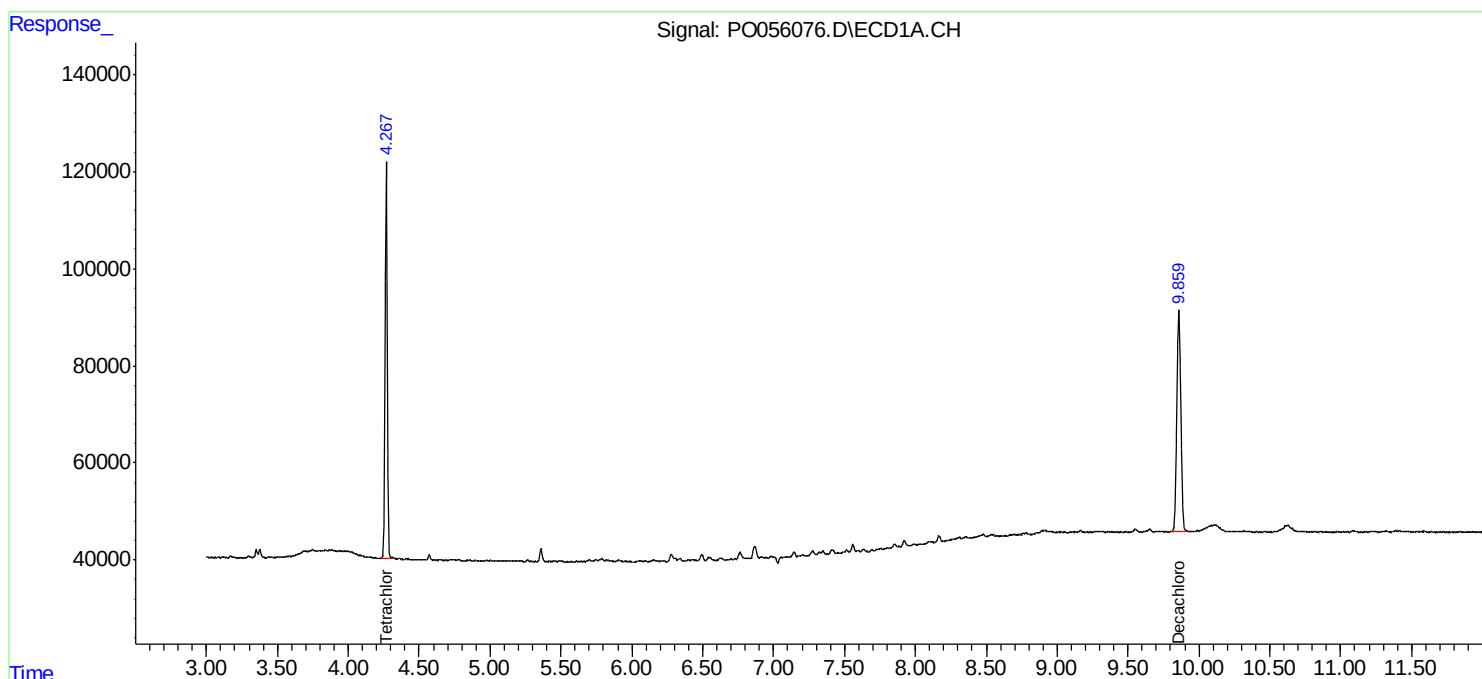


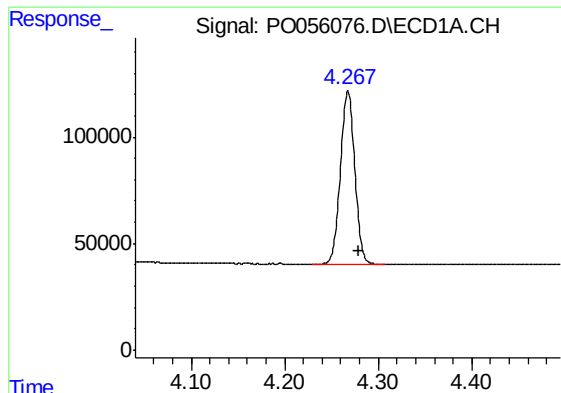

#1 Tetrachloro-m-xylene


R.T.: 4.268 min
Delta R.T.: -0.011 min
Response: 869790
Conc: 29.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRS-1

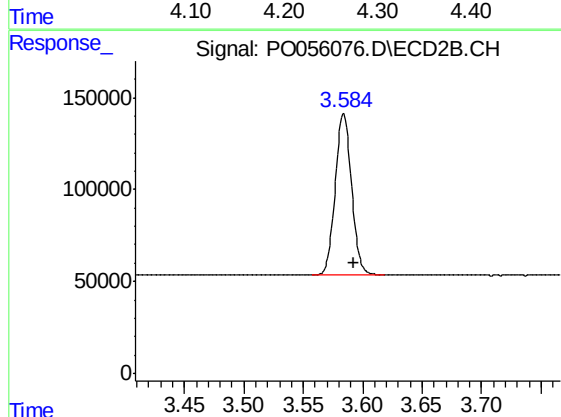


#1 Tetrachloro-m-xylene

R.T.: 3.584 min
Delta R.T.: -0.009 min
Response: 840589
Conc: 29.76 ng/ml

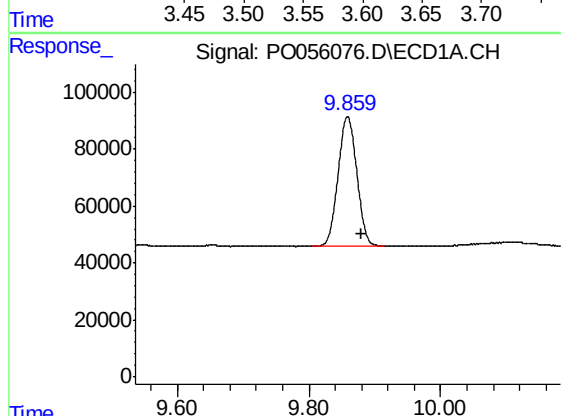

#2 Decachlorobiphenyl

R.T.: 9.859 min
Delta R.T.: -0.020 min
Response: 902174
Conc: 24.11 ng/ml

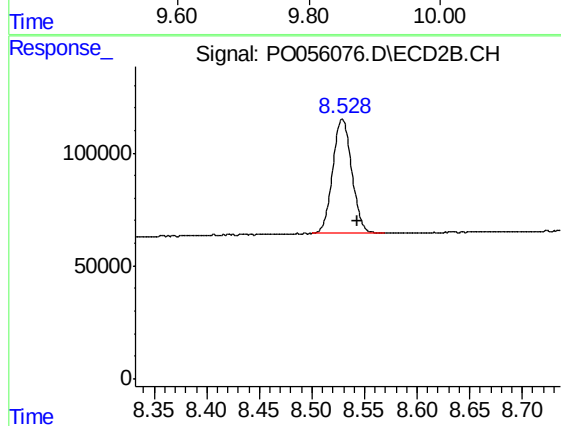

#2 Decachlorobiphenyl

R.T.: 8.529 min
Delta R.T.: -0.015 min
Response: 642288
Conc: 23.75 ng/ml