

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051119\
 Data File : P0056125.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2019 00:27
 Operator : SM/SJ
 Sample : PB119646BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB119646BL

Manual Integrations
 APPROVED

Ankita
 5/15/2019 8:51:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 03:52:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.265	3.582	768273	708943	25.673	25.101
2) SA Decachlor...	9.854	8.524	902362	646278	24.116	23.898m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051119\
Data File : P0056125.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2019 00:27
Operator : SM/SJ
Sample : PB119646BL
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB119646BL


Manual Integrations
APPROVED

Ankita
5/15/2019 8:51:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 03:52:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

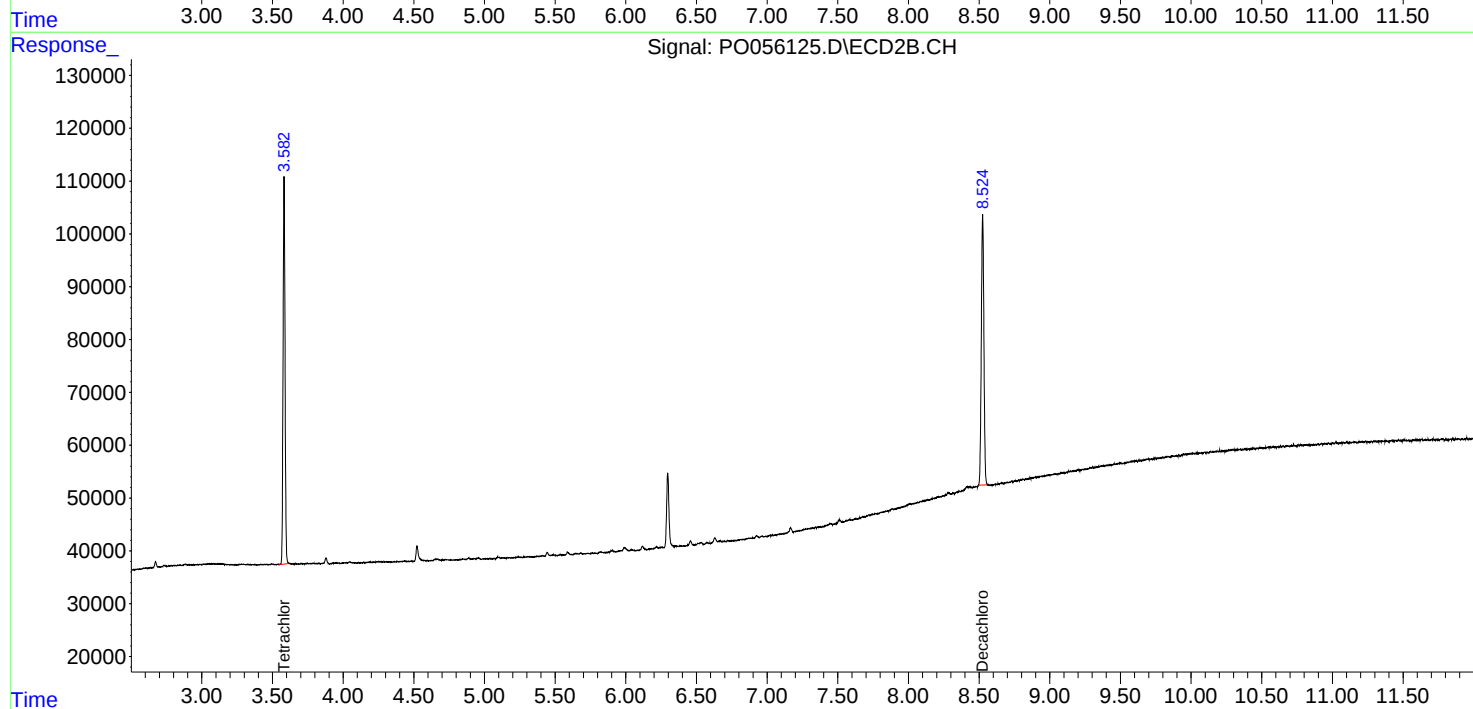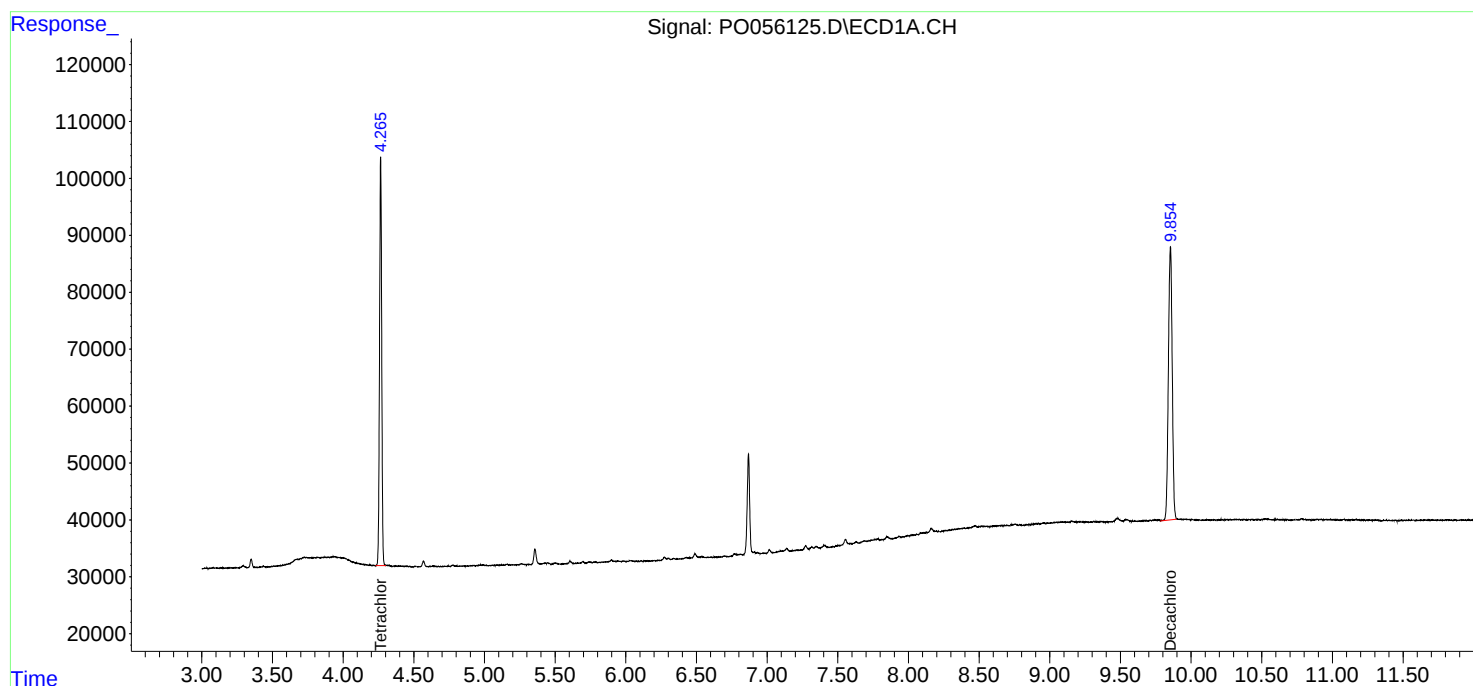

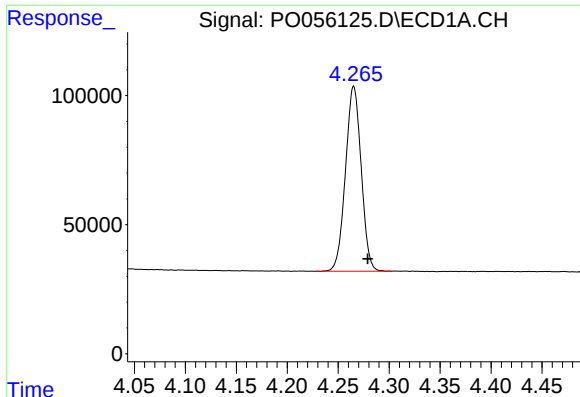


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: -0.014 min
Response: 768273
Conc: 25.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB119646BL


Manual Integrations
APPROVED

Ankita
5/15/2019 8:51:37 AM

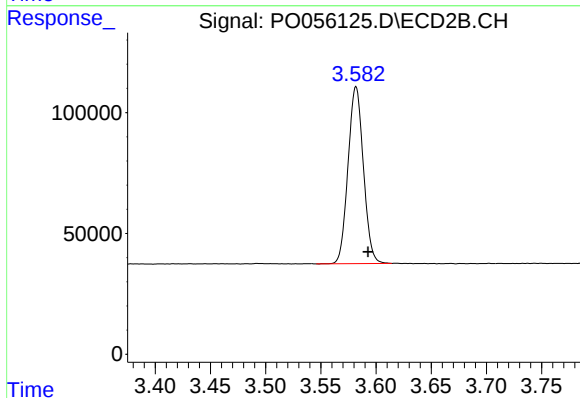


#1 Tetrachloro-m-xylene

R.T.: 3.582 min
Delta R.T.: -0.011 min
Response: 708943
Conc: 25.10 ng/ml

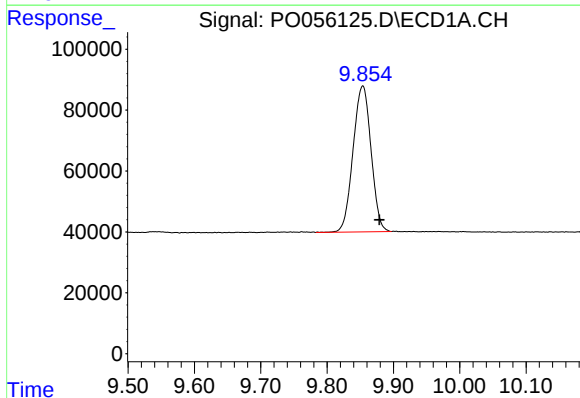

#2 Decachlorobiphenyl

R.T.: 9.854 min
Delta R.T.: -0.025 min
Response: 902362
Conc: 24.12 ng/ml

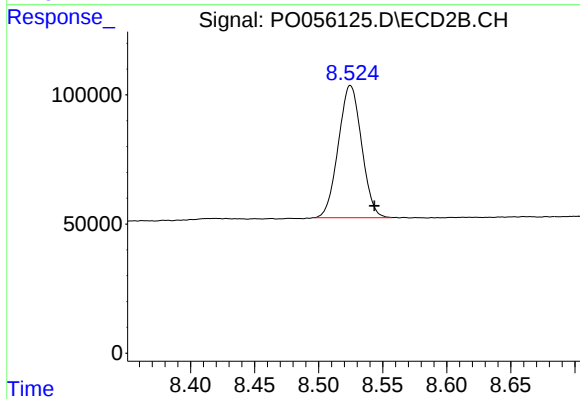

#2 Decachlorobiphenyl

R.T.: 8.524 min
Delta R.T.: -0.019 min
Response: 646278
Conc: 23.90 ng/ml m