

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051124\
 Data File : P0103626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2024 08:05
 Operator : YP/AJ
 Sample : P2437-04RE
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/13/2024
 Supervised By :Ankita Jodhani 05/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 22:26:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 07 04:55:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.465	3.611	85335710	29791230	11.089m	11.826m
2) SA Decachlor...	10.216	8.552	91807852	19794216	19.368	15.216

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051124\
Data File : PO103626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2024 08:05
Operator : YP/AJ
Sample : P2437-04RE
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/13/2024
Supervised By :Ankita Jodhani 05/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 22:26:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 07 04:55:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

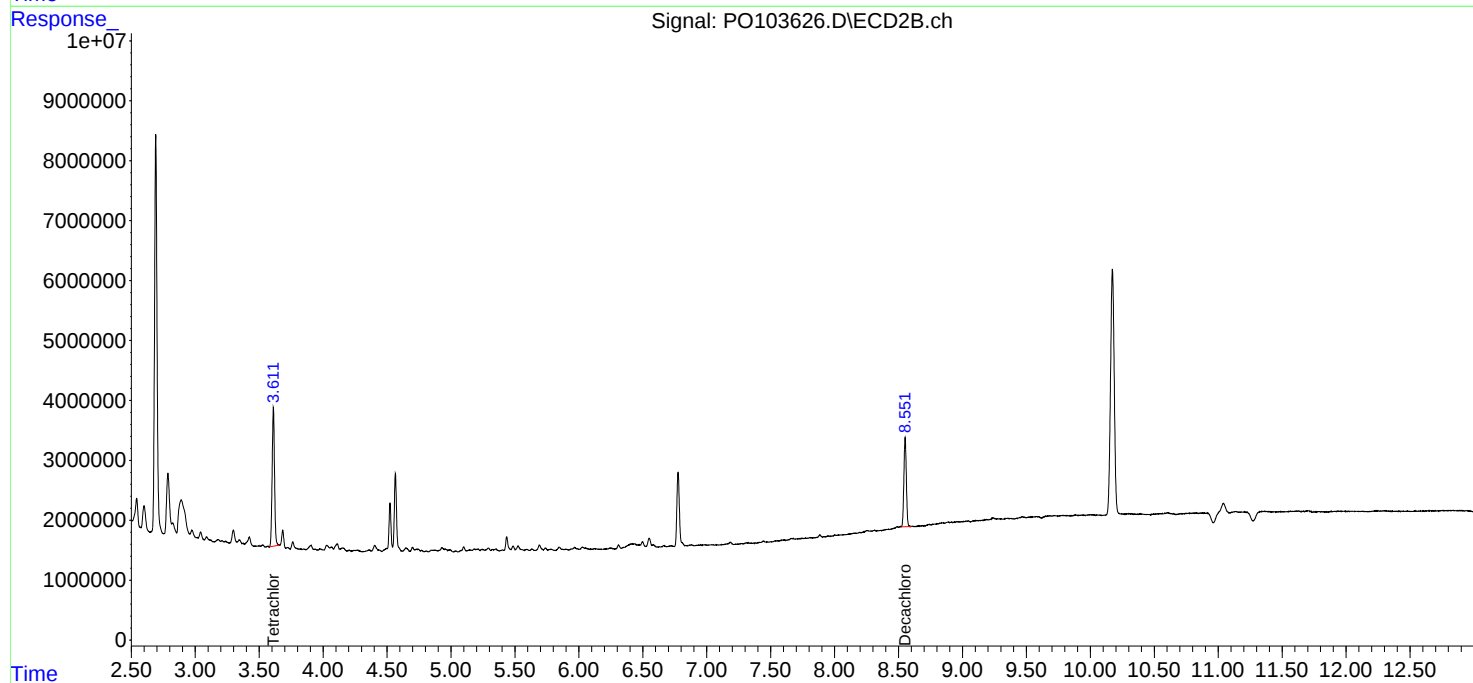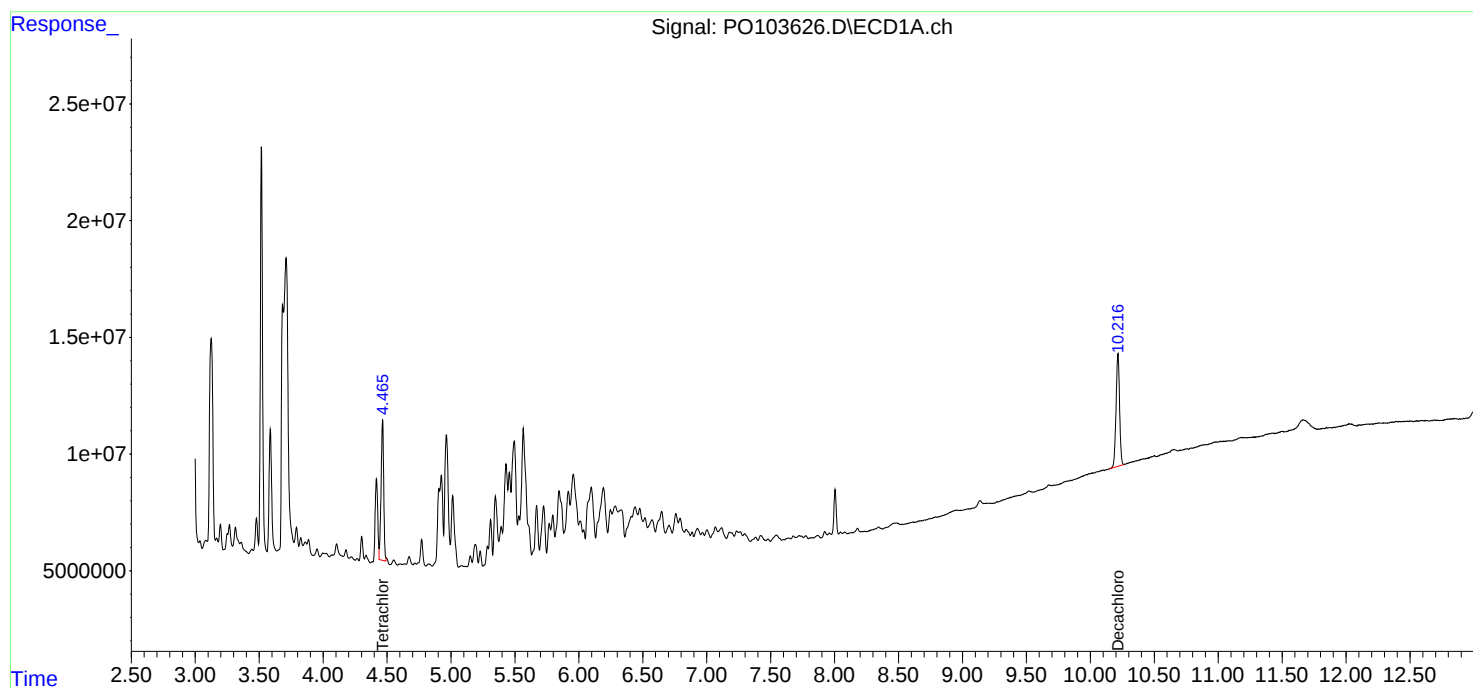

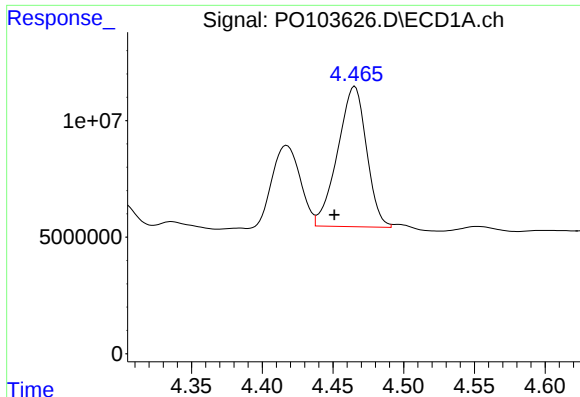


#1 Tetrachloro-m-xylene

R.T.: 4.465 min
Delta R.T.: 0.014 min
Response: 85335710
Conc: 11.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/13/2024
Supervised By :Ankita Jodhani 05/13/2024

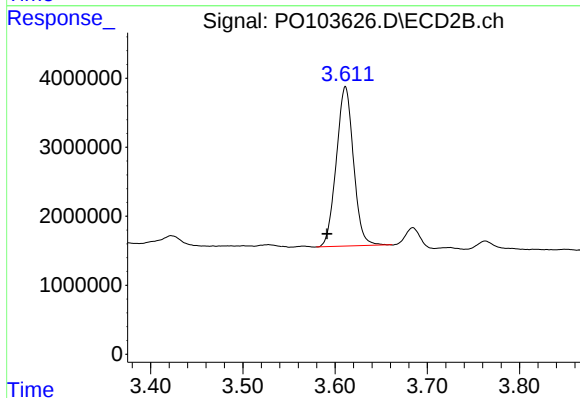


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.020 min
Response: 29791230
Conc: 11.83 ng/ml m

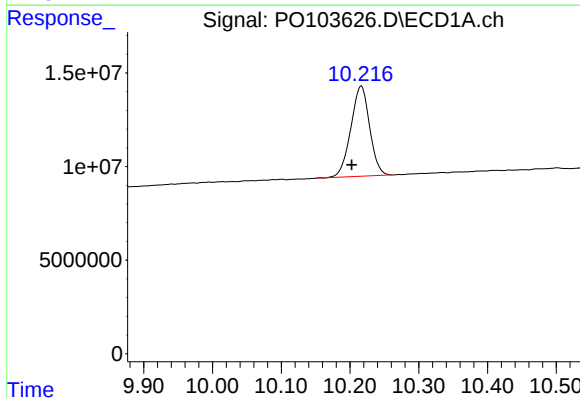

#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: 0.014 min
Response: 91807852
Conc: 19.37 ng/ml

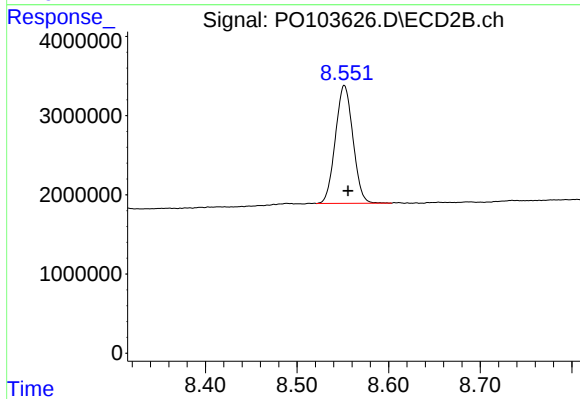

#2 Decachlorobiphenyl

R.T.: 8.552 min
Delta R.T.: -0.004 min
Response: 19794216
Conc: 15.22 ng/ml