

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051124\
 Data File : P0103636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2024 11:40
 Operator : YP/AJ
 Sample : P2437-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OUTSIDE-BLACK-DRUM

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/13/2024
 Supervised By :Ankita Jodhani 05/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 22:32:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 07 04:55:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.586	153.4E6	56482500	19.937	22.421m
2) SA Decachlor...	10.211	8.546	64153290	13709270	13.534	10.538

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051124\
Data File : PO103636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2024 11:40
Operator : YP/AJ
Sample : P2437-06
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OUTSIDE-BLACK-DRUM


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/13/2024
Supervised By :Ankita Jodhani 05/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 22:32:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 07 04:55:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

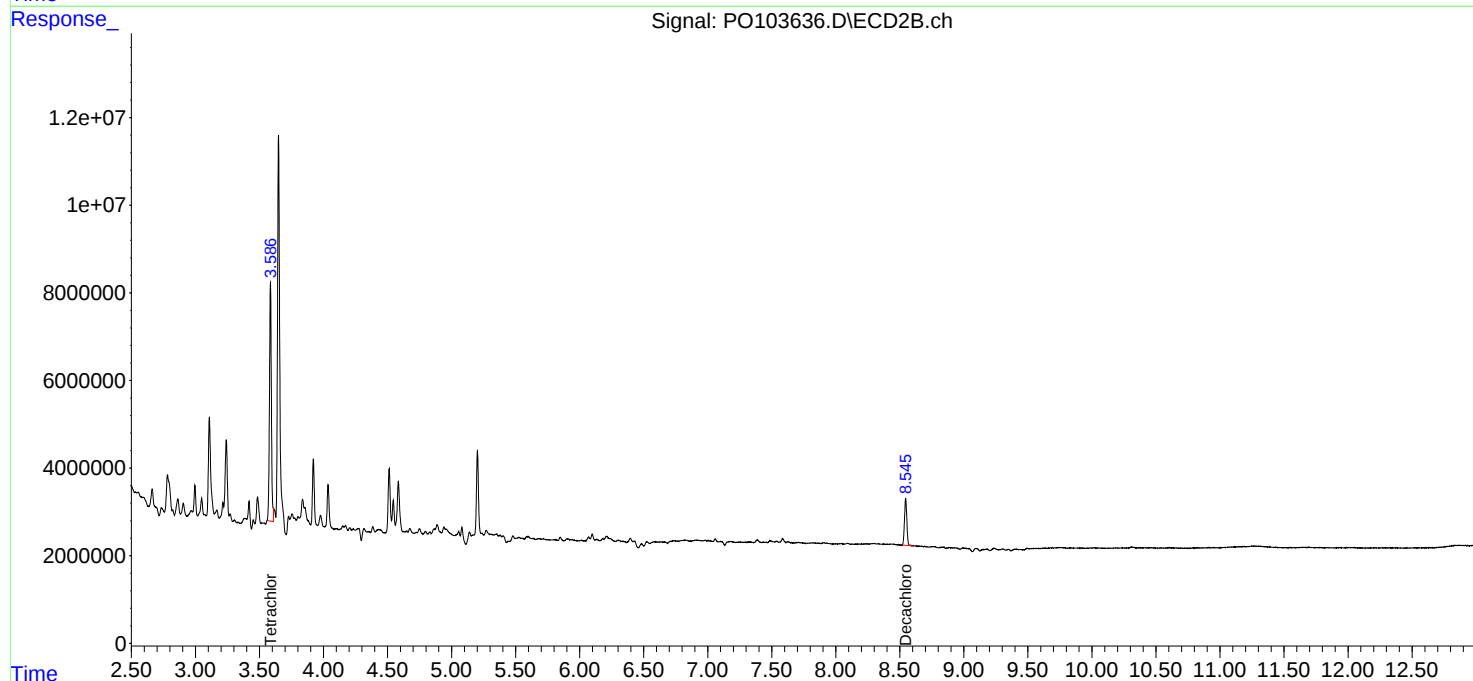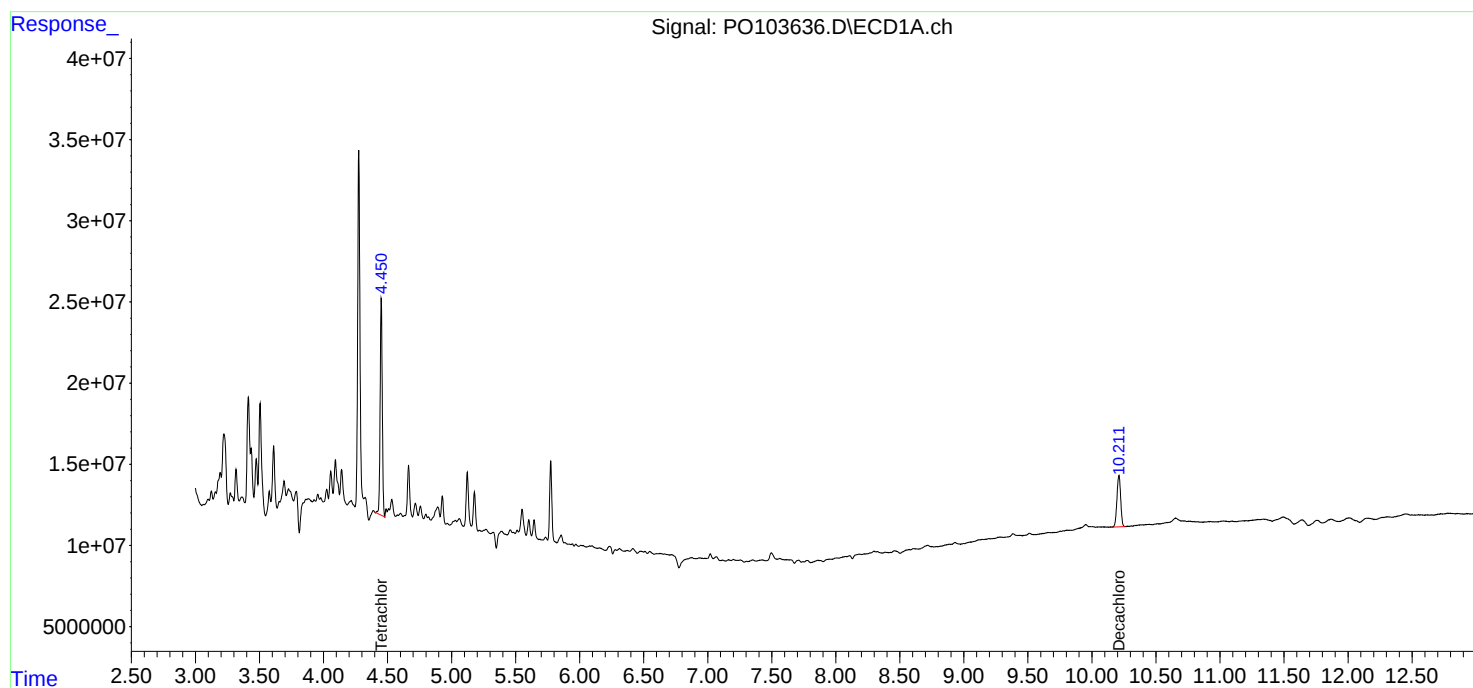

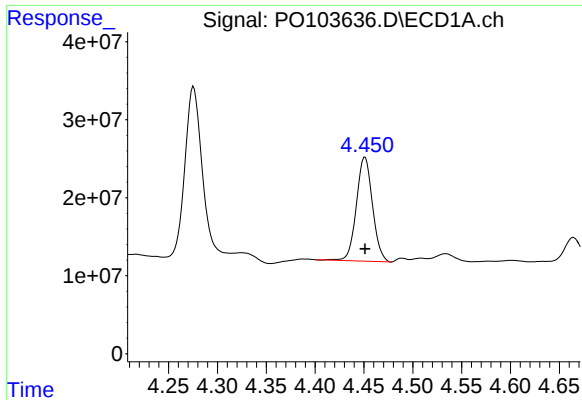


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 153430230
Conc: 19.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
OUTSIDE-BLACK-DRUM


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/13/2024
Supervised By :Ankita Jodhani 05/13/2024

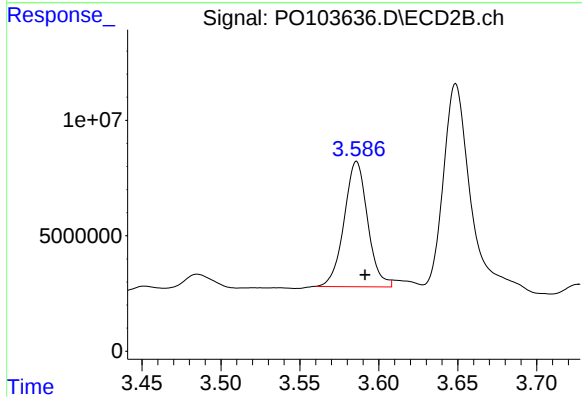


#1 Tetrachloro-m-xylene

R.T.: 3.586 min
Delta R.T.: -0.006 min
Response: 56482500
Conc: 22.42 ng/ml m

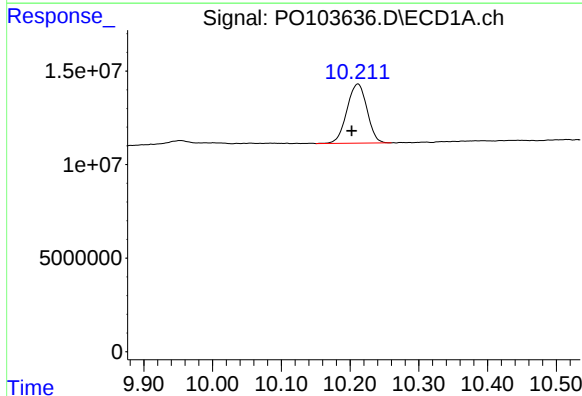

#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: 0.009 min
Response: 64153290
Conc: 13.53 ng/ml

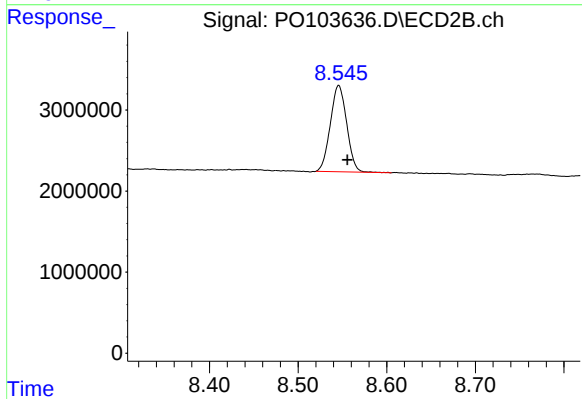

#2 Decachlorobiphenyl

R.T.: 8.546 min
Delta R.T.: -0.010 min
Response: 13709270
Conc: 10.54 ng/ml