

Data Path : P:\HPCHEM1\ECD_0\Data\P0051218\
 Data File : P0044642.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2018 19:30
 Operator : SM/UA
 Sample : J2828-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 FK-PS-01.025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:07:57 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 10 02:14:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.036	3.303	5046028	6919978	25.084	25.555
2) SA Decachlor...	9.352	8.039	1877909	1992466	12.933	11.404
Target Compounds						
9) L2 AR-1221-2	0.000	3.651	0	265235	N.D.	78.942 #
10) L2 AR-1221-3	4.407	3.651	197474	265235	23.923	23.900
11) L3 AR-1232-1	4.407	3.651	197474	265235	23.923	23.900
27) L6 AR-1254-2	0.000	5.269	0	249193	N.D.	17.042 #
32) L7 AR-1260-2	0.000	5.916	0	247728	N.D.	13.519 #
36) L8 AR-1262-1	0.000	5.916	0	247728	N.D.	14.458 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_0\Data\PO051218\
Data File : PO044642.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2018 19:30
Operator : SM/UA
Sample : J2828-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01.025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:07:57 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

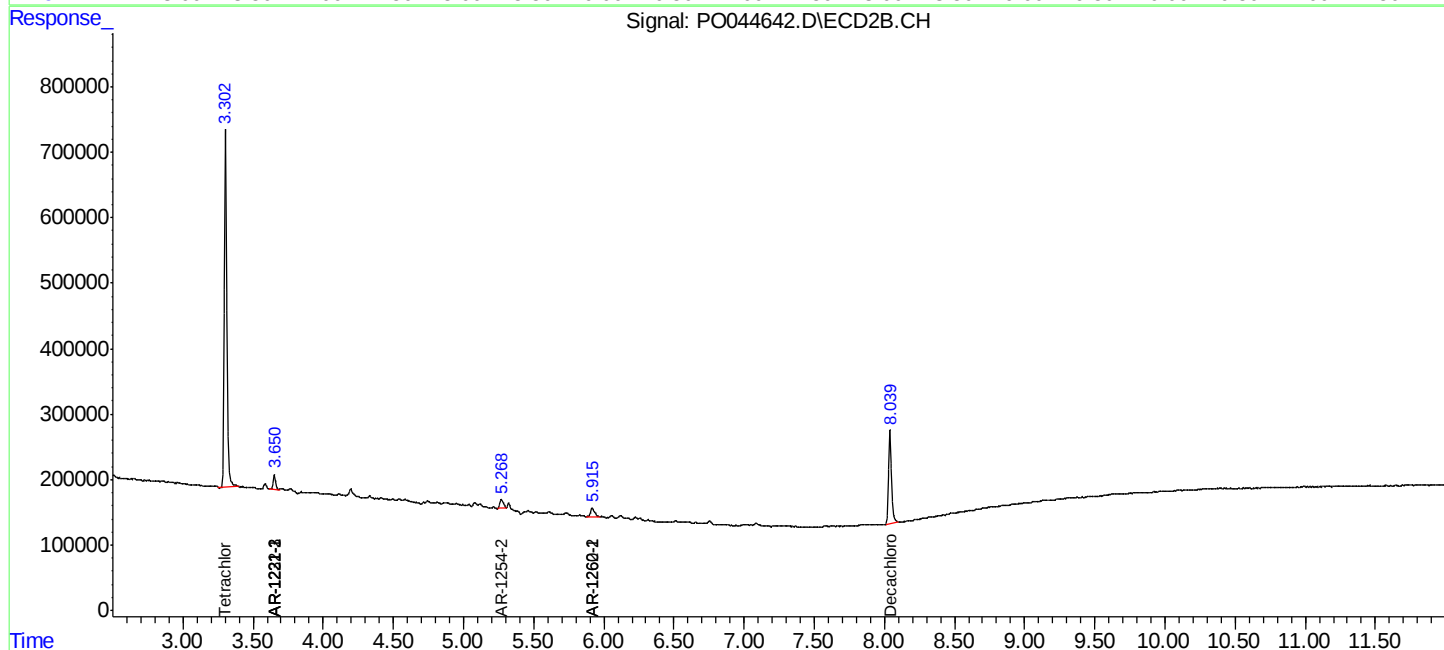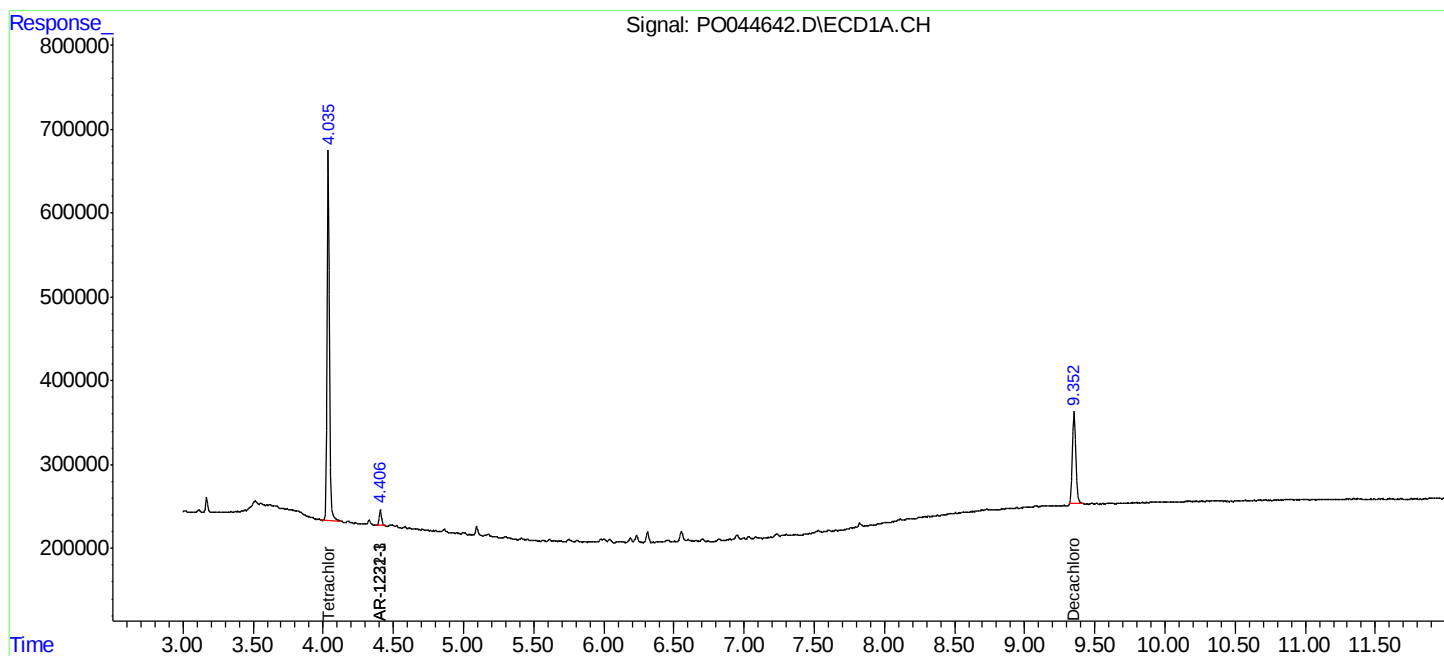


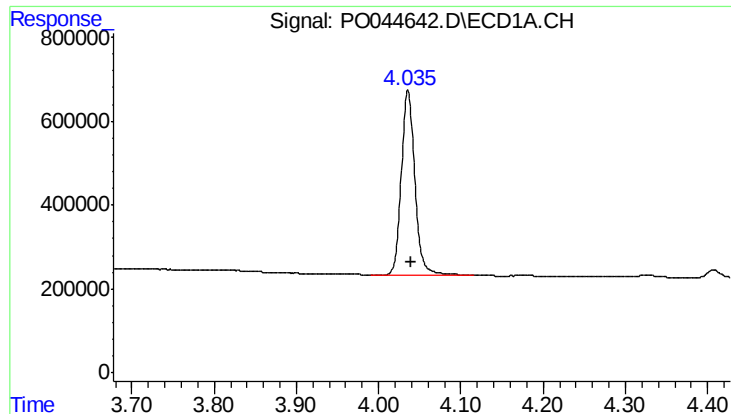

#1 Tetrachloro-m-xylene


R.T.: 4.036 min
Delta R.T.: -0.003 min
Response: 5046028
Conc: 25.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01.025

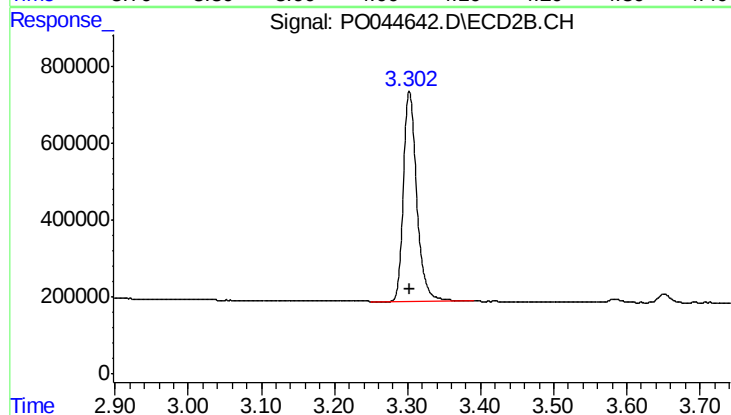


#1 Tetrachloro-m-xylene

R.T.: 3.303 min
Delta R.T.: 0.000 min
Response: 6919978
Conc: 25.55 ng/ml

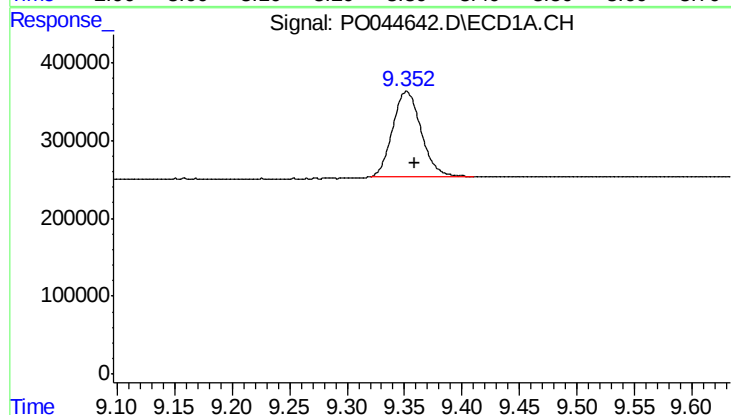


#2 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: -0.008 min
Response: 1877909
Conc: 12.93 ng/ml

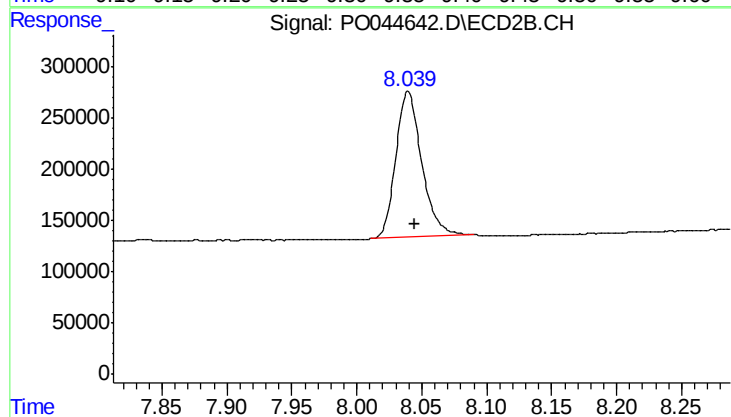

#2 Decachlorobiphenyl


R.T.: 8.039 min
Delta R.T.: -0.005 min
Response: 1992466
Conc: 11.40 ng/ml

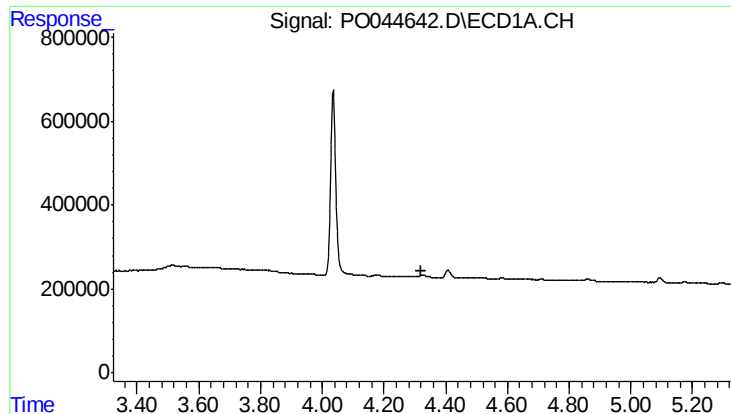

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01.025

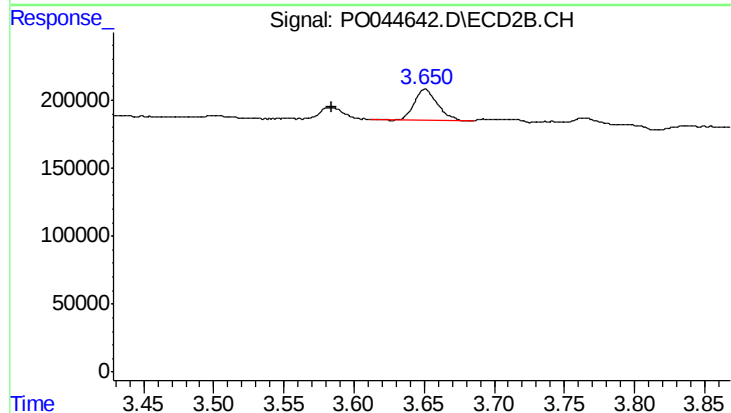


#9 AR-1221-2

R.T.: 3.651 min
Delta R.T.: 0.066 min
Response: 265235
Conc: 78.94 ng/ml

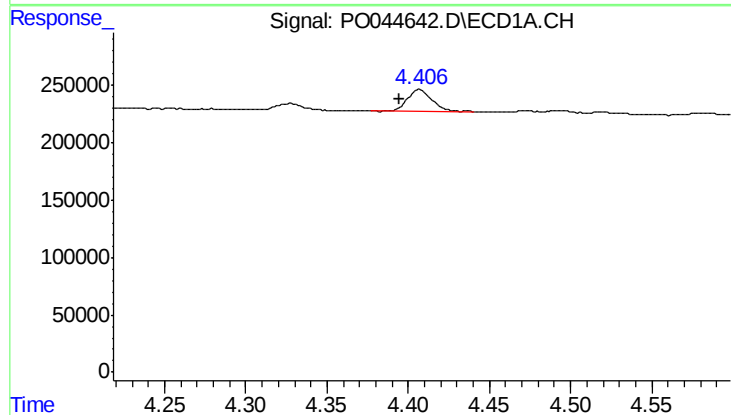


#10 AR-1221-3

R.T.: 4.407 min
Delta R.T.: 0.012 min
Response: 197474
Conc: 23.92 ng/ml

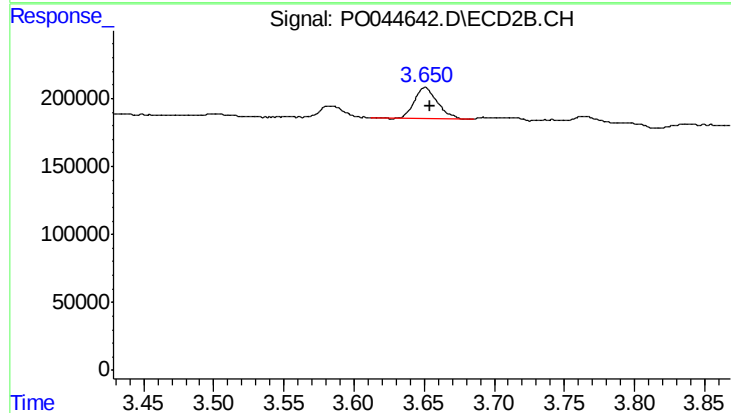

#10 AR-1221-3


R.T.: 3.651 min
Delta R.T.: -0.003 min
Response: 265235
Conc: 23.90 ng/ml

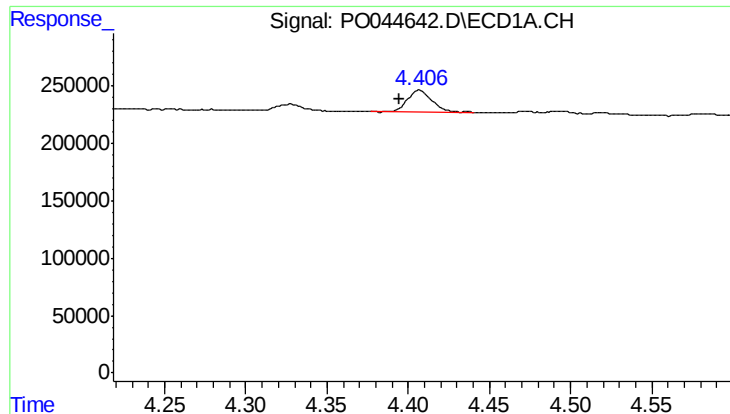

#11 AR-1232-1


R.T.: 4.407 min
Delta R.T.: 0.012 min
Response: 197474
Conc: 23.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01.025

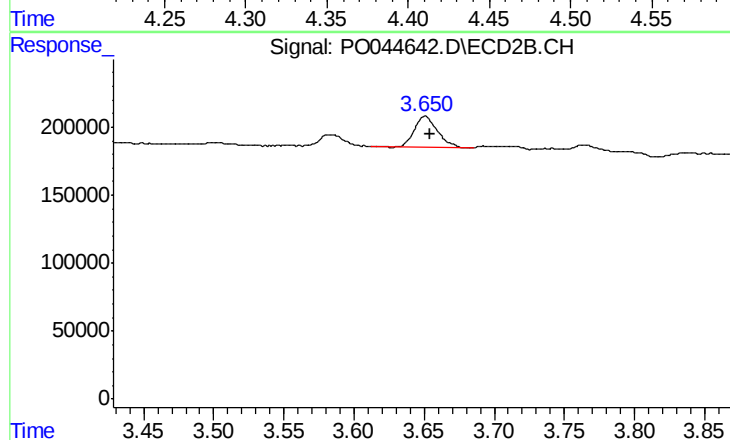


#11 AR-1232-1

R.T.: 3.651 min
Delta R.T.: -0.003 min
Response: 265235
Conc: 23.90 ng/ml

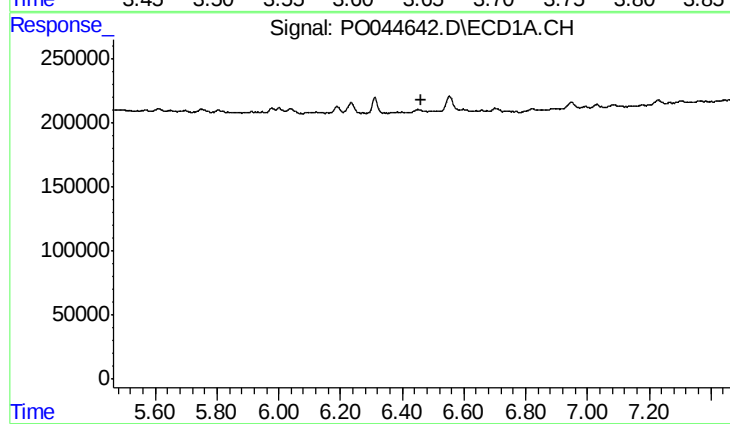


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

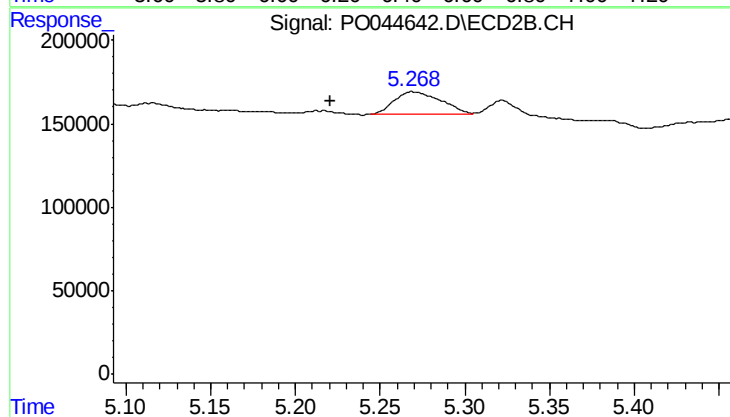

#27 AR-1254-2


R.T.: 5.269 min
Delta R.T.: 0.049 min
Response: 249193
Conc: 17.04 ng/ml

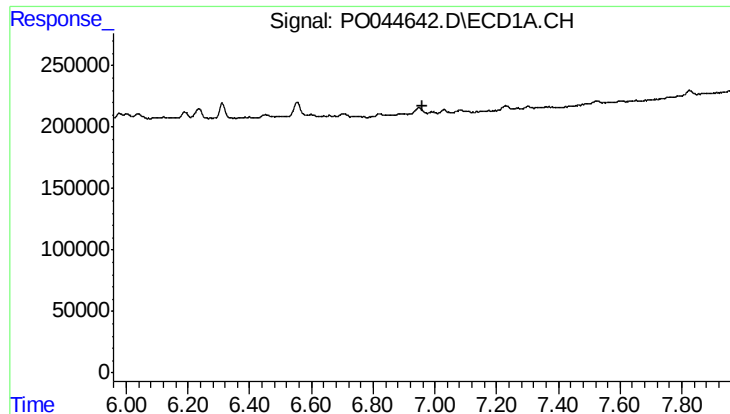

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 6.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01.025

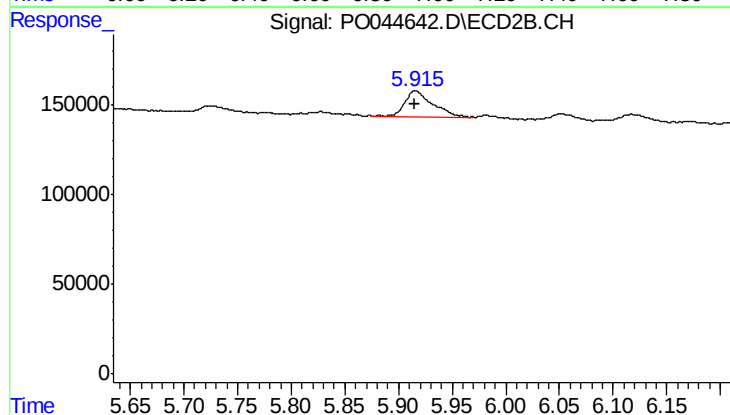


#32 AR-1260-2

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 247728
Conc: 13.52 ng/ml

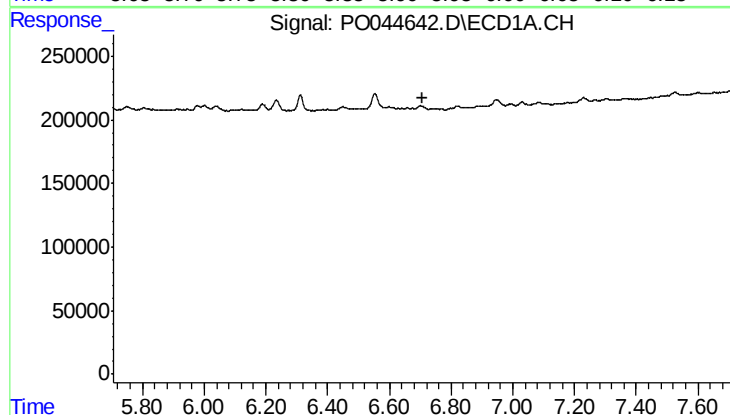

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

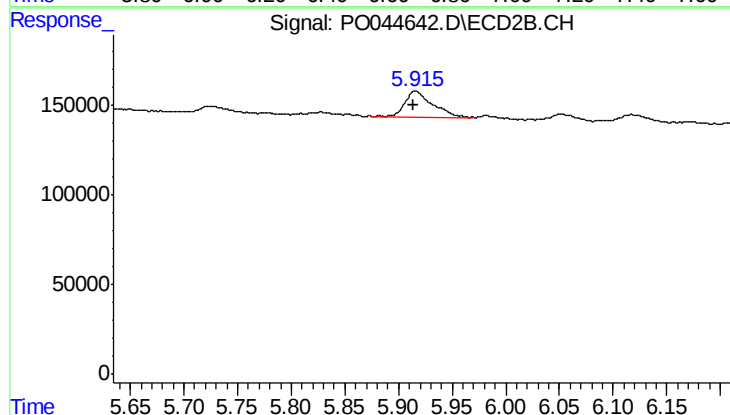

#36 AR-1262-1

R.T.: 5.916 min
Delta R.T.: 0.002 min
Response: 247728
Conc: 14.46 ng/ml