

Data Path : P:\HPCHEM1\ECD 0\Data\P0051218\
Data File : P0044638.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2018 18:29
Operator : SM/UA
Sample : J2825-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-025

Manual Integrations
APPROVED

ugo
5/16/2018 10:09:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 03:11:11 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.036	3.303	4625160	6595402	22.991	24.356
2) SA Decachlor...	9.352	8.040	2487340	2350557	17.130m	13.454

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0051218\
Data File : P0044638.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2018 18:29
Operator : SM/UA
Sample : J2825-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-PS-01-025


Manual Integrations
APPROVED

ugo
5/16/2018 10:09:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 03:11:11 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0050918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 10 02:14:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

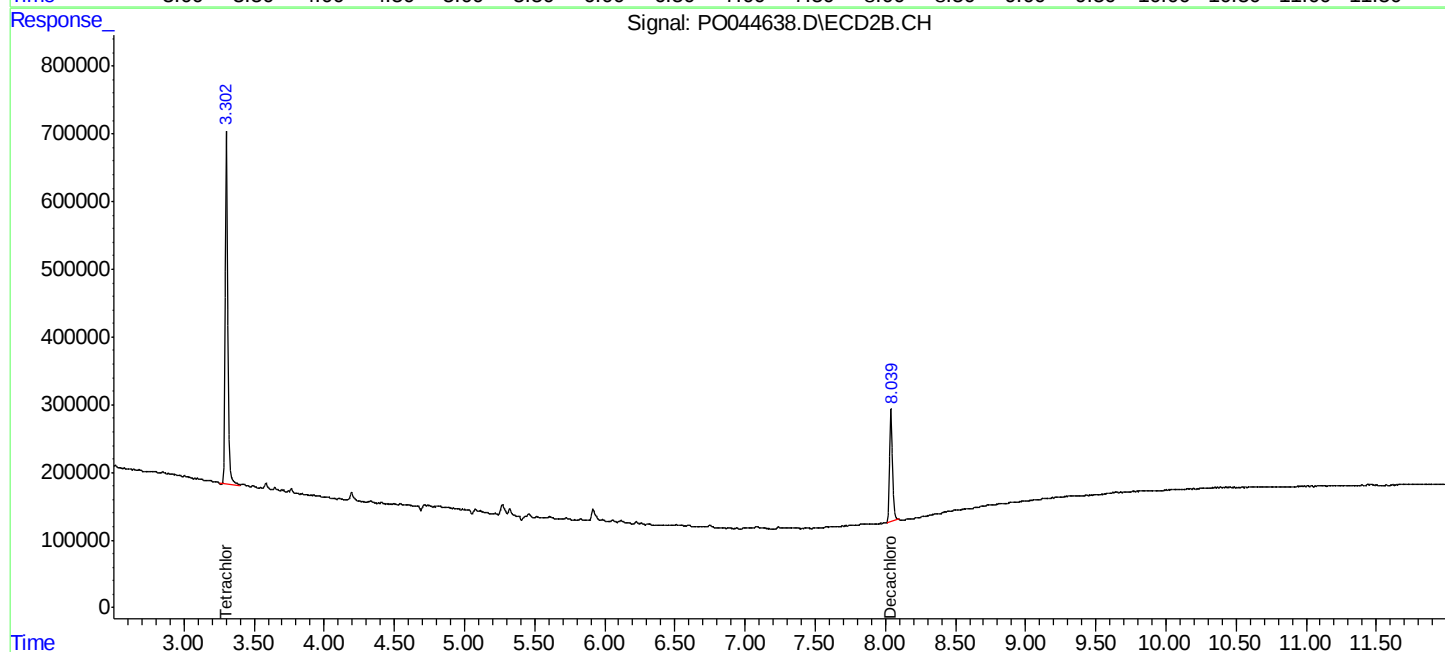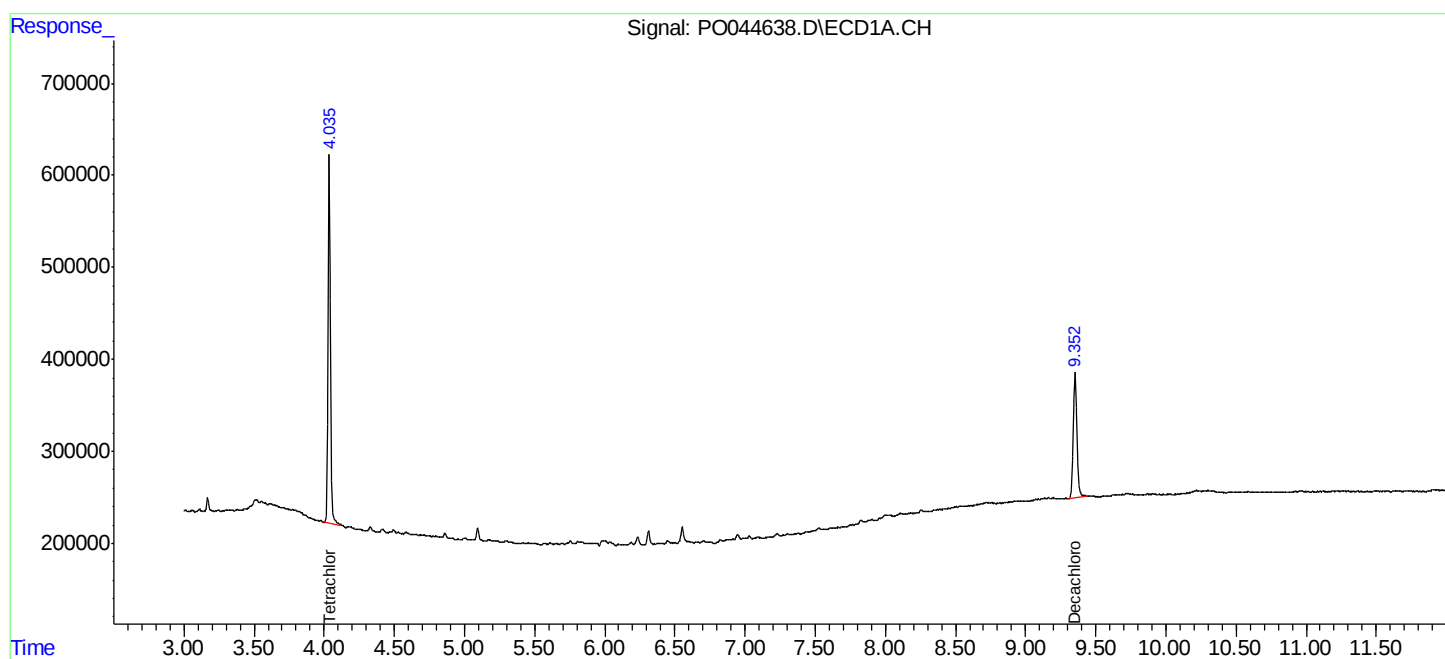

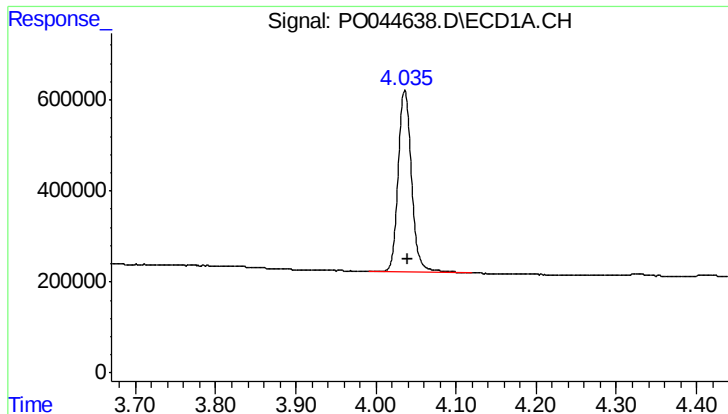


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: -0.003 min
Response: 4625160
Conc: 22.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-025


Manual Integrations
APPROVED

ugo
5/16/2018 10:09:28 AM

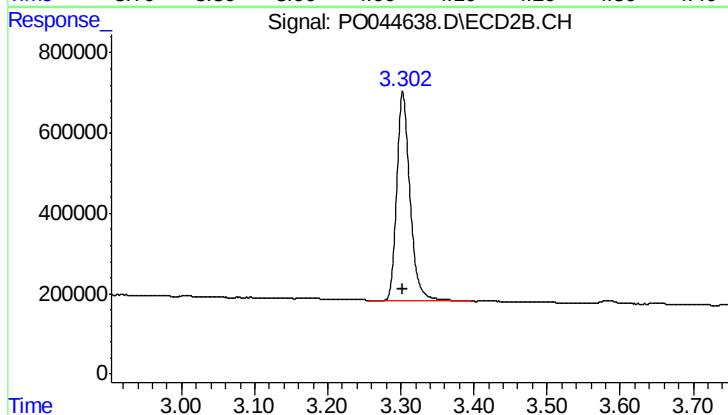


#1 Tetrachloro-m-xylene

R.T.: 3.303 min
Delta R.T.: 0.000 min
Response: 6595402
Conc: 24.36 ng/ml

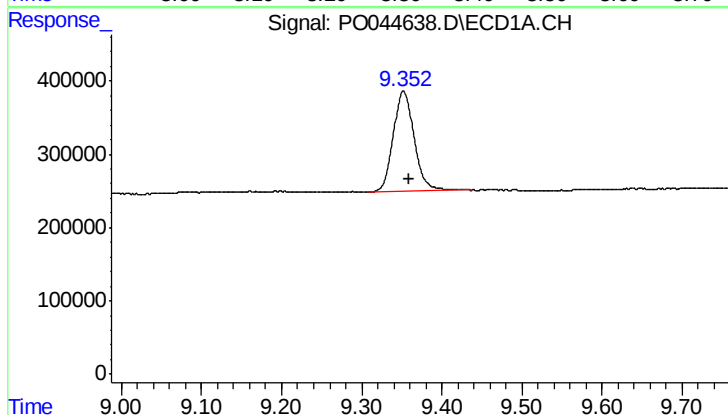

#2 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: -0.008 min
Response: 2487340
Conc: 17.13 ng/ml m

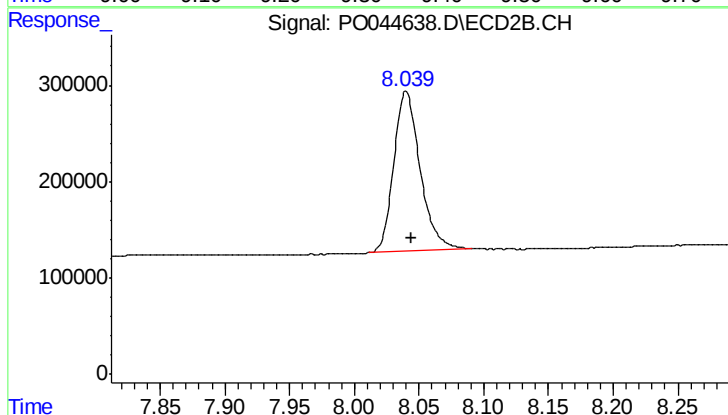

#2 Decachlorobiphenyl

R.T.: 8.040 min
Delta R.T.: -0.004 min
Response: 2350557
Conc: 13.45 ng/ml