

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051320\
 Data File : P0068338.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2020 12:31
 Operator : DD\AJ
 Sample : L2182-07
 Misc : AR1232 40PPB LOD
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/14/2020 2:30:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:01:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.903	3.931	503995	617017	17.970	17.981
2) SA Decachlor...	10.856	9.203	716518	765108	18.006m	19.873m
Target Compounds						
11) L3 AR-1232-1	5.341	4.374	23057	35785	37.542m	46.395
12) L3 AR-1232-2	5.927	5.203	18991	40846	61.625m	51.004
13) L3 AR-1232-3	6.247	5.393	29180	20405	45.768	48.049
14) L3 AR-1232-4	6.418	5.491	13057	16376	41.485m	43.616
15) L3 AR-1232-5	6.515	5.672	9493	12352	44.866	29.648m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051320\
Data File : P0068338.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2020 12:31
Operator : DD\AJ
Sample : L2182-07
Misc : AR1232 40PPB LOD
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:01:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

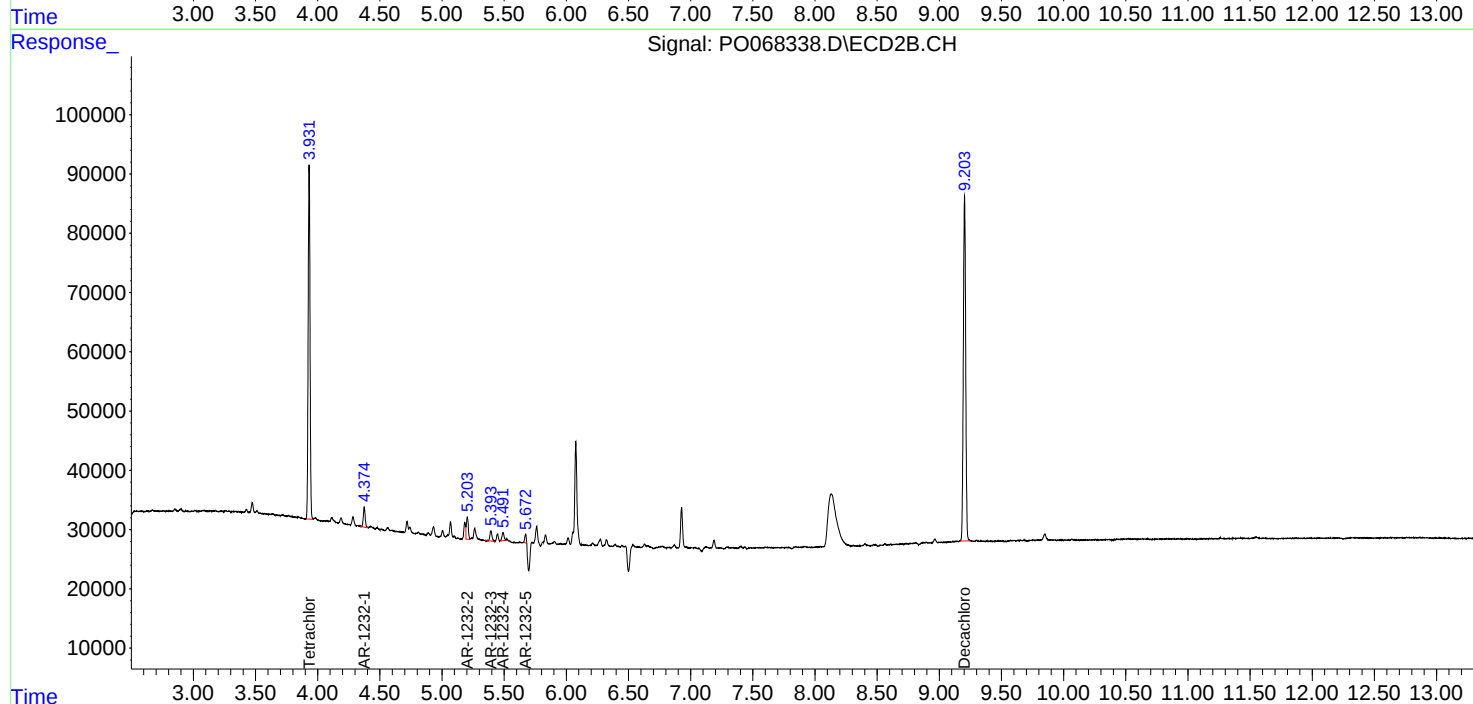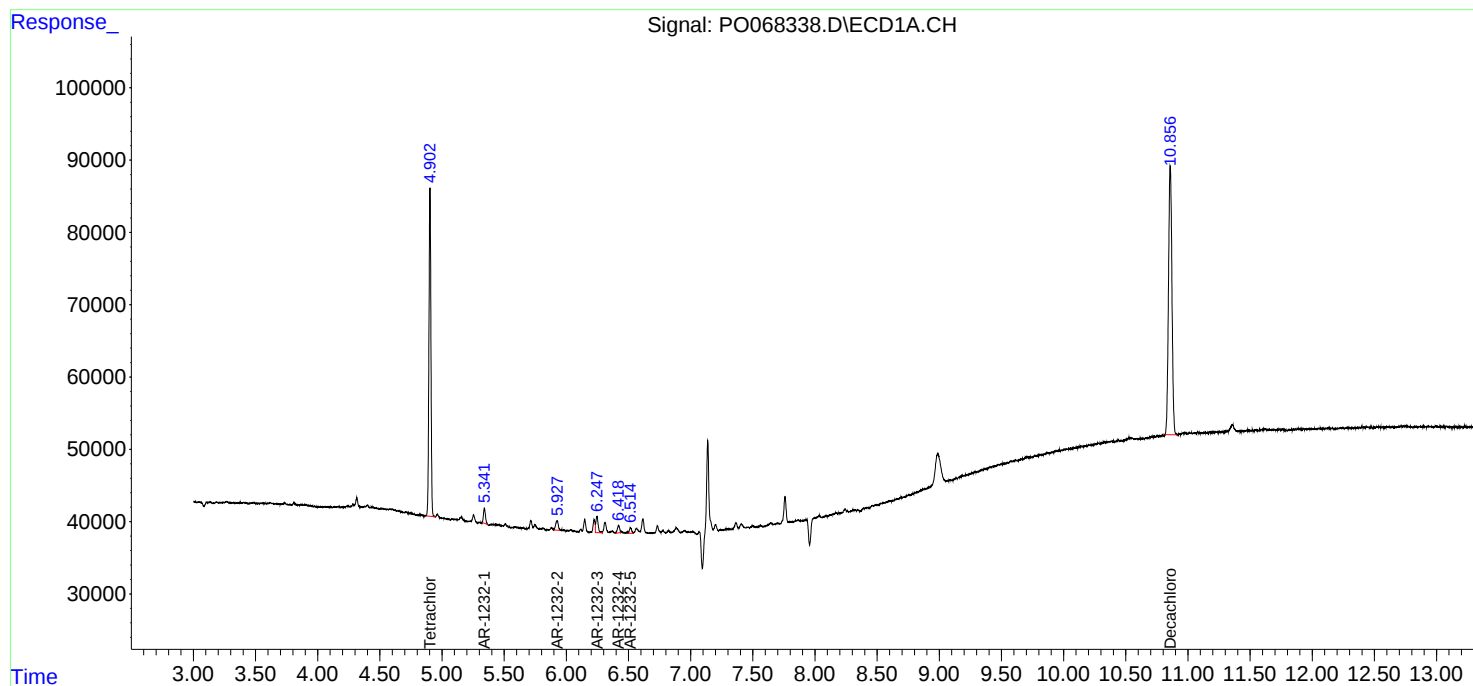

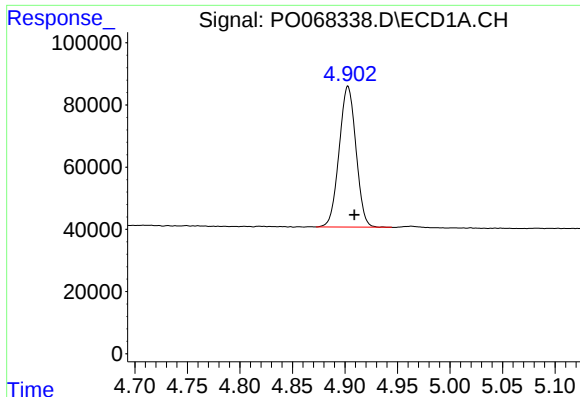


#1 Tetrachloro-m-xylene

R.T.: 4.903 min
Delta R.T.: -0.006 min
Response: 503995
Conc: 17.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:51 PM

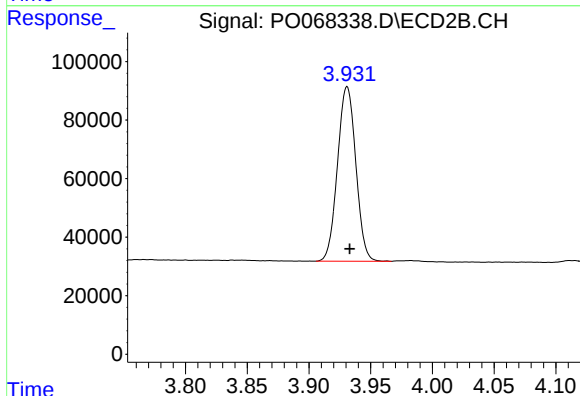


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 617017
Conc: 17.98 ng/ml

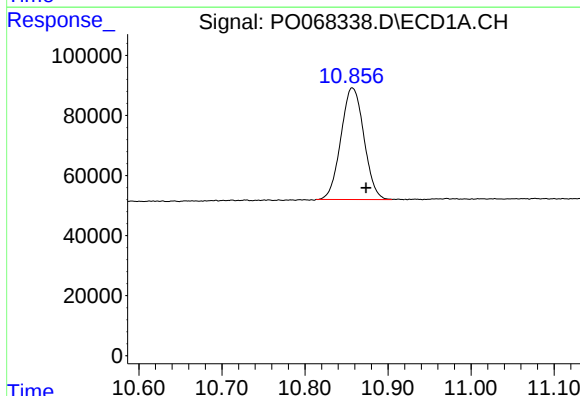


#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.017 min
Response: 716518
Conc: 18.01 ng/ml m

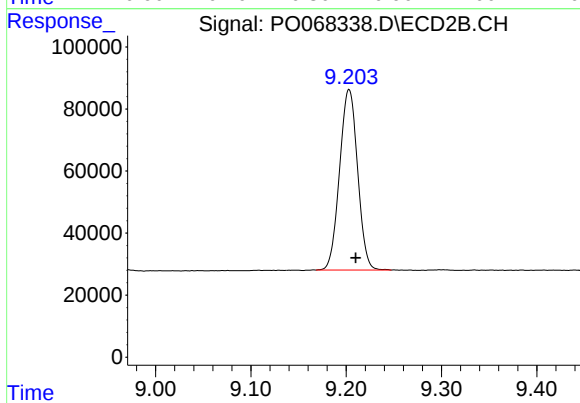

#2 Decachlorobiphenyl

R.T.: 9.203 min
Delta R.T.: -0.007 min
Response: 765108
Conc: 19.87 ng/ml m

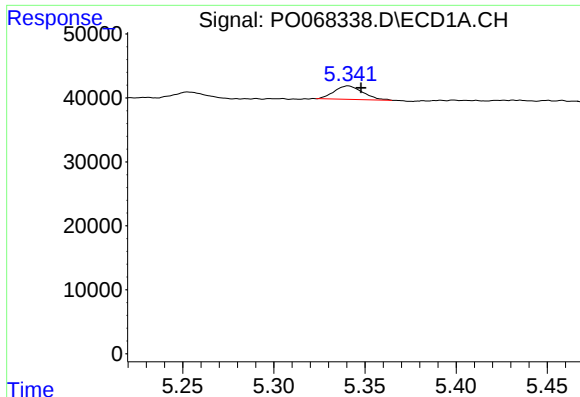


#11 AR-1232-1

R.T.: 5.341 min
Delta R.T.: -0.007 min
Response: 23057
Conc: 37.54 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:51 PM

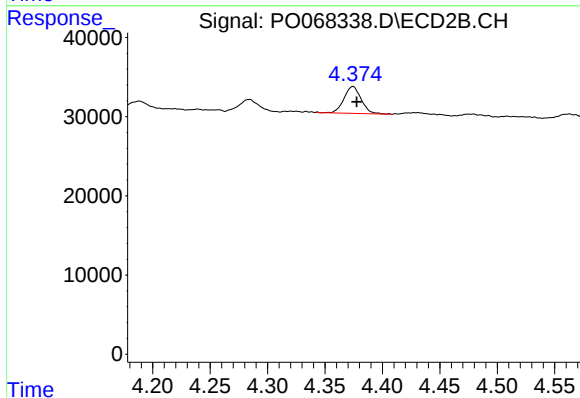


#11 AR-1232-1

R.T.: 4.374 min
Delta R.T.: -0.003 min
Response: 35785
Conc: 46.39 ng/ml

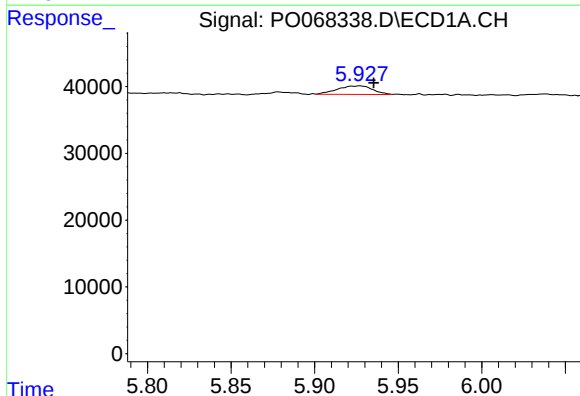


#12 AR-1232-2

R.T.: 5.927 min
Delta R.T.: -0.009 min
Response: 18991
Conc: 61.63 ng/ml m

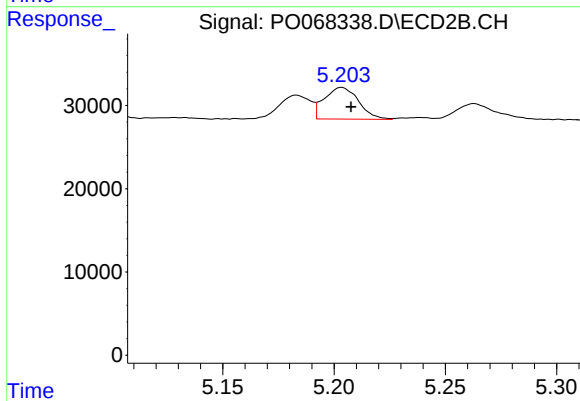

#12 AR-1232-2

R.T.: 5.203 min
Delta R.T.: -0.004 min
Response: 40846
Conc: 51.00 ng/ml

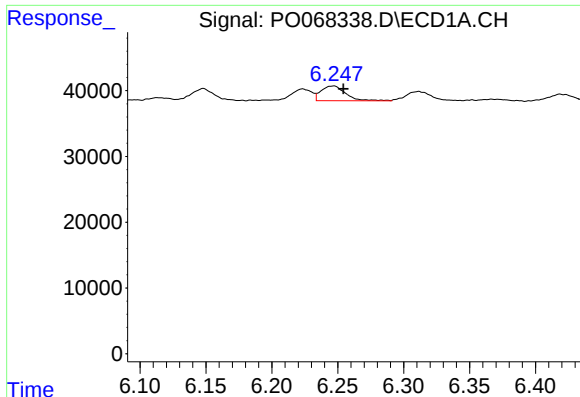


#13 AR-1232-3

R.T.: 6.247 min
Delta R.T.: -0.008 min
Response: 29180
Conc: 45.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:51 PM

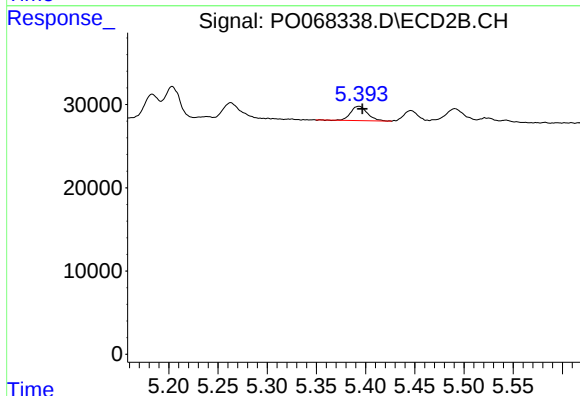


#13 AR-1232-3

R.T.: 5.393 min
Delta R.T.: -0.004 min
Response: 20405
Conc: 48.05 ng/ml

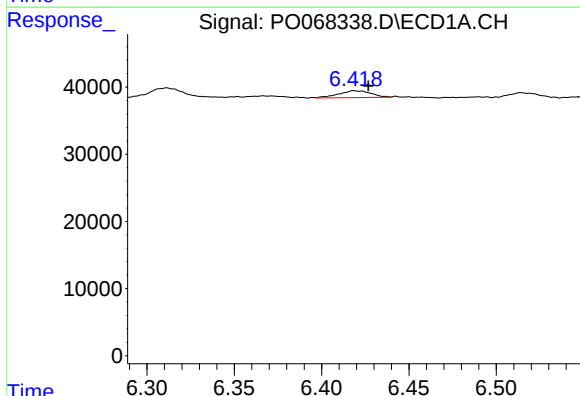


#14 AR-1232-4

R.T.: 6.418 min
Delta R.T.: -0.009 min
Response: 13057
Conc: 41.48 ng/ml m

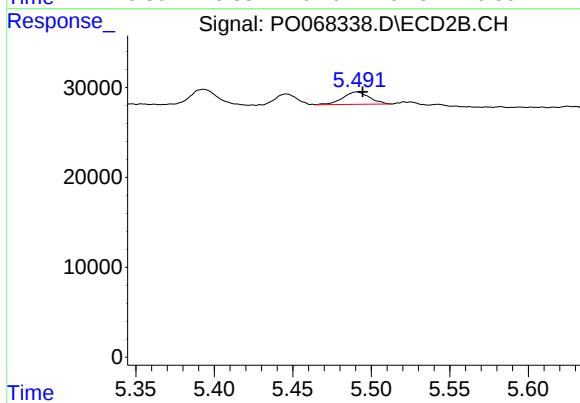

#14 AR-1232-4

R.T.: 5.491 min
Delta R.T.: -0.004 min
Response: 16376
Conc: 43.62 ng/ml

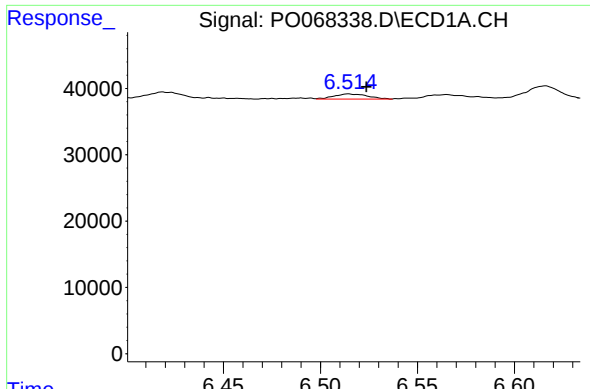


#15 AR-1232-5

R.T.: 6.515 min
Delta R.T.: -0.009 min
Response: 9493
Conc: 44.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:51 PM

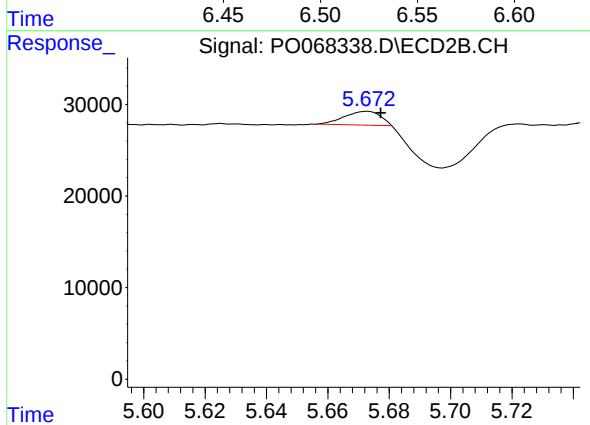

#15 AR-1232-5

R.T.: 5.672 min
Delta R.T.: -0.005 min
Response: 12352
Conc: 29.65 ng/ml m