

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051320\
 Data File : P0068343.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2020 13:57
 Operator : DD\AJ
 Sample : L2182-07
 Misc : AR1262 40PPB LOD
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/14/2020 2:30:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:03:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.906	3.932	645634	794152	23.020	23.144
2) SA Decachlor...	10.860	9.204	907449	957775	22.804m	24.878m
Target Compounds						
36) L8 AR-1262-1	8.533	7.296	114150	86344	57.058	60.698
37) L8 AR-1262-2	9.083	7.847	197328	267758	54.741	57.614
38) L8 AR-1262-3	9.384	8.132	134167	142890	51.690m	74.002 #
39) L8 AR-1262-4	9.479	8.195	107880	210063	52.214	59.806
40) L8 AR-1262-5	10.131	8.691	70482	104808	46.134	60.755 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051320\
Data File : P0068343.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2020 13:57
Operator : DD\AJ
Sample : L2182-07
Misc : AR1262 40PPB LOD
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:03:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

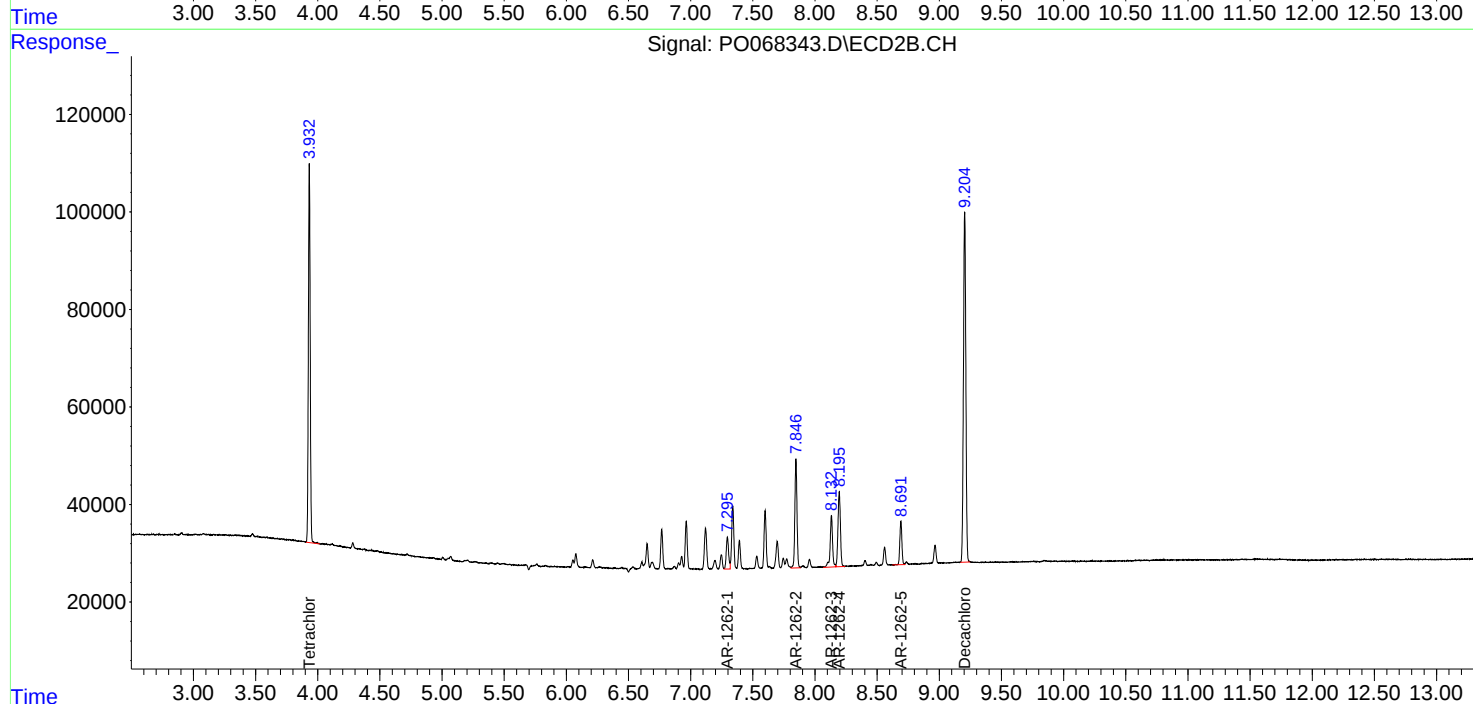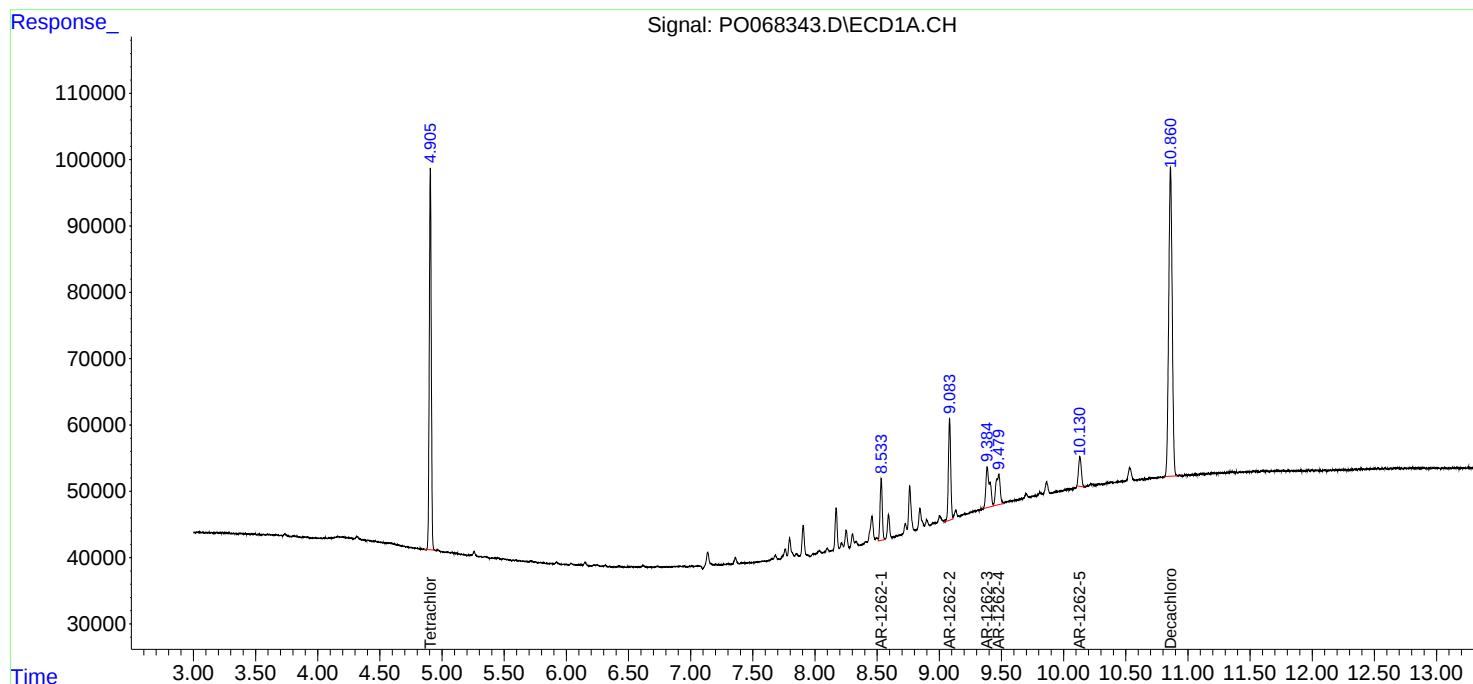

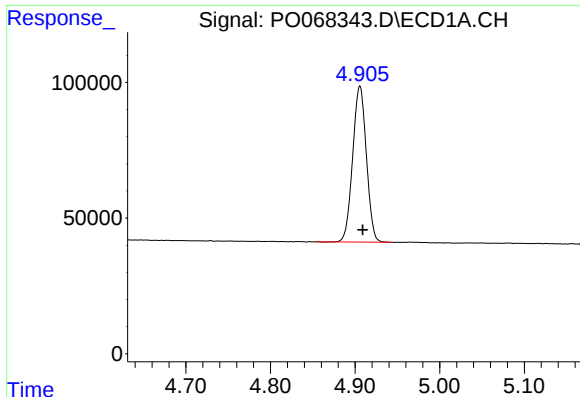


#1 Tetrachloro-m-xylene

R.T.: 4.906 min
Delta R.T.: -0.003 min
Response: 645634
Conc: 23.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:54 PM

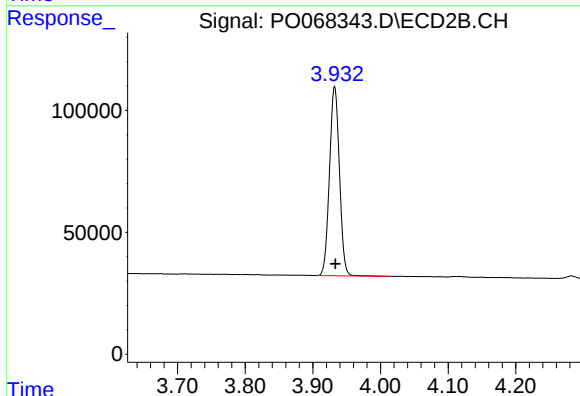


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 794152
Conc: 23.14 ng/ml

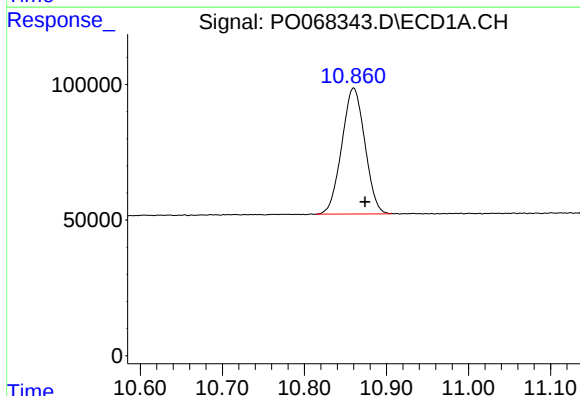


#2 Decachlorobiphenyl

R.T.: 10.860 min
Delta R.T.: -0.014 min
Response: 907449
Conc: 22.80 ng/ml m

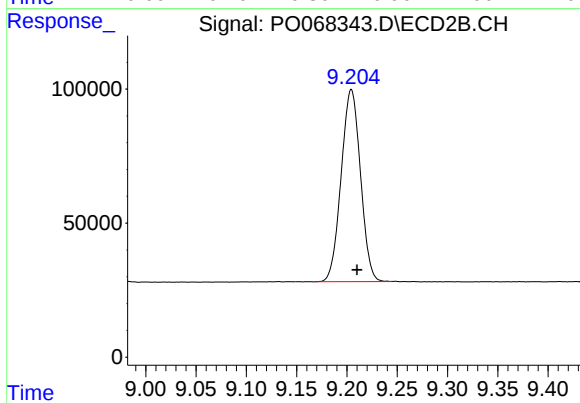

#2 Decachlorobiphenyl

R.T.: 9.204 min
Delta R.T.: -0.006 min
Response: 957775
Conc: 24.88 ng/ml m

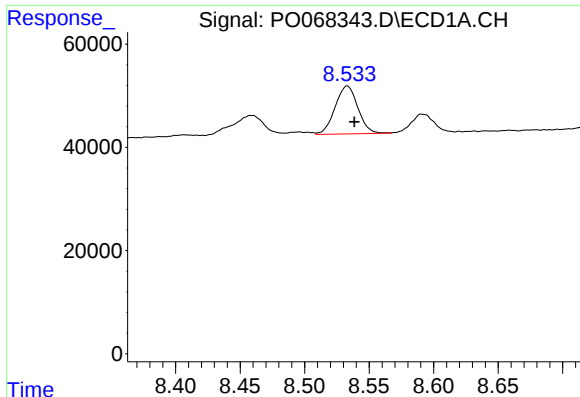


#36 AR-1262-1

R.T.: 8.533 min
Delta R.T.: -0.005 min
Response: 114150
Conc: 57.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:54 PM

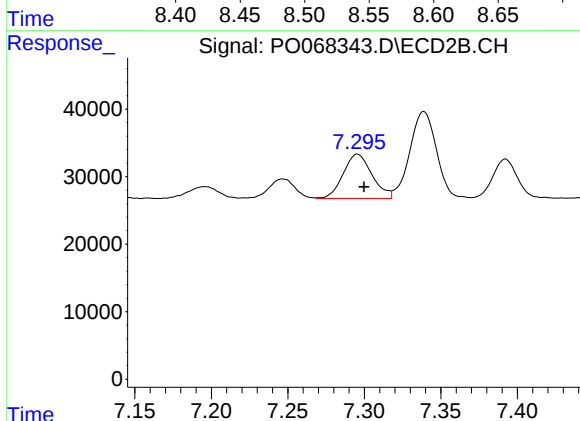


#36 AR-1262-1

R.T.: 7.296 min
Delta R.T.: -0.004 min
Response: 86344
Conc: 60.70 ng/ml

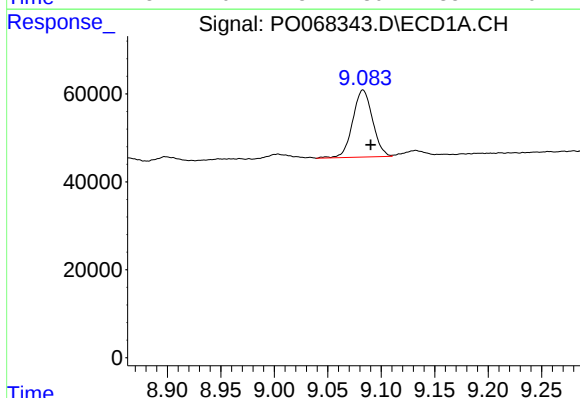


#37 AR-1262-2

R.T.: 9.083 min
Delta R.T.: -0.007 min
Response: 197328
Conc: 54.74 ng/ml

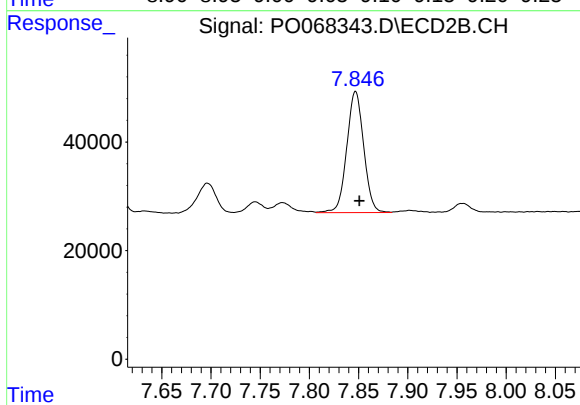

#37 AR-1262-2

R.T.: 7.847 min
Delta R.T.: -0.004 min
Response: 267758
Conc: 57.61 ng/ml

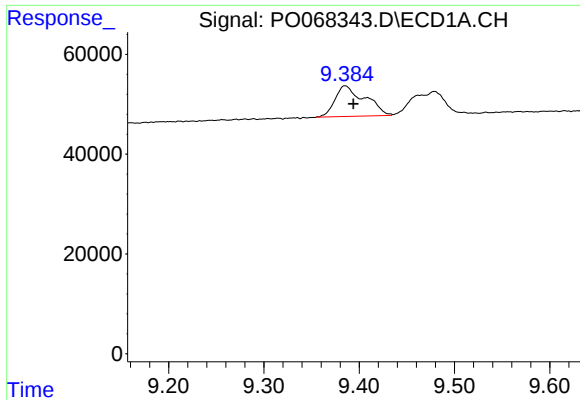


#38 AR-1262-3

R.T.: 9.384 min
Delta R.T.: -0.010 min
Response: 134167
Conc: 51.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020


Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:54 PM

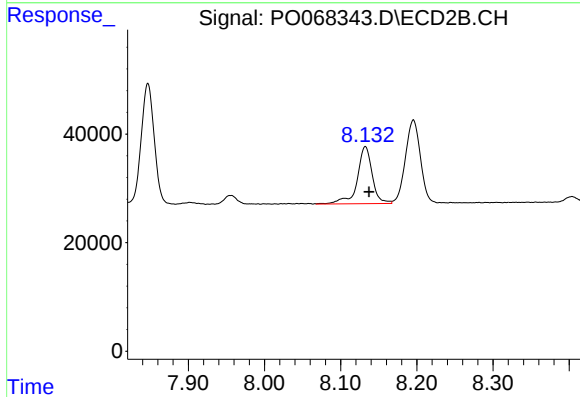


#38 AR-1262-3

R.T.: 8.132 min
Delta R.T.: -0.005 min
Response: 142890
Conc: 74.00 ng/ml

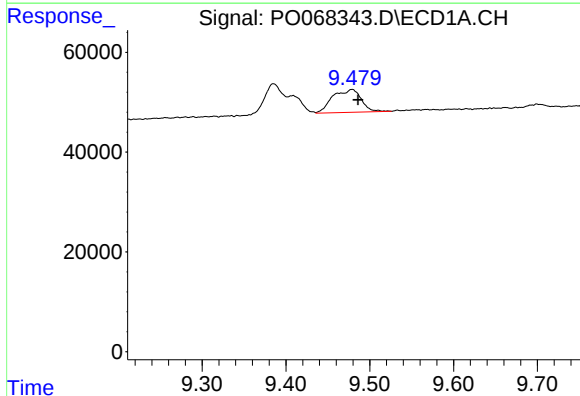


#39 AR-1262-4

R.T.: 9.479 min
Delta R.T.: -0.007 min
Response: 107880
Conc: 52.21 ng/ml

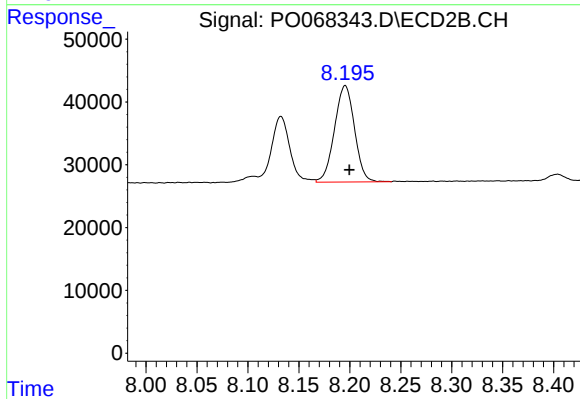

#39 AR-1262-4

R.T.: 8.195 min
Delta R.T.: -0.004 min
Response: 210063
Conc: 59.81 ng/ml

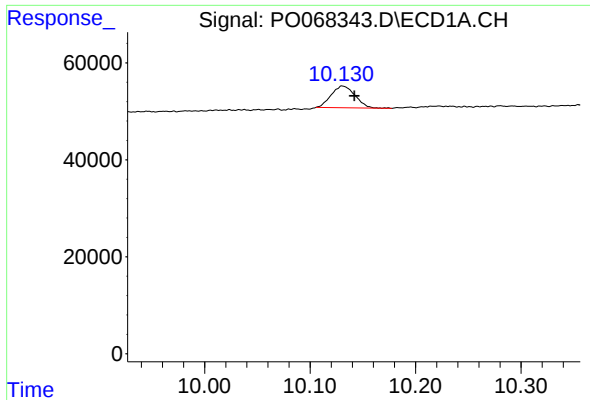


#40 AR-1262-5

R.T.: 10.131 min
Delta R.T.: -0.011 min
Response: 70482
Conc: 46.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

Manual Integrations
APPROVED

Sohil
5/14/2020 2:30:54 PM

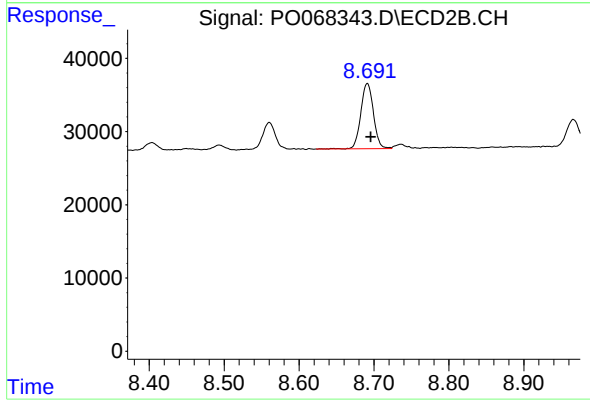

#40 AR-1262-5

R.T.: 8.691 min
Delta R.T.: -0.004 min
Response: 104808
Conc: 60.75 ng/ml