

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051419\
 Data File : P0056224.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2019 14:03
 Operator : SM/SJ
 Sample : K2779-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RT-5124

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 14:27:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.264	3.578	698911	657355	23.355	23.275
2)	SA Decachlor...	9.854	8.524	851663	654860	22.761	24.215
Target Compounds							
27)	L6 AR-1254-2	6.492	0.000	31190	0	9.398	N.D. #
28)	L6 AR-1254-3	6.859	0.000	48099	0	13.230	N.D. #
30)	L6 AR-1254-5	7.556	0.000	22191	0	7.742	N.D. #
31)	L7 AR-1260-1	7.017	0.000	31207	0	14.451	N.D. #
32)	L7 AR-1260-2	7.270	0.000	43425	0	16.581	N.D. #
34)	L7 AR-1260-4	7.851	0.000	58622	0	25.349	N.D. #
35)	L7 AR-1260-5	8.163	0.000	52034	0	12.266	N.D. #
37)	L8 AR-1262-2	8.163	0.000	52034	0	9.692	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051419\
Data File : P0056224.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2019 14:03
Operator : SM/SJ
Sample : K2779-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RT-5124

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 14:27:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

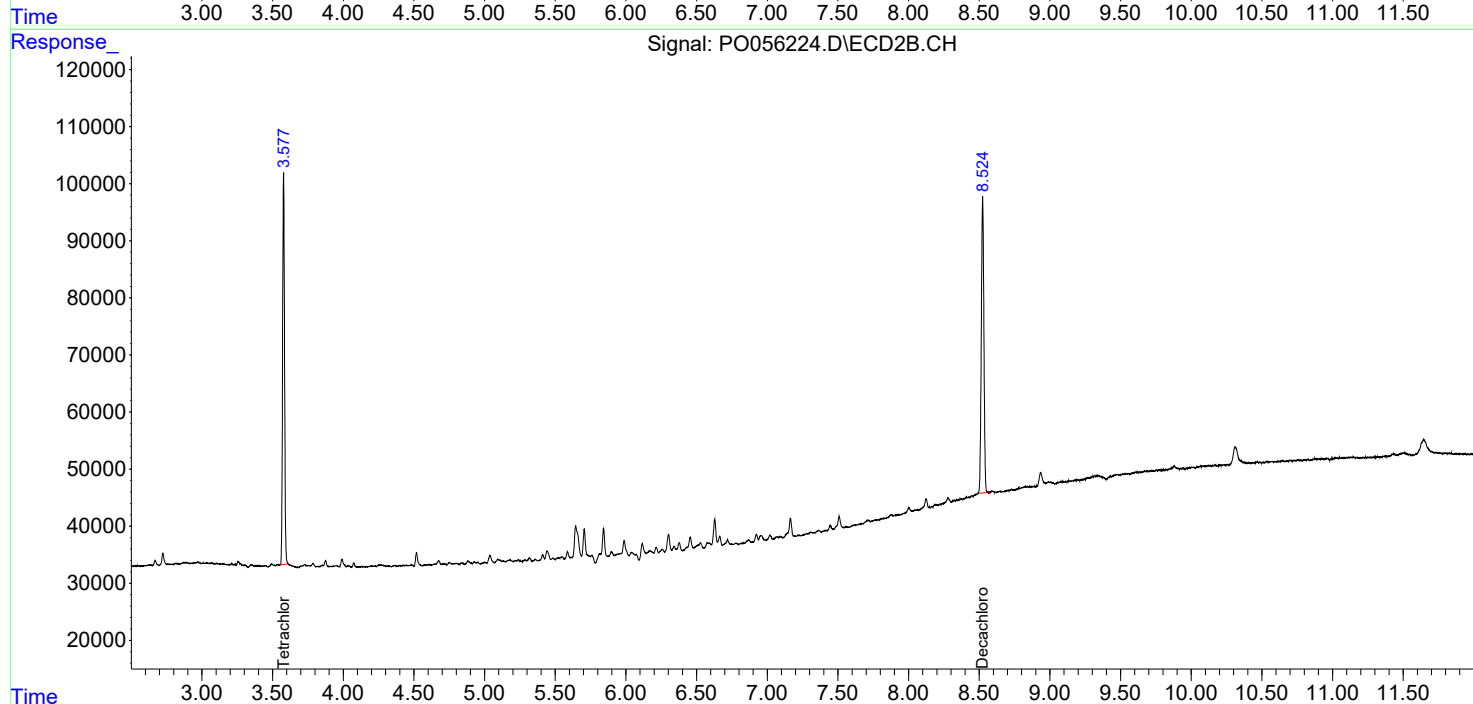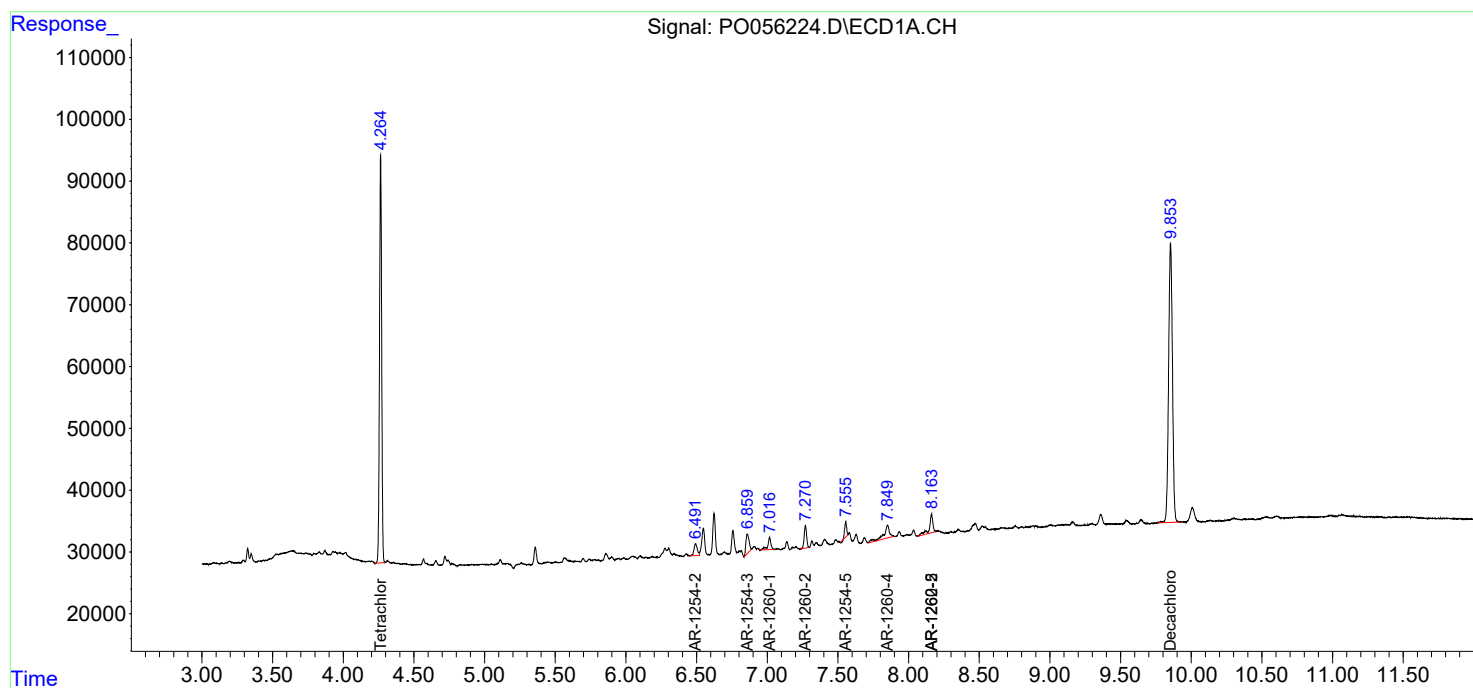


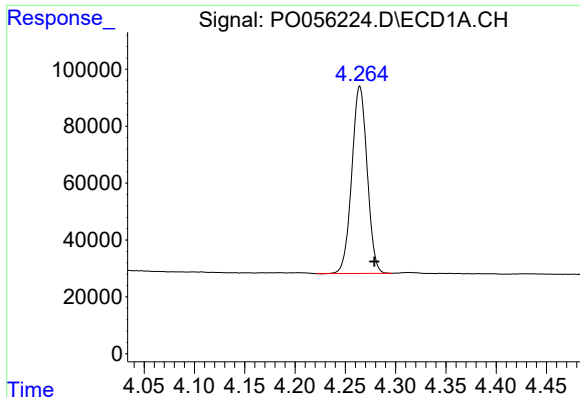

#1 Tetrachloro-m-xylene


R.T.: 4.264 min
Delta R.T.: -0.015 min
Response: 698911
Conc: 23.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-5124

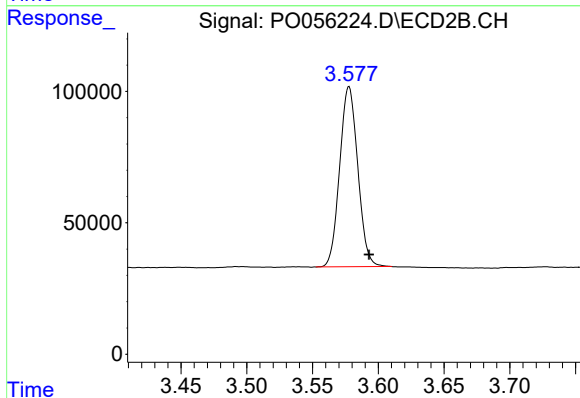


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: -0.015 min
Response: 657355
Conc: 23.27 ng/ml

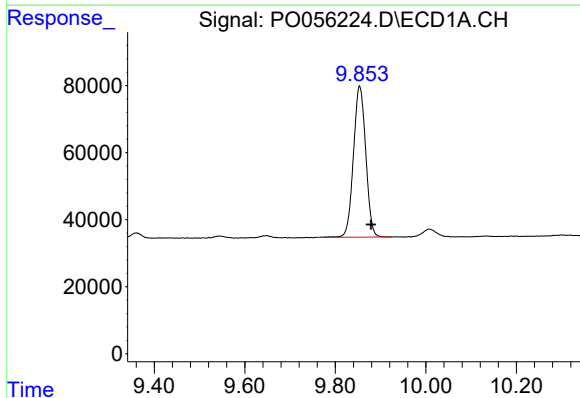


#2 Decachlorobiphenyl

R.T.: 9.854 min
Delta R.T.: -0.025 min
Response: 851663
Conc: 22.76 ng/ml

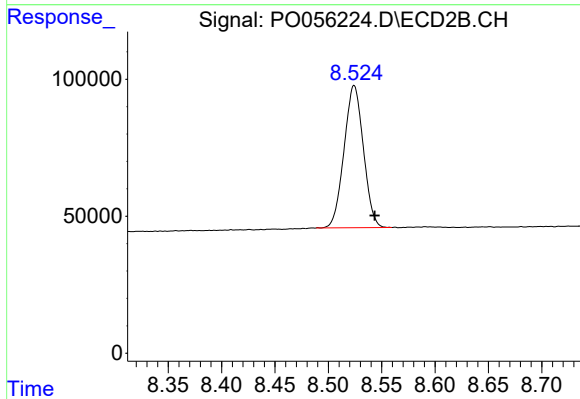

#2 Decachlorobiphenyl


R.T.: 8.524 min
Delta R.T.: -0.019 min
Response: 654860
Conc: 24.22 ng/ml

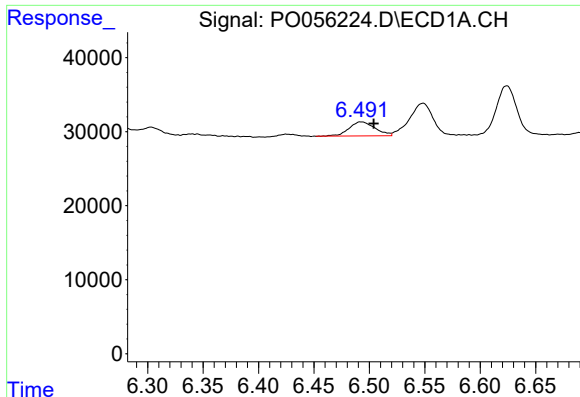

#27 AR-1254-2


R.T.: 6.492 min
Delta R.T.: -0.012 min
Response: 31190
Conc: 9.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-5124

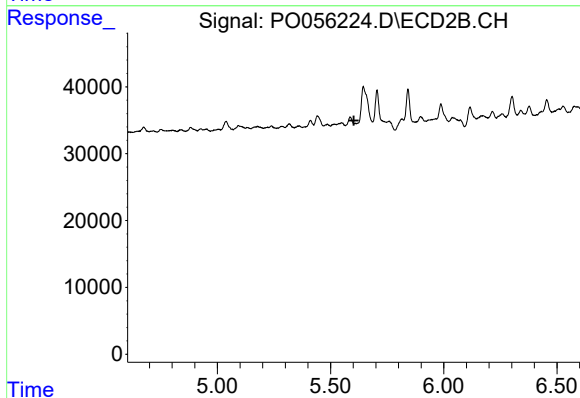


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.603 min
Response: 0
Conc: N.D.

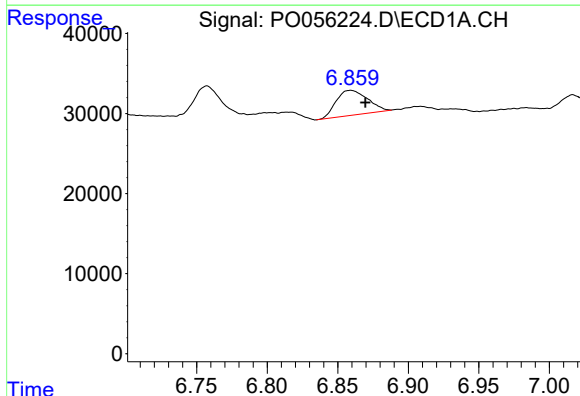


#28 AR-1254-3

R.T.: 6.859 min
Delta R.T.: -0.010 min
Response: 48099
Conc: 13.23 ng/ml

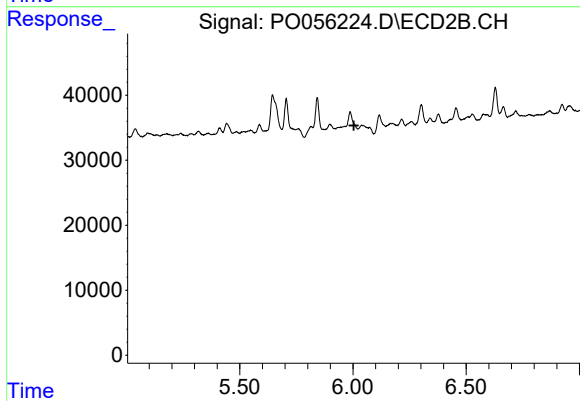

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.

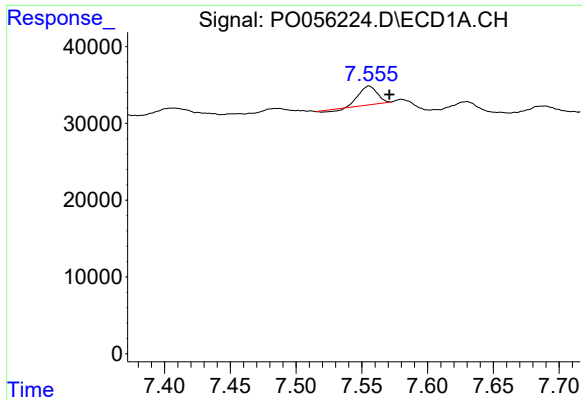

#30 AR-1254-5


R.T.: 7.556 min
Delta R.T.: -0.015 min
Response: 22191
Conc: 7.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-5124

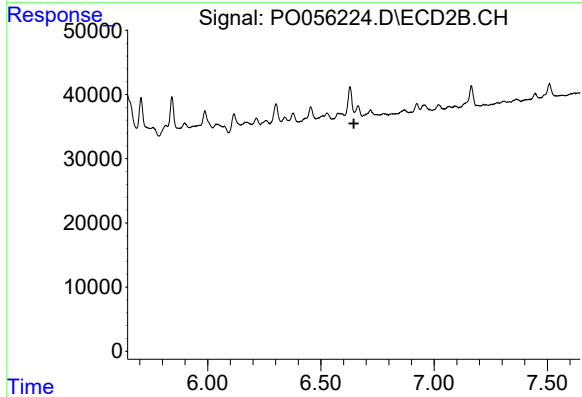


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

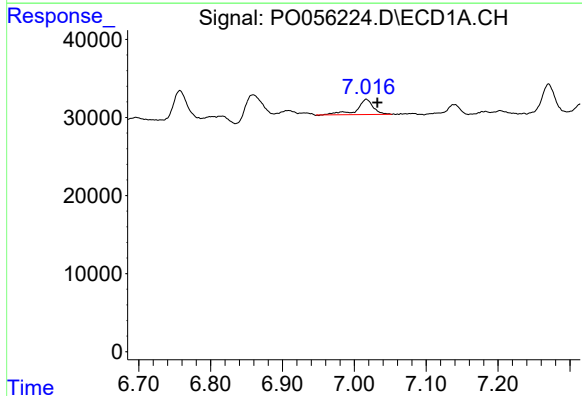


#31 AR-1260-1

R.T.: 7.017 min
Delta R.T.: -0.016 min
Response: 31207
Conc: 14.45 ng/ml

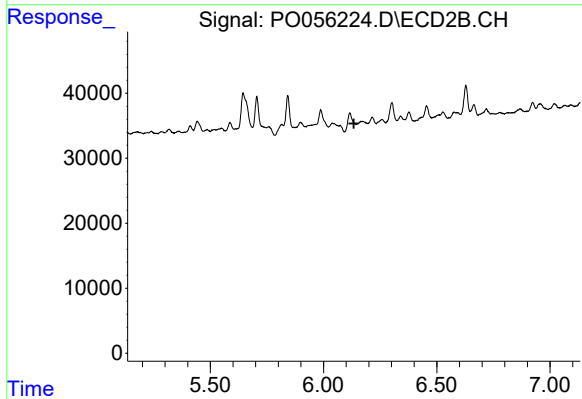

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.134 min
Response: 0
Conc: N.D.

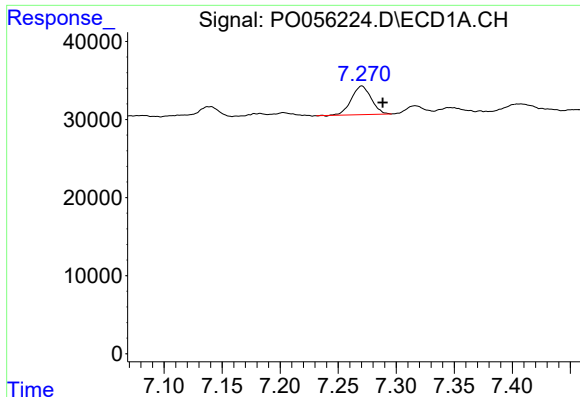

#32 AR-1260-2


R.T.: 7.270 min
Delta R.T.: -0.018 min
Response: 43425
Conc: 16.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-5124

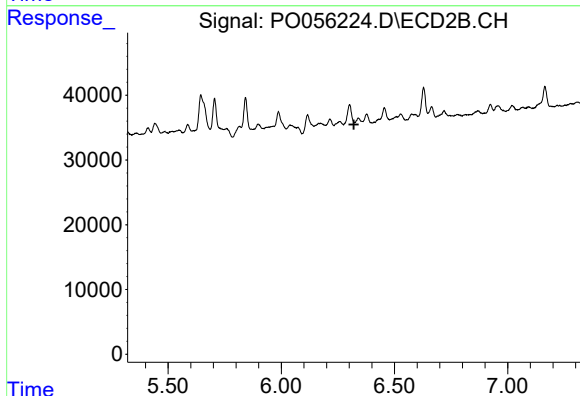


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.320 min
Response: 0
Conc: N.D.

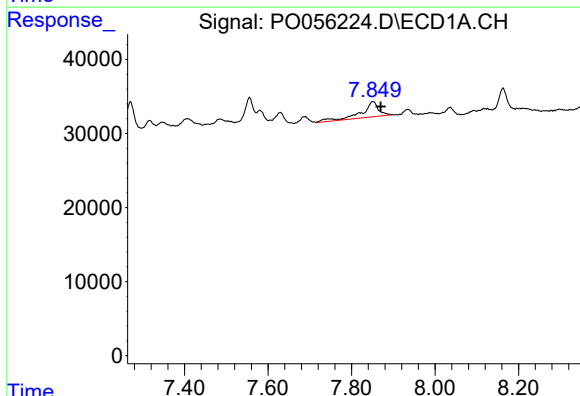


#34 AR-1260-4

R.T.: 7.851 min
Delta R.T.: -0.019 min
Response: 58622
Conc: 25.35 ng/ml

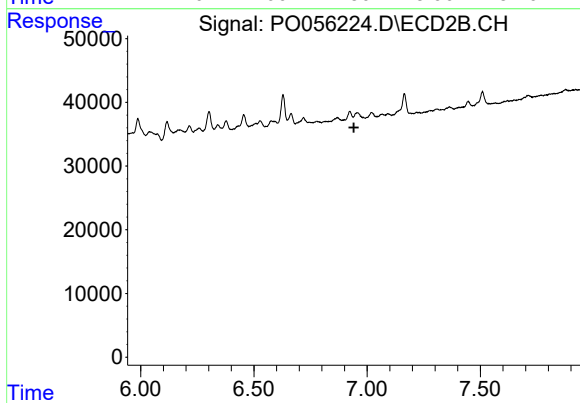

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.942 min
Response: 0
Conc: N.D.

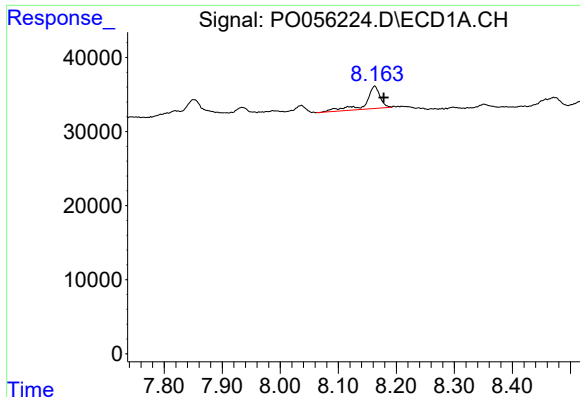

#35 AR-1260-5


R.T.: 8.163 min
Delta R.T.: -0.016 min
Response: 52034
Conc: 12.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-5124

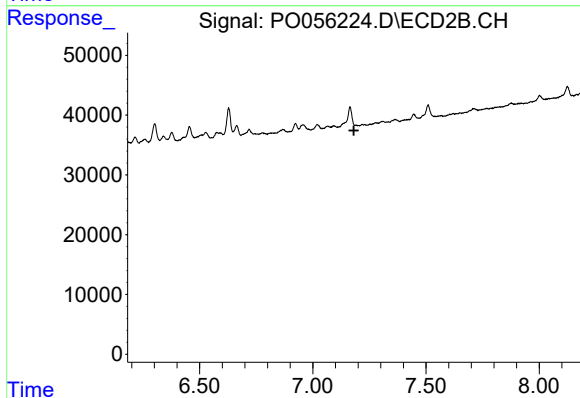


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

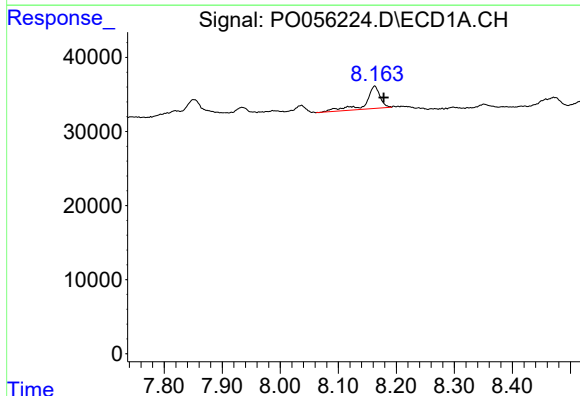

#37 AR-1262-2

R.T.: 8.163 min
Delta R.T.: -0.015 min
Response: 52034
Conc: 9.69 ng/ml

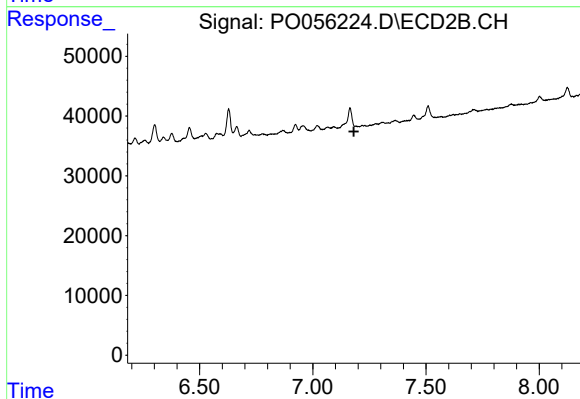

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.181 min
Response: 0
Conc: N.D.