

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051419\
 Data File : P0056222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2019 13:28
 Operator : SM/SJ
 Sample : K2771-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-047

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 14:27:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.579	762284	721618	25.473	25.550
2) SA Decachlor...	9.867	8.526	873887	675325	23.355	24.972

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051419\
Data File : P0056222.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2019 13:28
Operator : SM/SJ
Sample : K2771-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 14:27:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

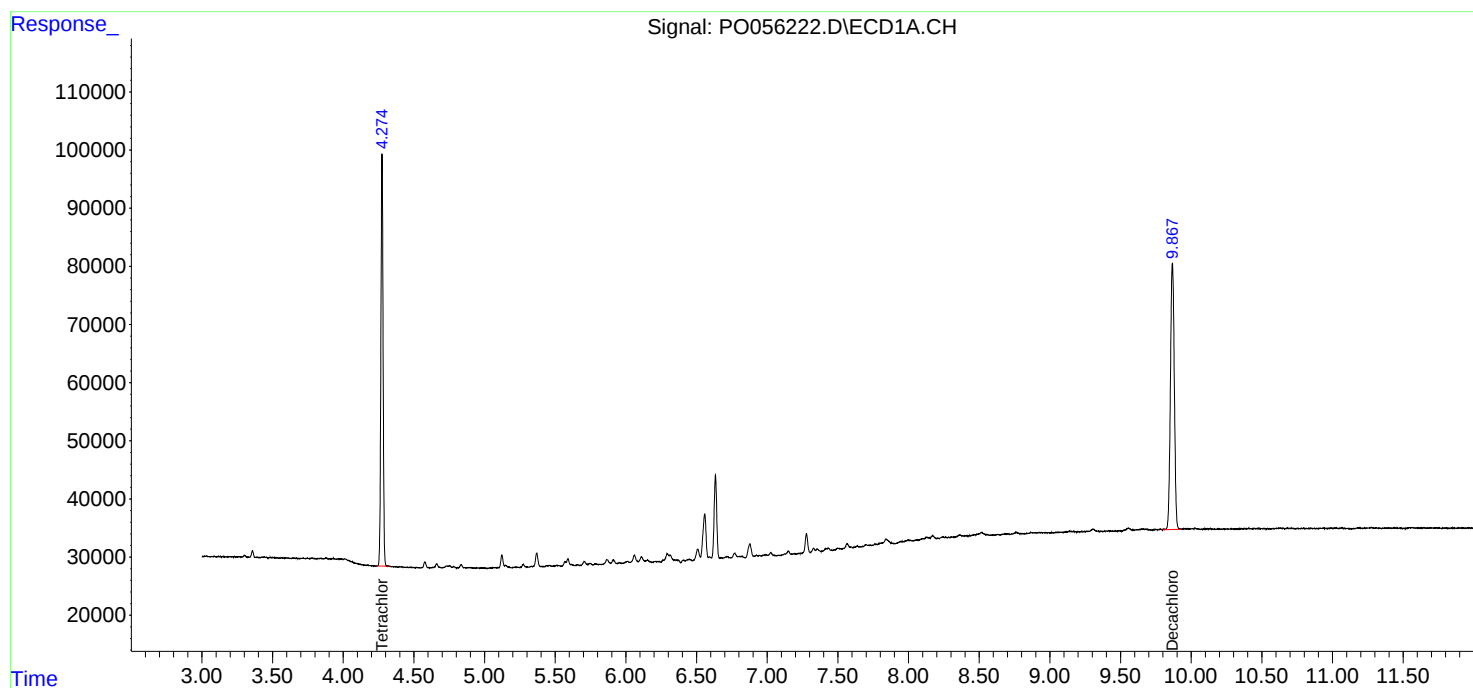


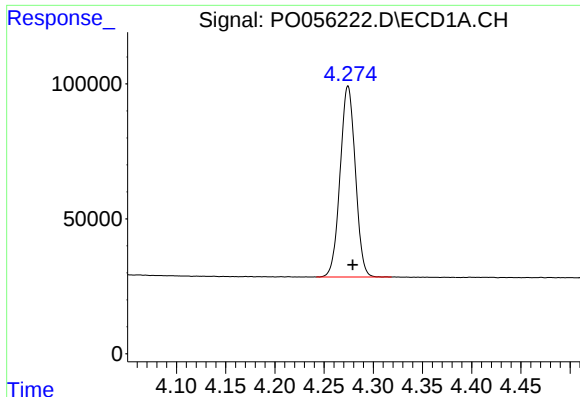

#1 Tetrachloro-m-xylene


R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 762284
Conc: 25.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047

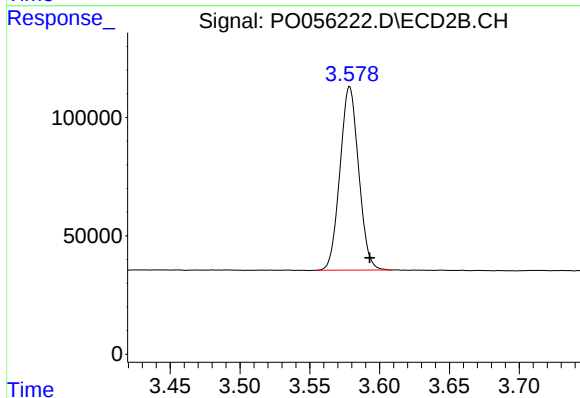


#1 Tetrachloro-m-xylene

R.T.: 3.579 min
Delta R.T.: -0.014 min
Response: 721618
Conc: 25.55 ng/ml

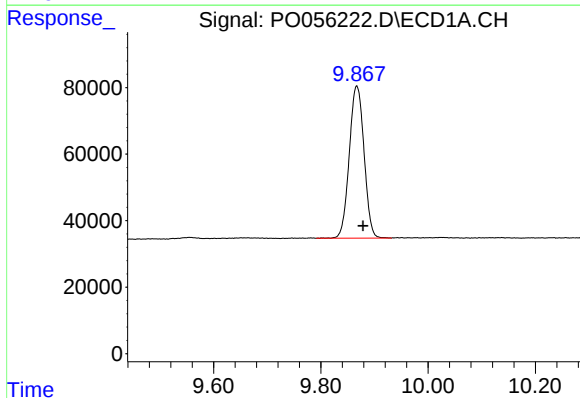

#2 Decachlorobiphenyl

R.T.: 9.867 min
Delta R.T.: -0.012 min
Response: 873887
Conc: 23.36 ng/ml

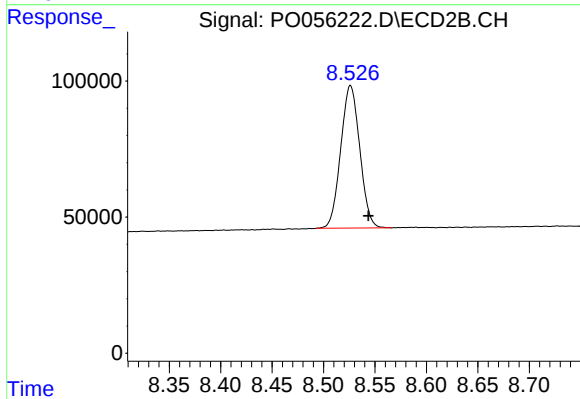

#2 Decachlorobiphenyl

R.T.: 8.526 min
Delta R.T.: -0.017 min
Response: 675325
Conc: 24.97 ng/ml