

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051419\
 Data File : P0056223.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2019 13:45
 Operator : SM/SJ
 Sample : K2774-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-048

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 14:27:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.263	3.578	764003	713303	25.530	25.256
2) SA Decachlor...	9.852	8.523	881407	673674	23.556	24.911

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051419\
Data File : PO056223.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2019 13:45
Operator : SM/SJ
Sample : K2774-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 14:27:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

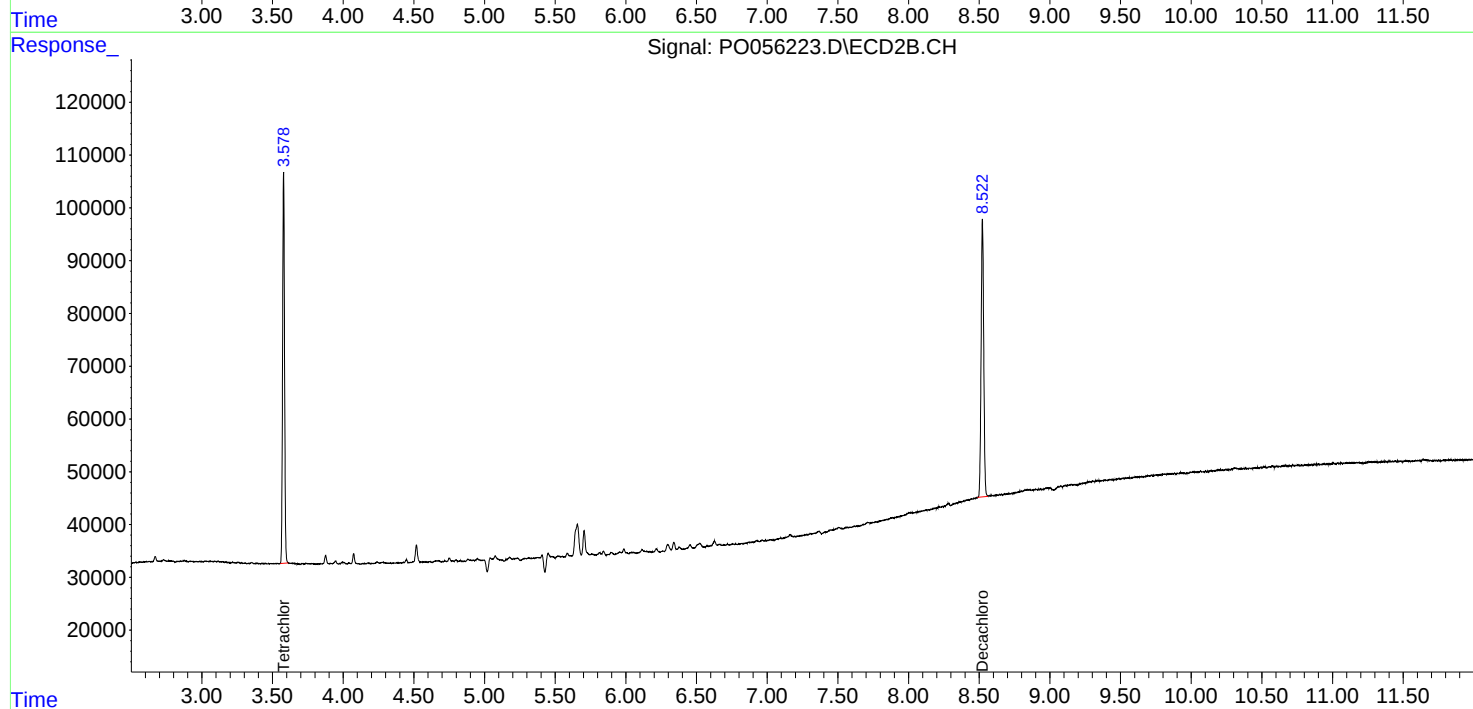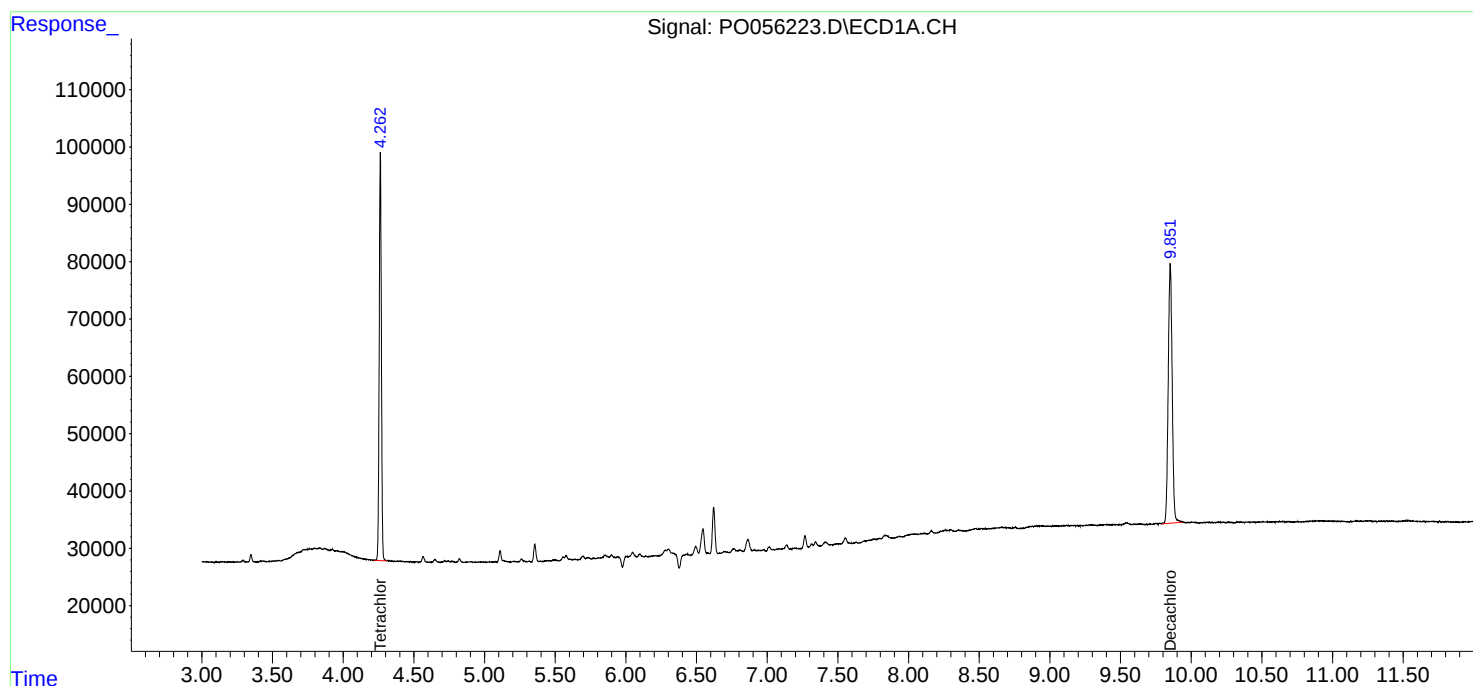


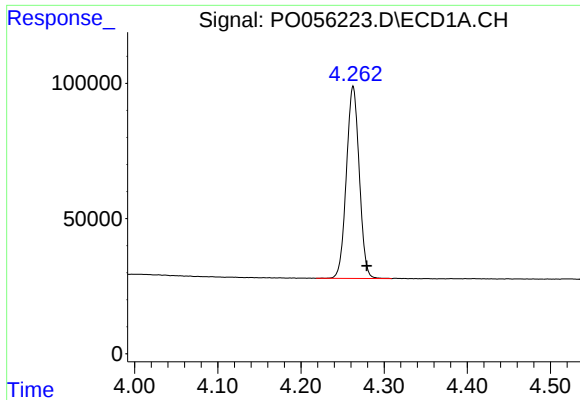

#1 Tetrachloro-m-xylene


R.T.: 4.263 min
Delta R.T.: -0.016 min
Response: 764003
Conc: 25.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-048

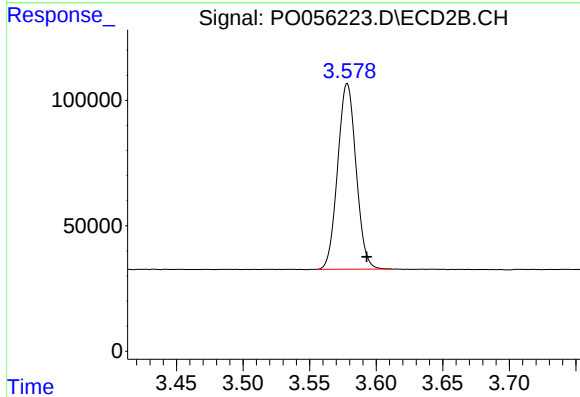


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: -0.015 min
Response: 713303
Conc: 25.26 ng/ml

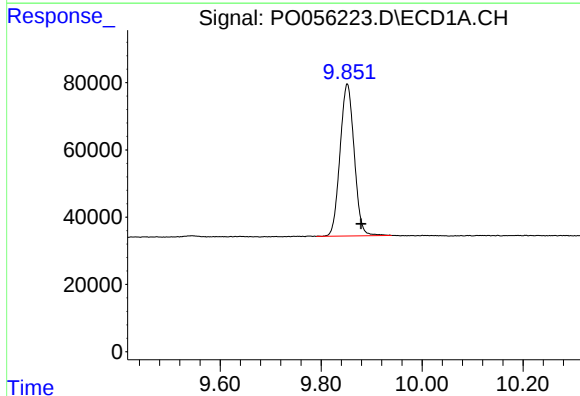

#2 Decachlorobiphenyl

R.T.: 9.852 min
Delta R.T.: -0.027 min
Response: 881407
Conc: 23.56 ng/ml

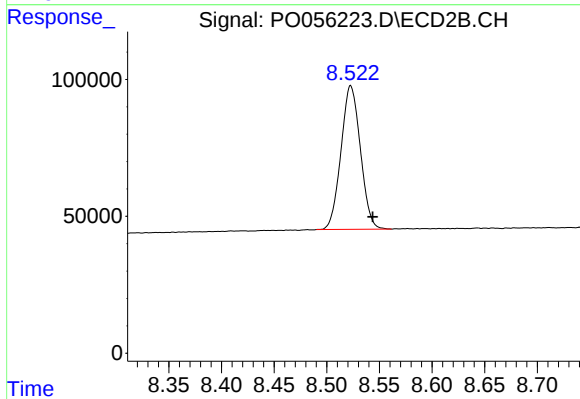

#2 Decachlorobiphenyl

R.T.: 8.523 min
Delta R.T.: -0.021 min
Response: 673674
Conc: 24.91 ng/ml