

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051420\
 Data File : P0068371.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2020 13:01
 Operator : DD\AJ
 Sample : L2594-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-056-A

Manual Integrations
 APPROVED

Sohil
 5/15/2020 12:34:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 22:58:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.902	3.932	1099480	1357299	39.202	39.555
2) SA Decachlor...	10.853	9.204	1407078	1292973	35.360m	33.584

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051420\
Data File : P0068371.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2020 13:01
Operator : DD\AJ
Sample : L2594-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-GF-02-056-A


Manual Integrations
APPROVED

Sohil
5/15/2020 12:34:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 22:58:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

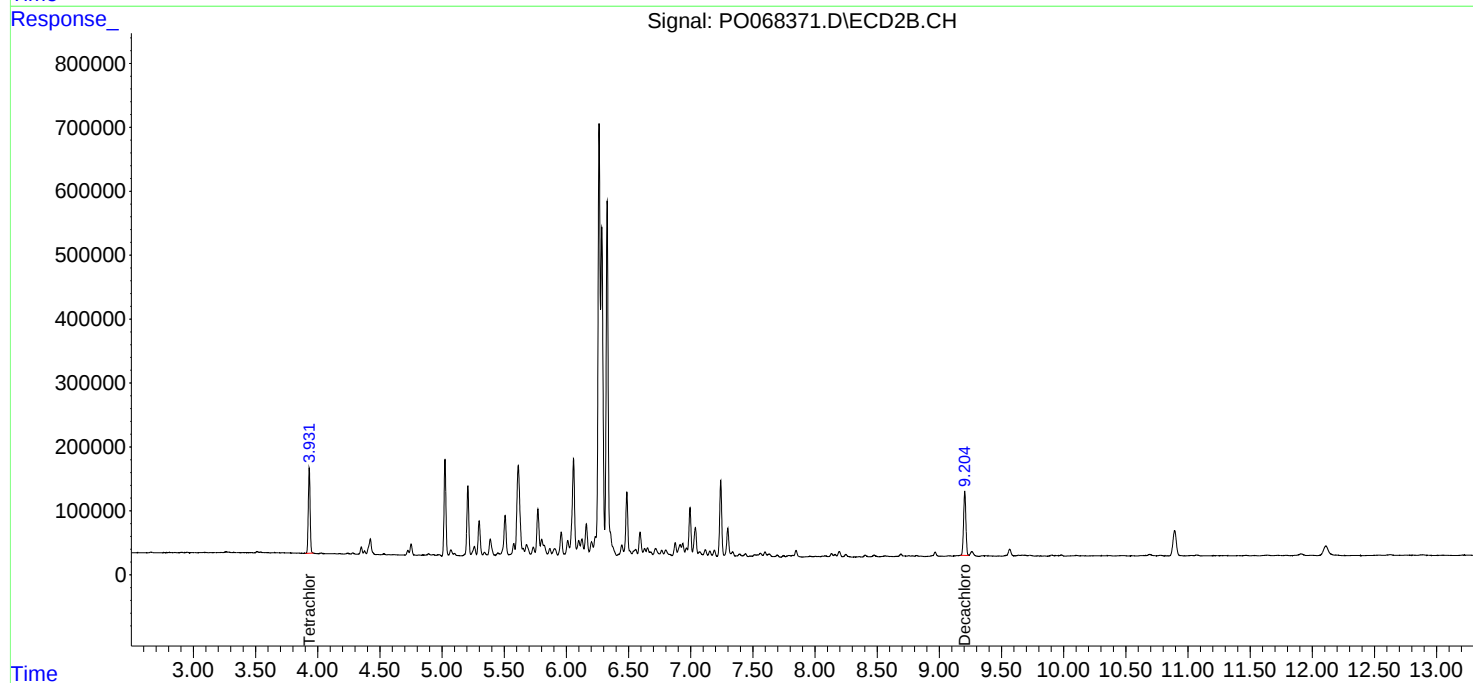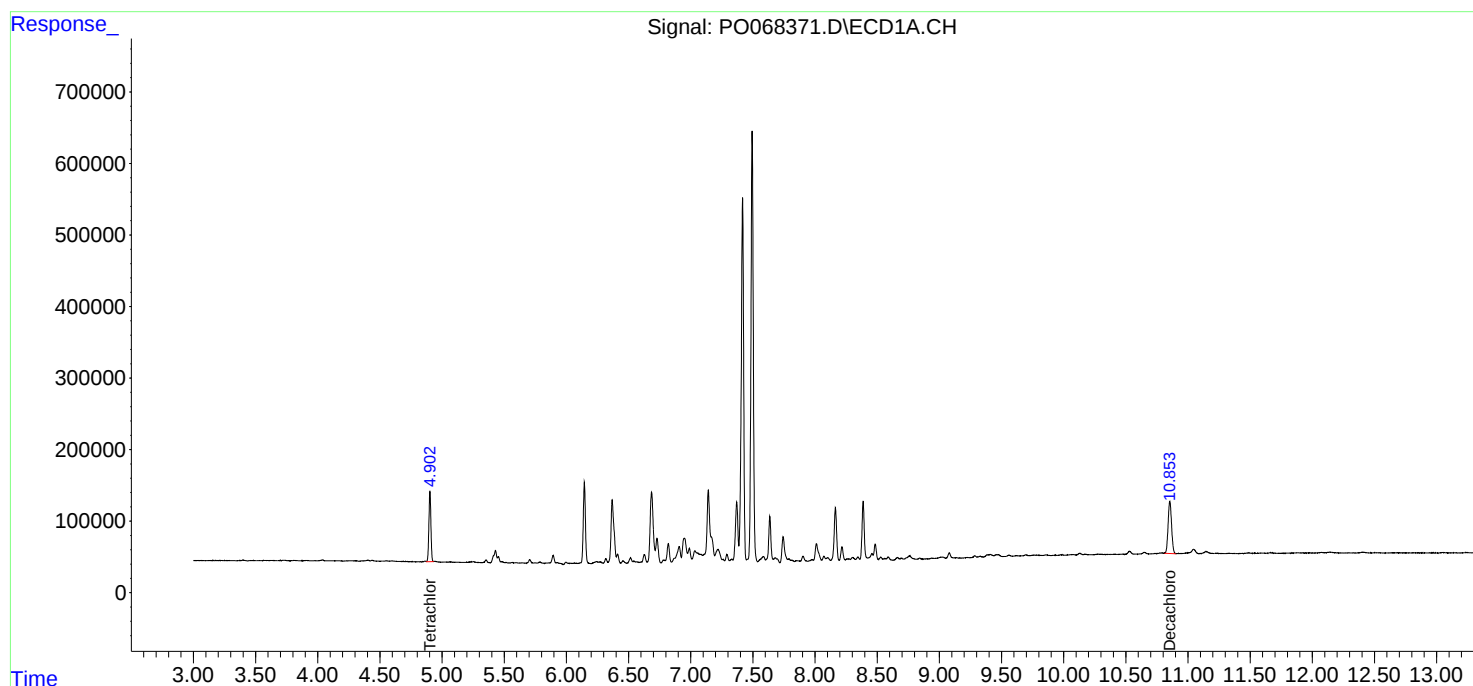

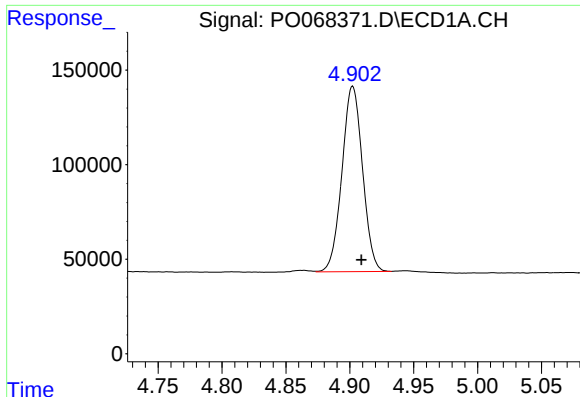


#1 Tetrachloro-m-xylene

R.T.: 4.902 min
Delta R.T.: -0.007 min
Response: 1099480
Conc: 39.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-056-A


Manual Integrations
APPROVED

Sohil
5/15/2020 12:34:52 PM

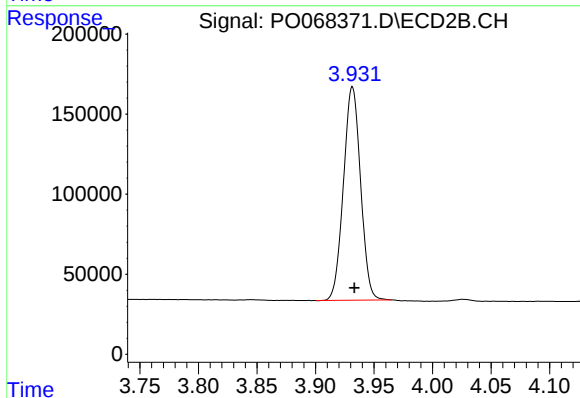


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.002 min
Response: 1357299
Conc: 39.56 ng/ml

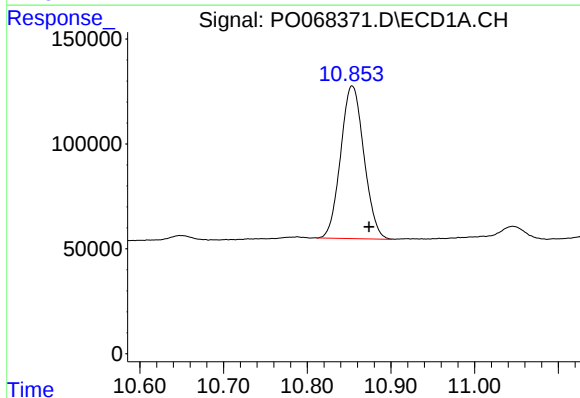

#2 Decachlorobiphenyl

R.T.: 10.853 min
Delta R.T.: -0.021 min
Response: 1407078
Conc: 35.36 ng/ml m

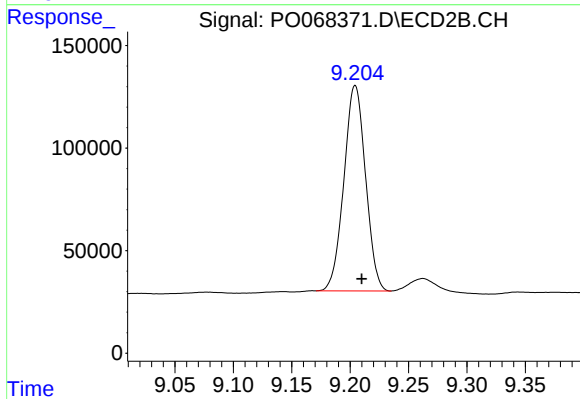

#2 Decachlorobiphenyl

R.T.: 9.204 min
Delta R.T.: -0.006 min
Response: 1292973
Conc: 33.58 ng/ml