

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051520\
 Data File : P0068382.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 May 2020 9:21
 Operator : DD\AJ
 Sample : L2635-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROLL-OFF-P72-11933

Manual Integrations
 APPROVED

Sohil
 5/18/2020 3:39:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 01:07:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.902	3.932	769789	946541	27.447m	27.585
2) SA Decachlor...	10.855	9.204	896109	915632	22.519	23.783

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051520\
Data File : P0068382.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 May 2020 9:21
Operator : DD\AJ
Sample : L2635-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROLL-OFF-P72-11933


Manual Integrations
APPROVED

Sohil
5/18/2020 3:39:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 01:07:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

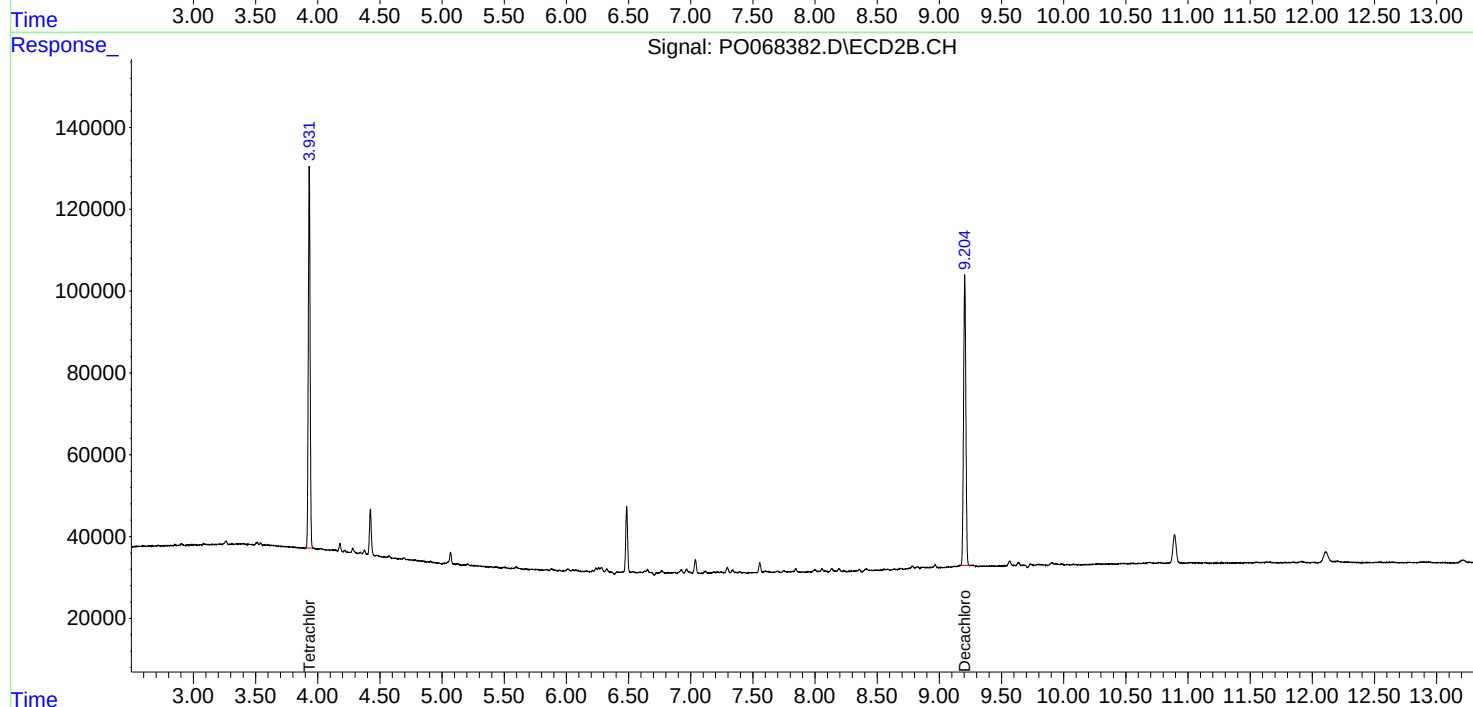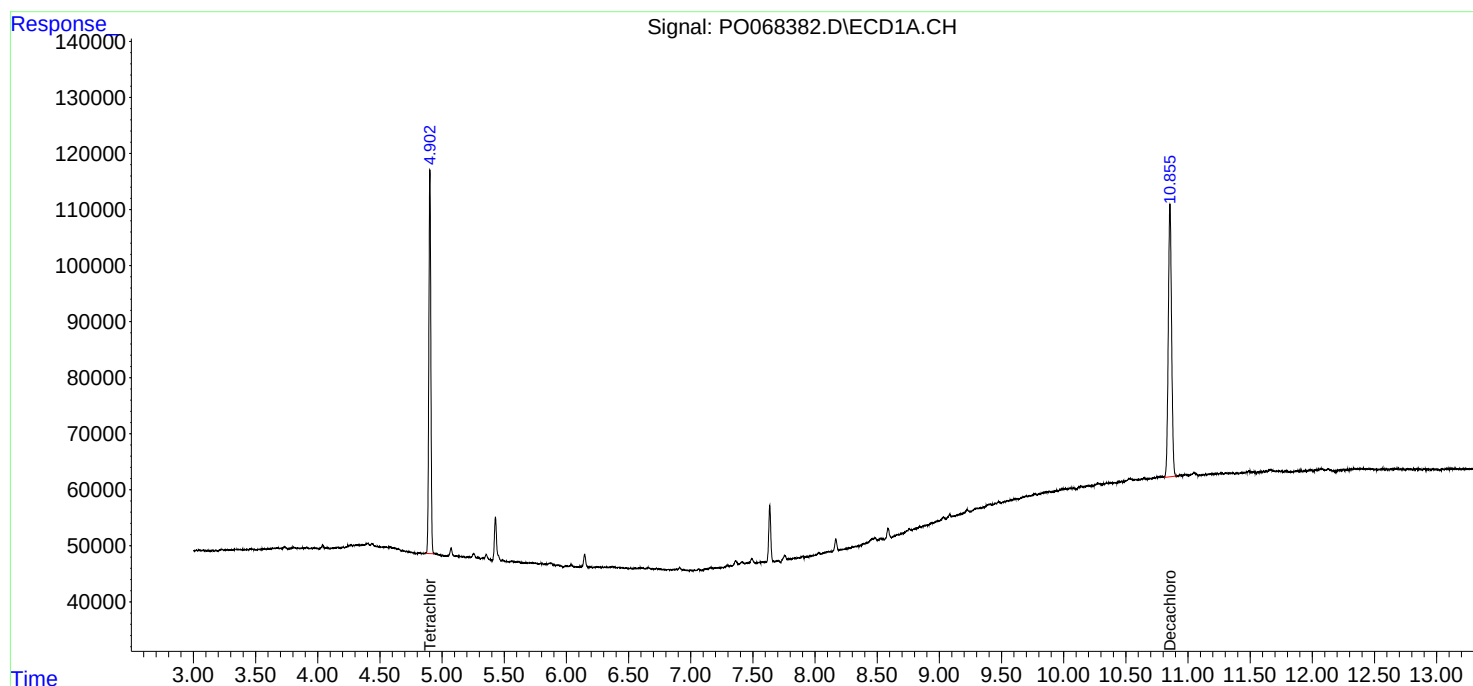

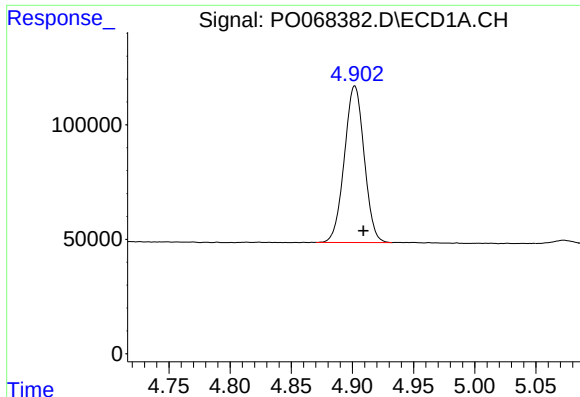


#1 Tetrachloro-m-xylene

R.T.: 4.902 min
Delta R.T.: -0.007 min
Response: 769789
Conc: 27.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ROLL-OFF-P72-11933


Manual Integrations
APPROVED

Sohil
5/18/2020 3:39:56 PM

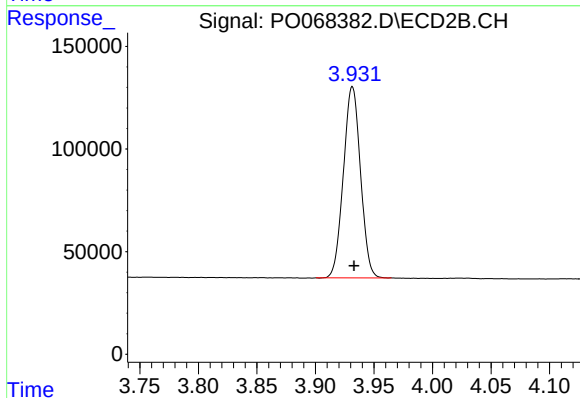


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.002 min
Response: 946541
Conc: 27.58 ng/ml

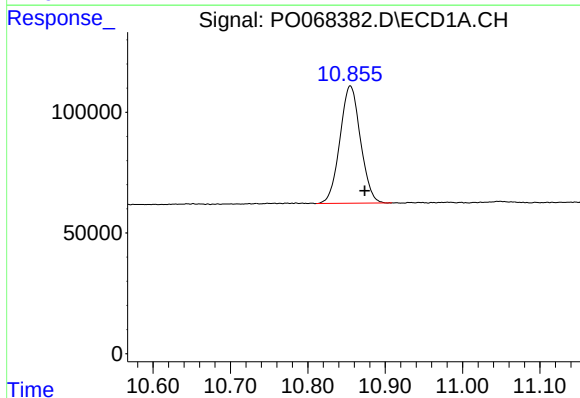

#2 Decachlorobiphenyl

R.T.: 10.855 min
Delta R.T.: -0.019 min
Response: 896109
Conc: 22.52 ng/ml

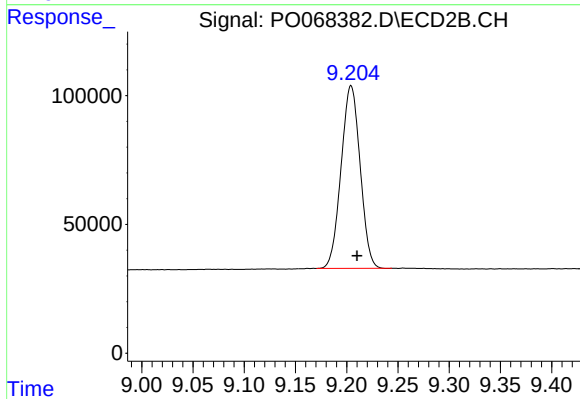

#2 Decachlorobiphenyl

R.T.: 9.204 min
Delta R.T.: -0.006 min
Response: 915632
Conc: 23.78 ng/ml