

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051719\
 Data File : P0056328.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2019 21:23
 Operator : SM/SJ
 Sample : K2884-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-07-20190515

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 23:48:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 17 23:42:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.257	3.577	686786	628180	14.798	14.949
2) SA Decachlor...	9.839	8.516	659272	538871	13.727	13.269

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051719\
Data File : PO056328.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2019 21:23
Operator : SM/SJ
Sample : K2884-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MW-07-20190515

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 23:48:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 17 23:42:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

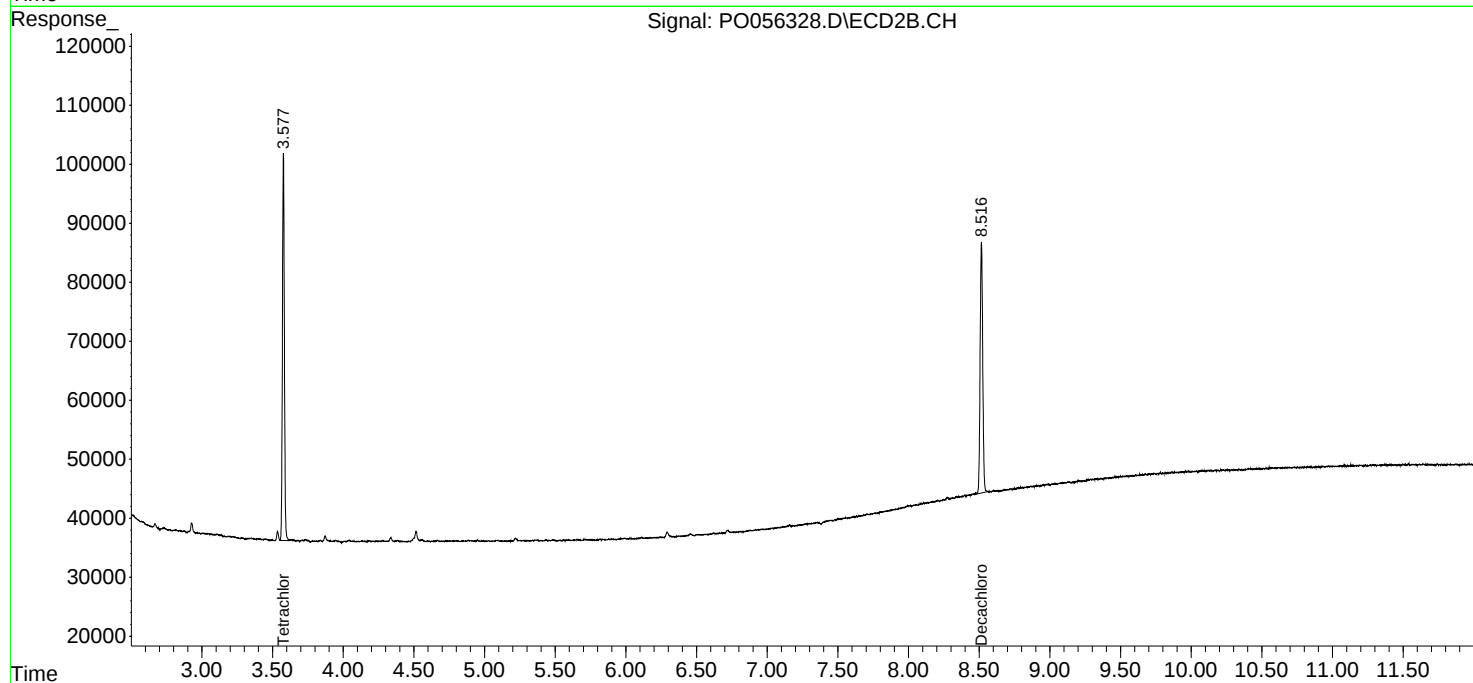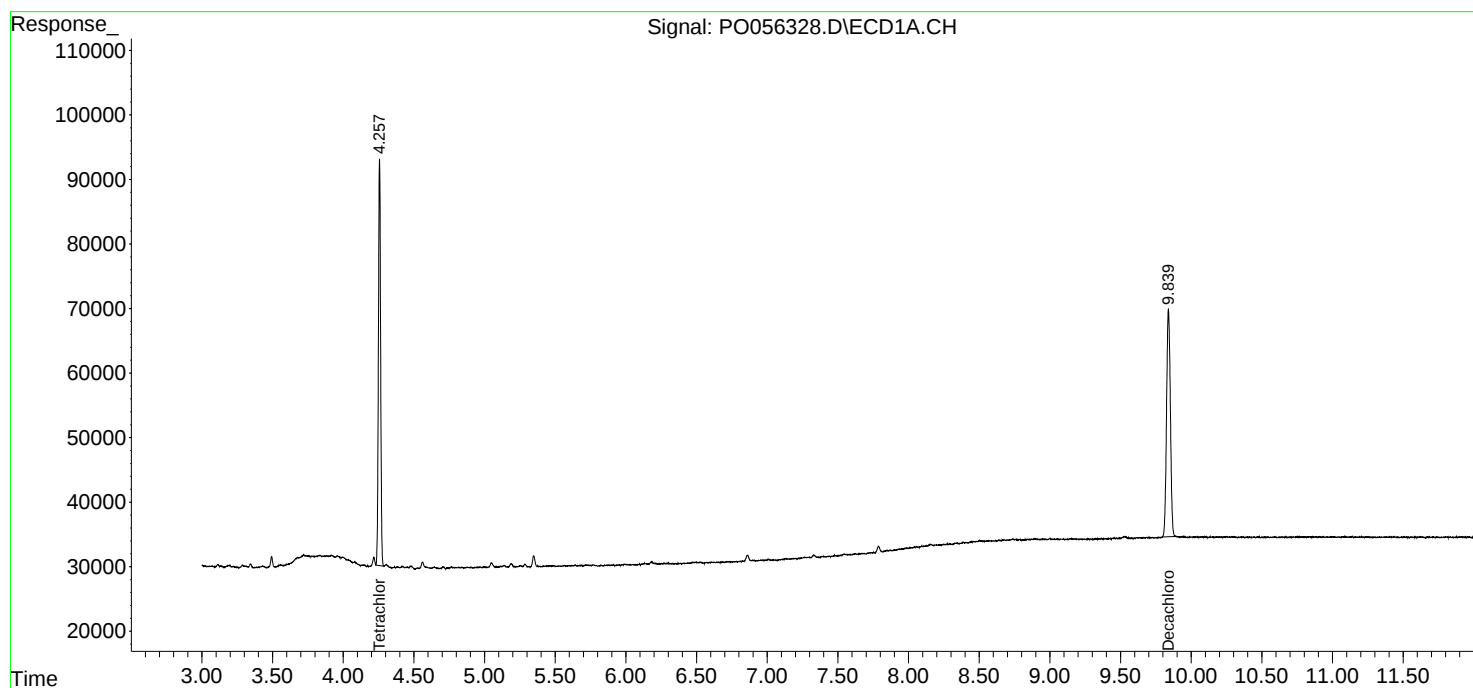


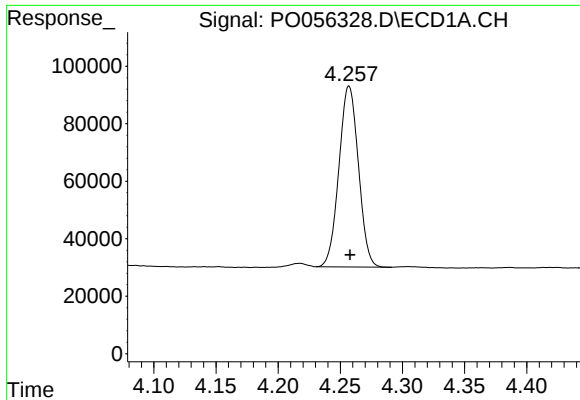

#1 Tetrachloro-m-xylene


R.T.: 4.257 min
Delta R.T.: 0.000 min
Response: 686786
Conc: 14.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-07-20190515

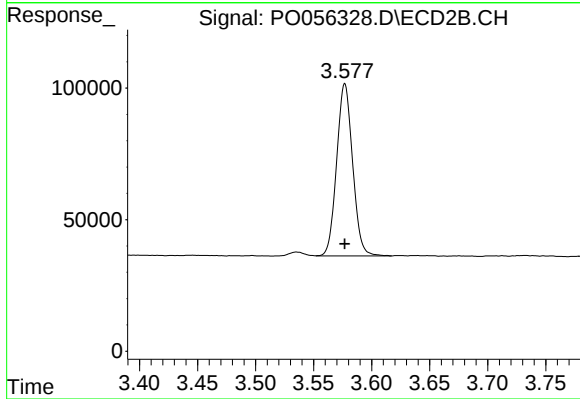


#1 Tetrachloro-m-xylene

R.T.: 3.577 min
Delta R.T.: 0.000 min
Response: 628180
Conc: 14.95 ng/ml

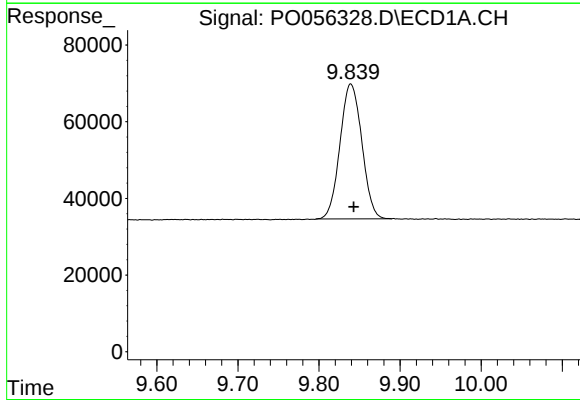

#2 Decachlorobiphenyl

R.T.: 9.839 min
Delta R.T.: -0.004 min
Response: 659272
Conc: 13.73 ng/ml

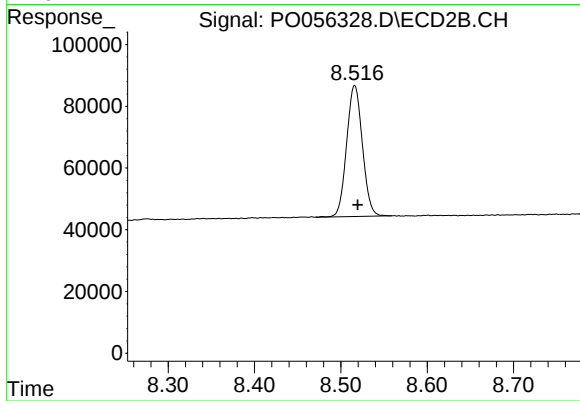

#2 Decachlorobiphenyl

R.T.: 8.516 min
Delta R.T.: -0.003 min
Response: 538871
Conc: 13.27 ng/ml