

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051719\
 Data File : P0056343.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2019 1:38
 Operator : SM/SJ
 Sample : K2869-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-MANHOLE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 02:57:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 17 23:42:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.258	3.578	949043	875761	20.448	20.840
2) SA Decachlor...	9.841	8.517	938244	762840	19.535	18.784

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051719\
Data File : PO056343.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2019 1:38
Operator : SM/SJ
Sample : K2869-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-MANHOLE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 02:57:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 17 23:42:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

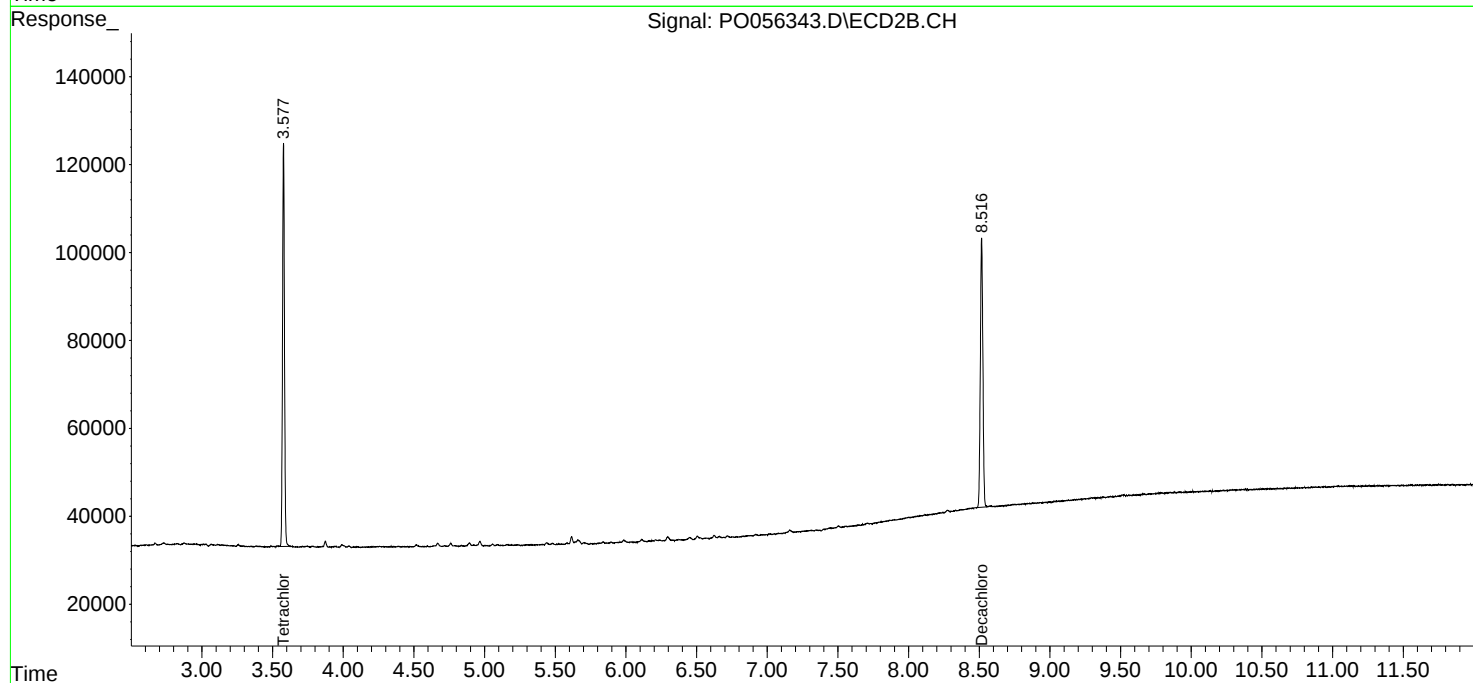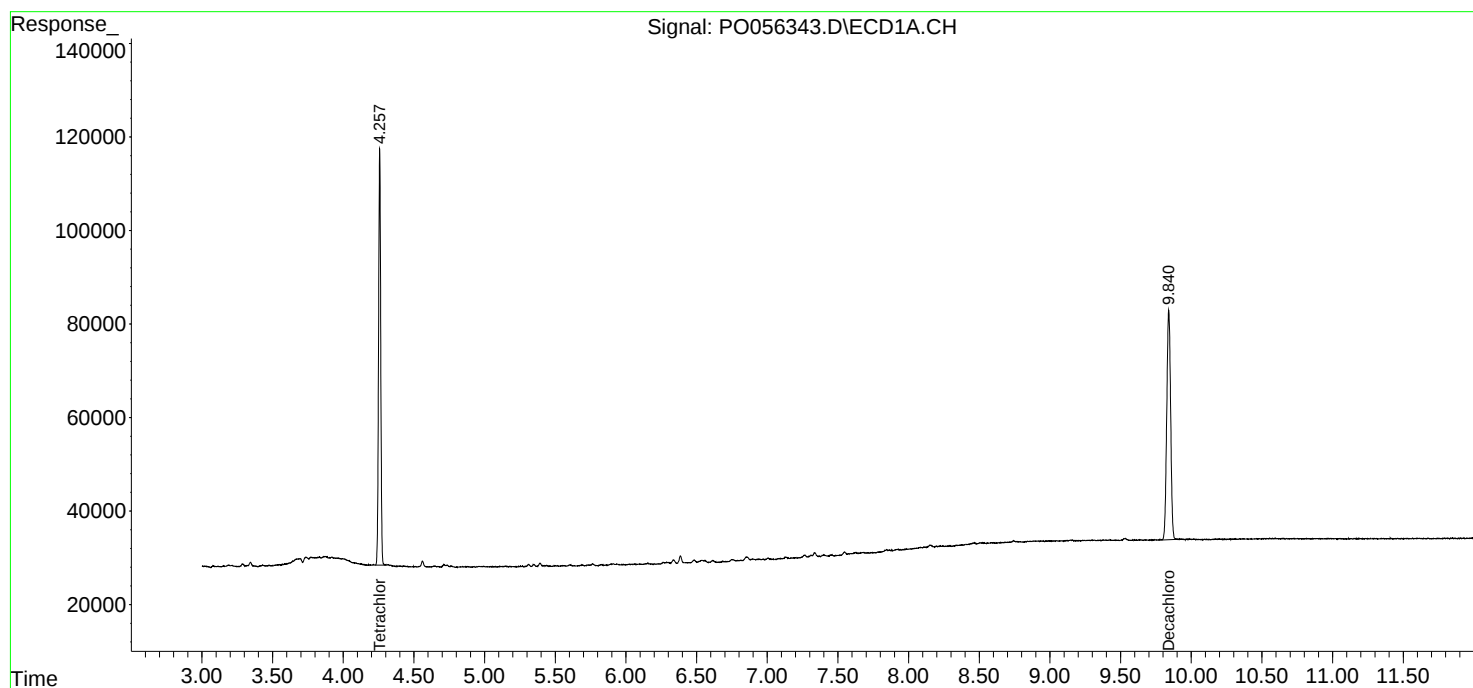


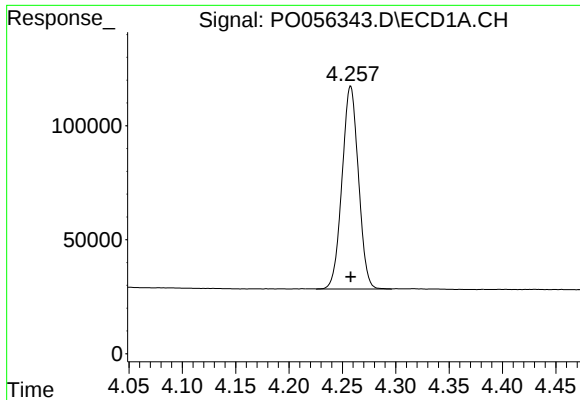

#1 Tetrachloro-m-xylene


R.T.: 4.258 min
Delta R.T.: 0.000 min
Response: 949043
Conc: 20.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-MANHOLE

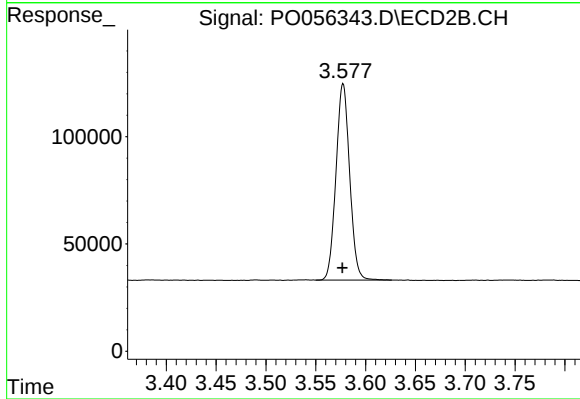


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: 0.000 min
Response: 875761
Conc: 20.84 ng/ml

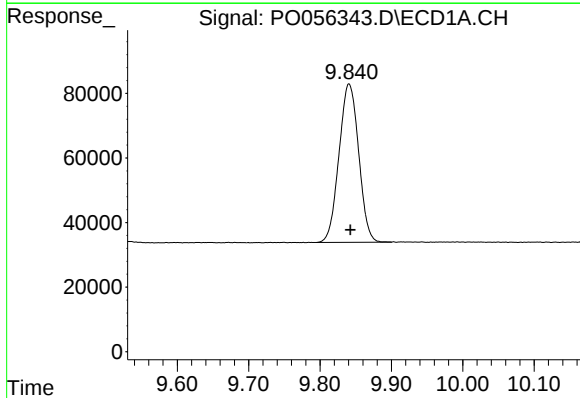

#2 Decachlorobiphenyl

R.T.: 9.841 min
Delta R.T.: -0.002 min
Response: 938244
Conc: 19.54 ng/ml

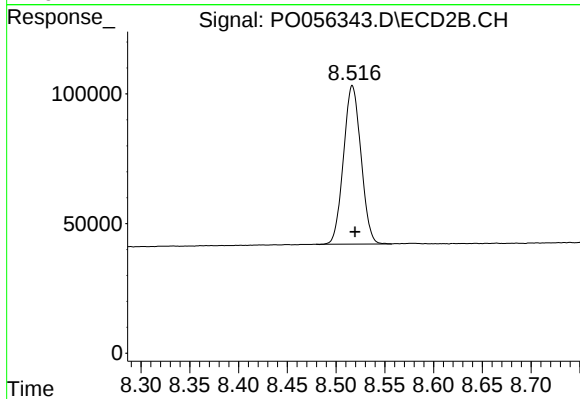

#2 Decachlorobiphenyl

R.T.: 8.517 min
Delta R.T.: -0.003 min
Response: 762840
Conc: 18.78 ng/ml